

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX033021\
 Data File : VX021661.D
 Acq On : 31 Mar 2021 04:11
 Operator : JC/MD
 Sample : M1842-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 RE104D1-20210323

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M

Title : SW846 8260

Signal : TIC: VX021661.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.581	247	254	261	rBV	3306	7145	1.87%	0.303%
2	5.464	733	744	757	rBV2	47489	136456	35.69%	5.782%
3	5.629	760	772	789	rBV	66958	187432	49.02%	7.942%
4	6.029	827	840	856	rBV	51491	136836	35.79%	5.798%
5	6.829	964	976	991	rBV	116849	276039	72.19%	11.697%
6	7.188	1027	1037	1052	rBV	110207	235079	61.48%	9.962%
7	8.694	1286	1293	1307	rBV	244471	382367	100.00%	16.203%
8	9.318	1394	1399	1404	rBV	11763	17337	4.53%	0.735%
9	10.094	1525	1531	1547	rVB	265211	366815	95.93%	15.544%
10	11.118	1700	1705	1715	rVB	215388	280807	73.44%	11.899%
11	12.059	1860	1865	1871	rBV	267409	333558	87.24%	14.135%




Sum of corrected areas: 2359871

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX033021\
Data File : VX021661.D
Acq On : 31 Mar 2021 04:11
Operator : JC/MD
Sample : M1842-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE104D1-20210323

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

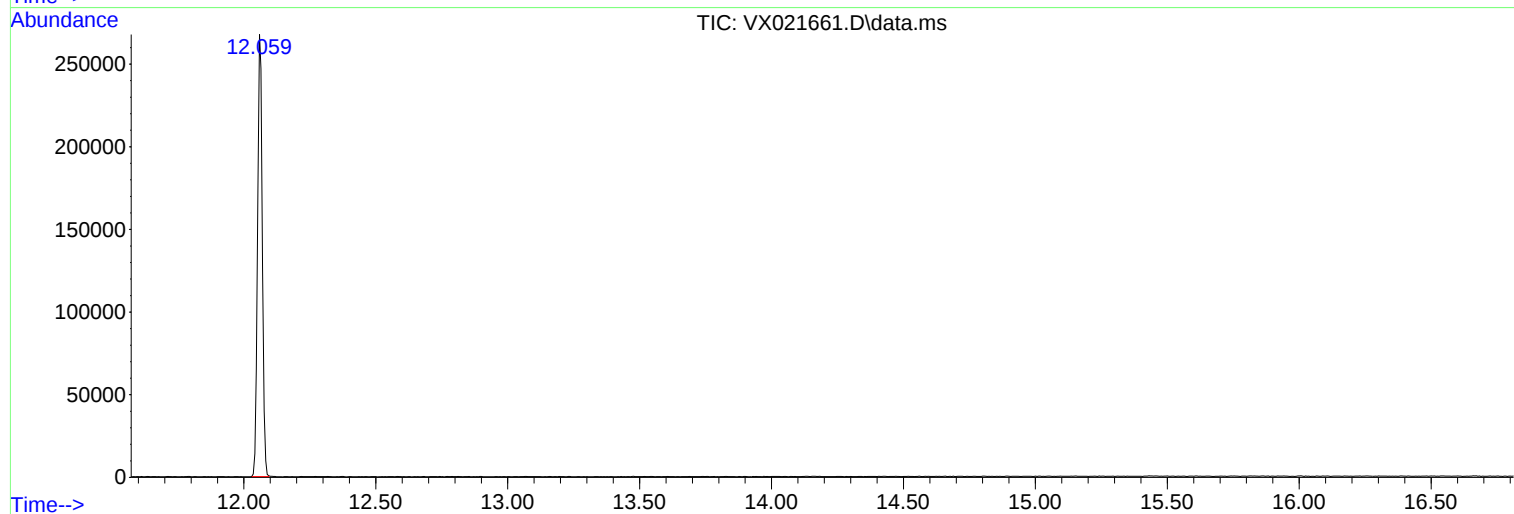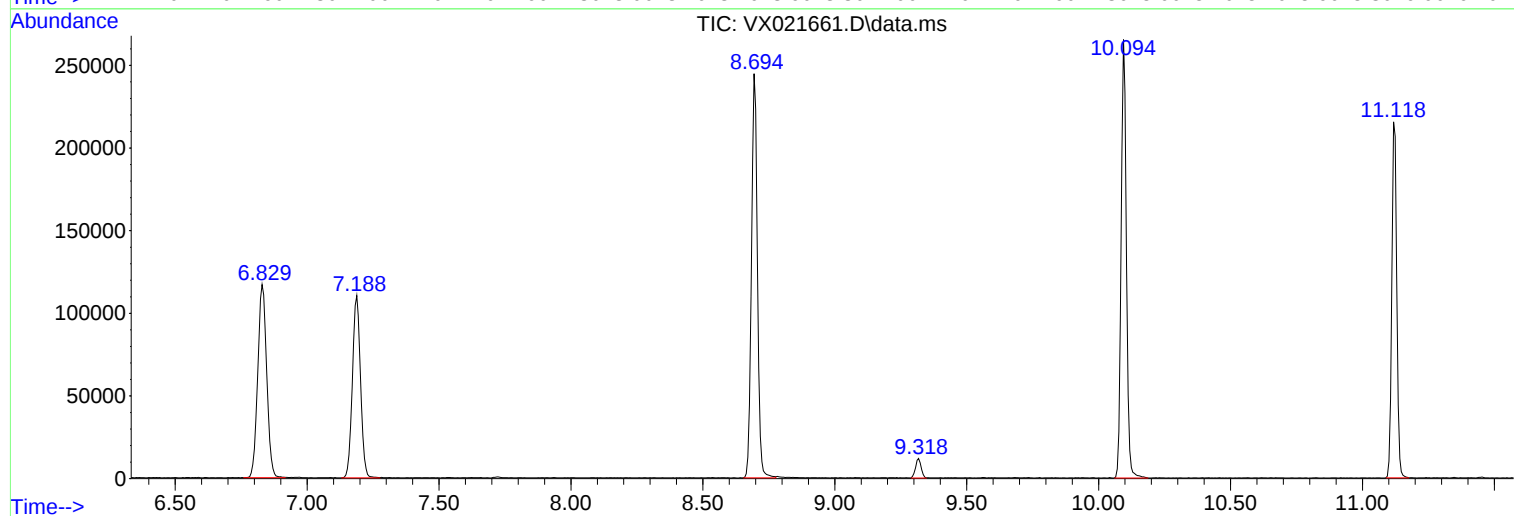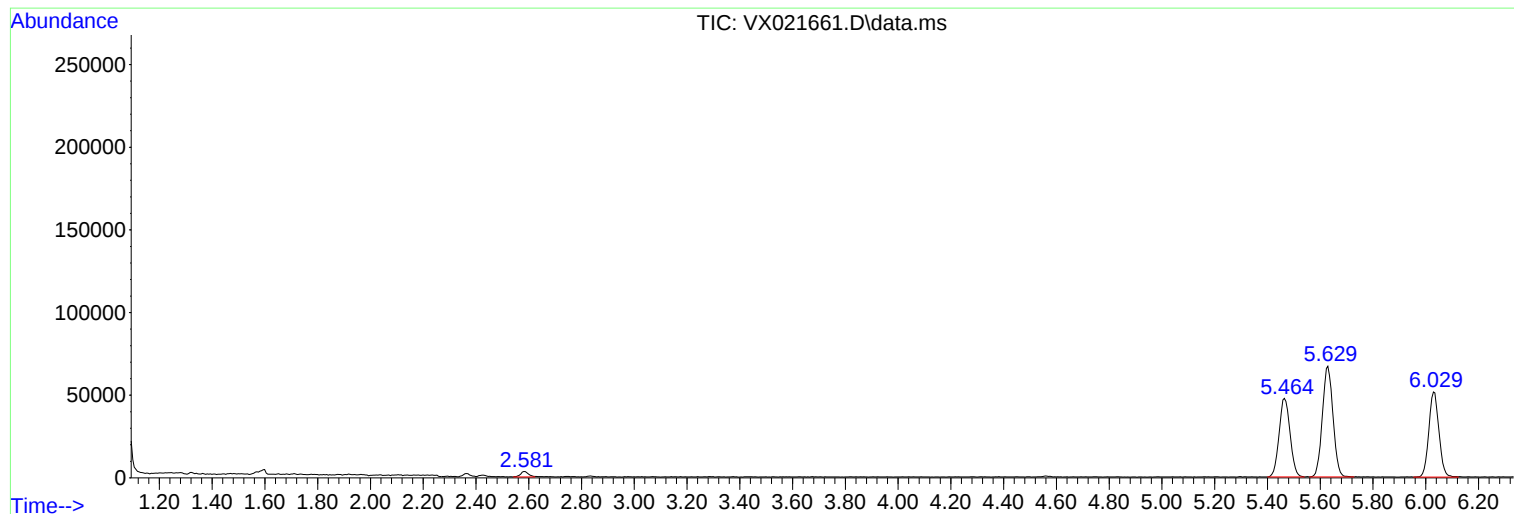

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX033021\
Data File : VX021661.D
Acq On : 31 Mar 2021 04:11
Operator : JC/MD
Sample : M1842-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE104D1-20210323

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX033021\
Data File : VX021661.D
Acq On : 31 Mar 2021 04:11
Operator : JC/MD
Sample : M1842-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE104D1-20210323

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
