

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX033021\
 Data File : VX021663.D
 Acq On : 31 Mar 2021 04:58
 Operator : JC/MD
 Sample : M1842-08
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 RE104D2-20210323

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M

Title : SW846 8260

Signal : TIC: VX021663.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.564	580	591	604	rBV	49230	134476	14.33%	4.352%
2	5.176	686	695	706	rVB2	3825	11478	1.22%	0.371%
3	5.464	732	744	760	rVB	47834	134199	14.30%	4.343%
4	5.629	760	772	785	rBV	67417	187836	20.02%	6.080%
5	6.029	829	840	856	rBV	50606	134048	14.28%	4.339%
6	6.829	965	976	987	rBV	112364	266571	28.41%	8.628%
7	7.188	1025	1037	1050	rBV	437993	938439	100.00%	30.374%
8	8.694	1284	1293	1310	rBV	241323	373666	39.82%	12.094%
9	10.094	1525	1531	1546	rBV	258612	351410	37.45%	11.374%
10	11.118	1700	1705	1721	rBV	202250	261721	27.89%	8.471%
11	12.059	1860	1865	1872	rBV	239129	295812	31.52%	9.574%




Sum of corrected areas: 3089656

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX033021\
Data File : VX021663.D
Acq On : 31 Mar 2021 04:58
Operator : JC/MD
Sample : M1842-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE104D2-20210323

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

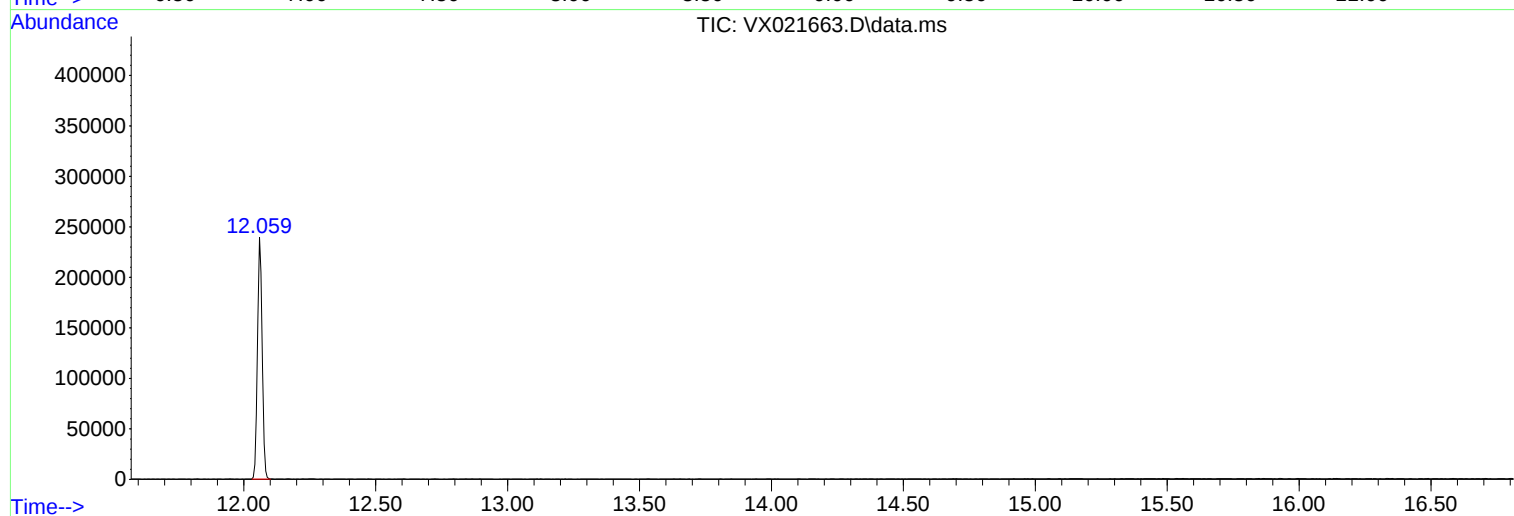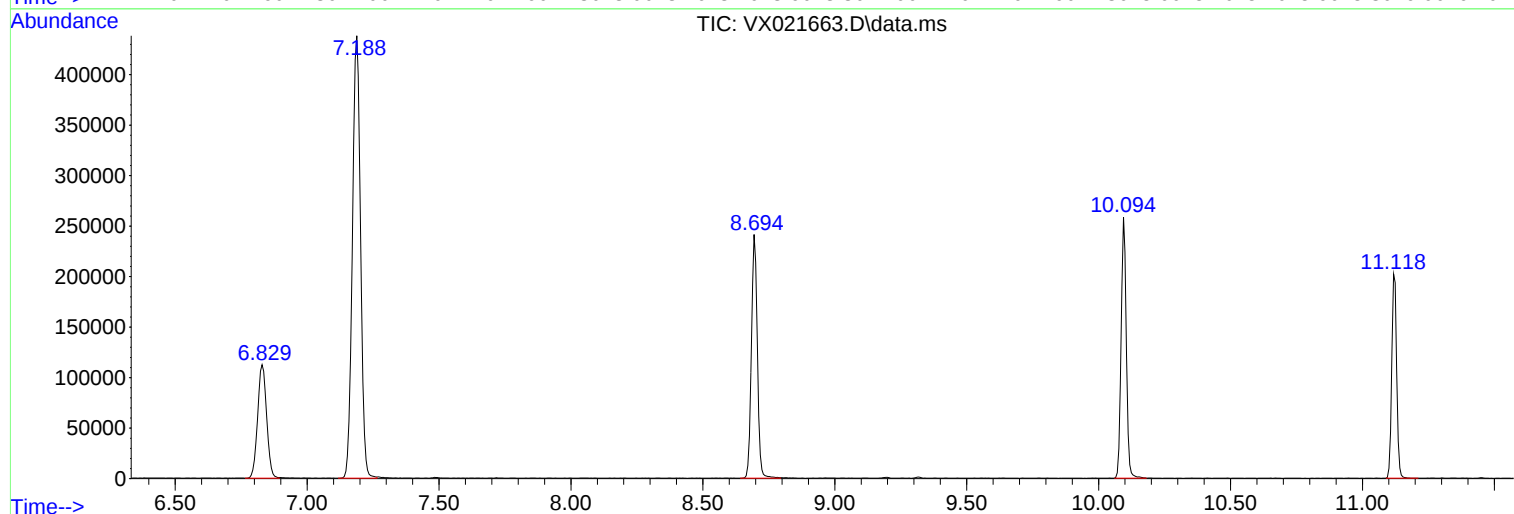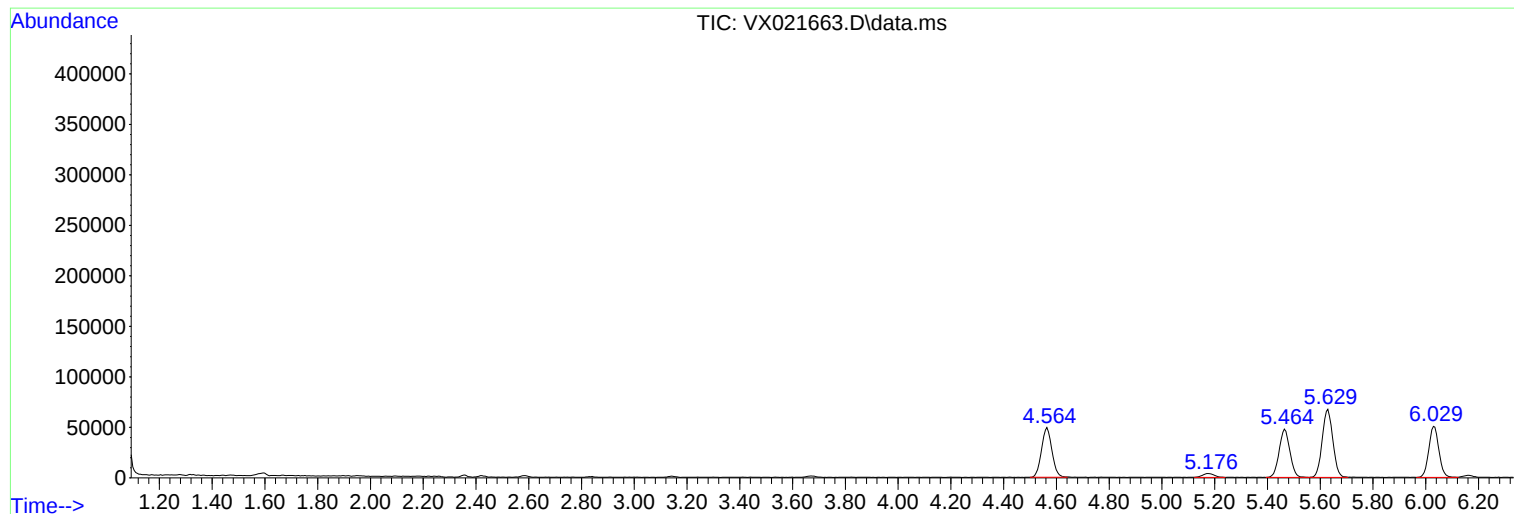

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX033021\
Data File : VX021663.D
Acq On : 31 Mar 2021 04:58
Operator : JC/MD
Sample : M1842-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE104D2-20210323

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX033021\
Data File : VX021663.D
Acq On : 31 Mar 2021 04:58
Operator : JC/MD
Sample : M1842-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE104D2-20210323

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
