
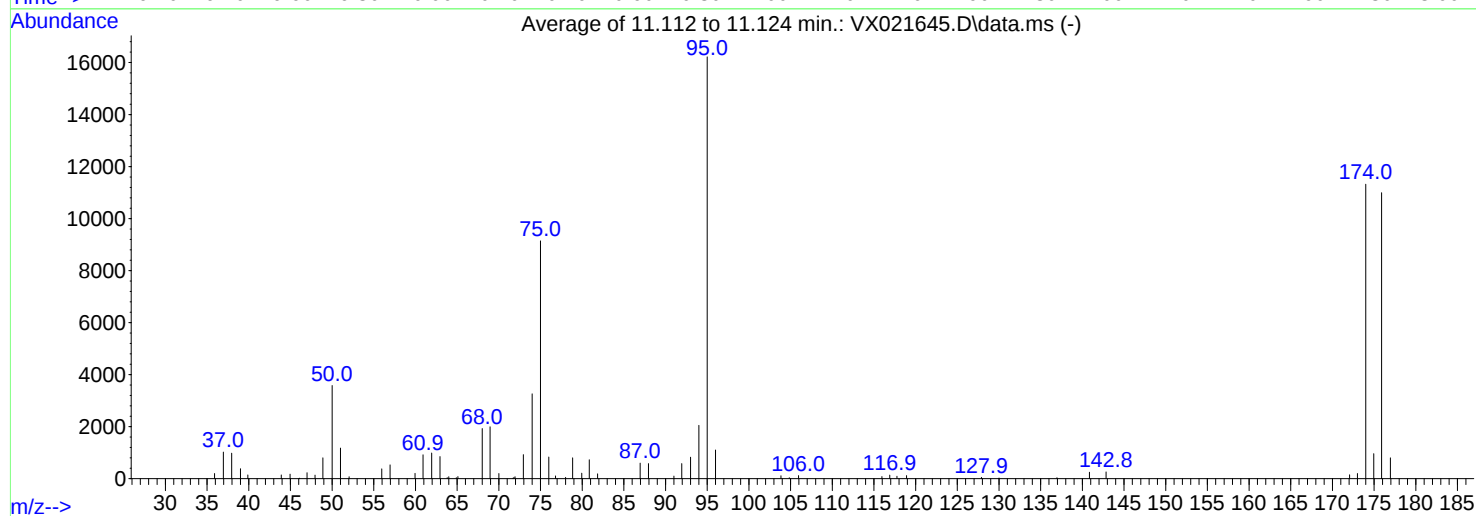


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX033021\
 Data File : VX021645.D
 Acq On : 30 Mar 2021 21:33
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X032621W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Sat Mar 27 04:47:38 2021

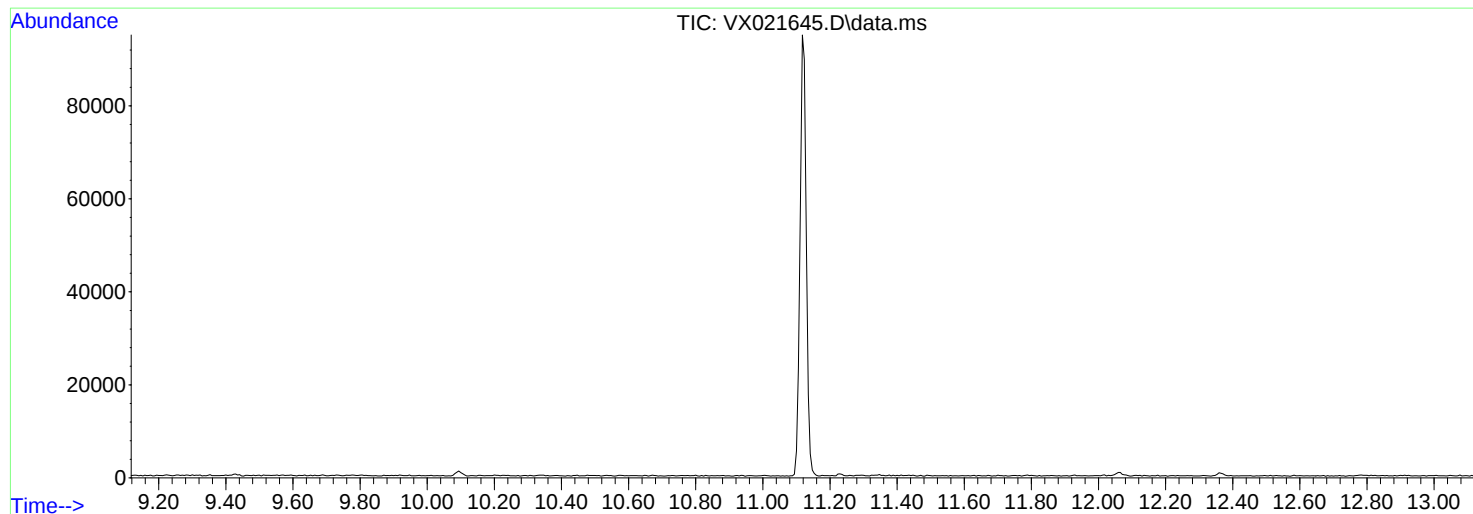

AutoFind: Scans 1704, 1705, 1706; Background Corrected with Scan 1699

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.1	3581	PASS
75	95	30	60	56.4	9143	PASS
95	95	100	100	100.0	16219	PASS
96	95	5	9	6.8	1101	PASS
173	174	0.00	2	1.7	195	PASS
174	95	50	100	69.8	11318	PASS
175	174	5	9	8.5	960	PASS
176	174	95	101	97.2	10996	PASS
177	176	5	9	7.2	797	PASS