

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX033022\  
 Data File : VX027799.D  
 Acq On : 30 Mar 2022 10:36  
 Operator : JC/MD  
 Sample : VX0330WBL01  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 3 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 VX0330WBL01

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X032922W.M

Title : SW846 8260

Signal : TIC: VX027799.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 1.246       | 22            | 26          | 38           | rBV3     | 2488           | 6595          | 1.47%           | 0.280%        |
| 2         | 5.385       | 694           | 705         | 722          | rBV      | 50286          | 144753        | 32.31%          | 6.157%        |
| 3         | 5.556       | 722           | 733         | 747          | rBV2     | 93228          | 267625        | 59.73%          | 11.383%       |
| 4         | 5.958       | 789           | 799         | 817          | rBV      | 53154          | 139925        | 31.23%          | 5.951%        |
| 5         | 6.763       | 920           | 931         | 944          | rBV      | 142541         | 334495        | 74.65%          | 14.227%       |
| 6         | 8.653       | 1234          | 1241        | 1255         | rBV      | 282051         | 448064        | 100.00%         | 19.057%       |
| 7         | 10.055      | 1465          | 1471        | 1481         | rBV      | 284327         | 388790        | 86.77%          | 16.536%       |
| 8         | 11.079      | 1634          | 1639        | 1652         | rBV      | 219862         | 288955        | 64.49%          | 12.290%       |
| 9         | 12.024      | 1788          | 1794        | 1807         | rVB      | 270467         | 331959        | 74.09%          | 14.119%       |




Sum of corrected areas: 2351161

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX033022\  
Data File : VX027799.D  
Acq On : 30 Mar 2022 10:36  
Operator : JC/MD  
Sample : VX0330WBL01  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
VX0330WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X032922W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

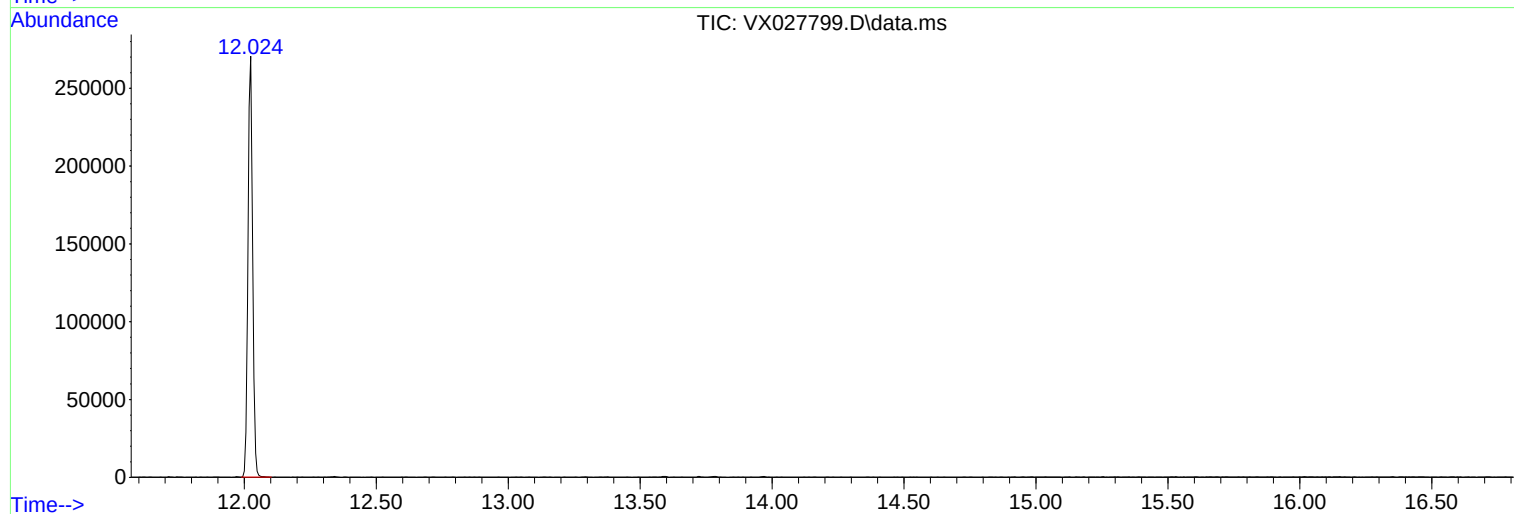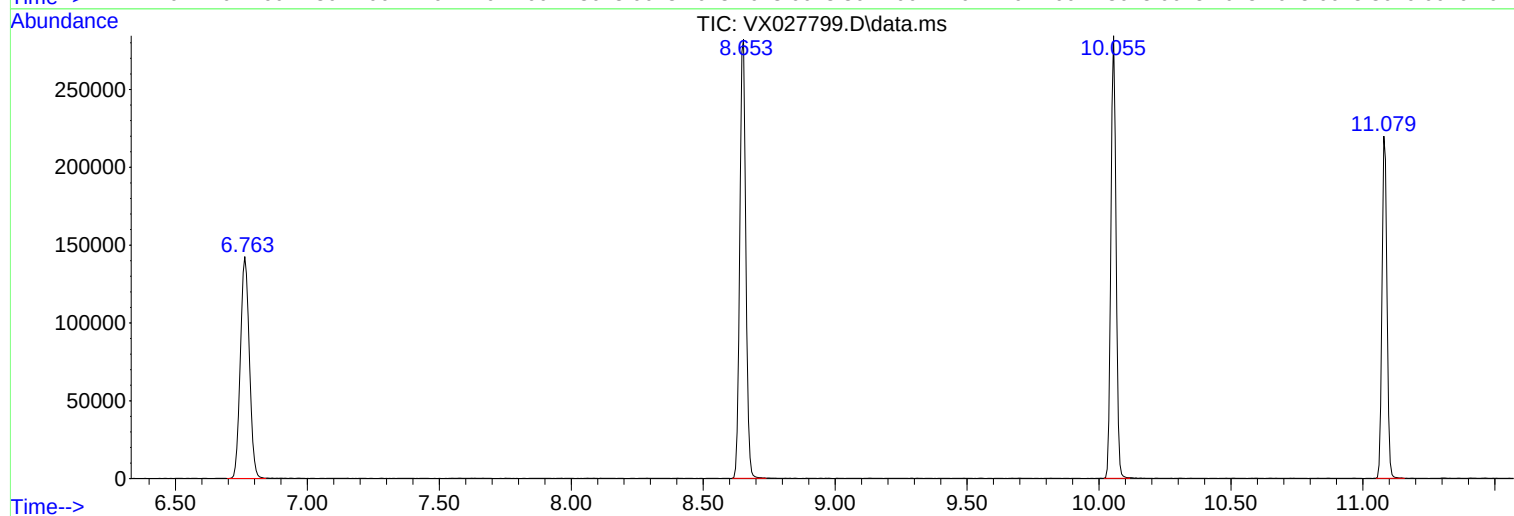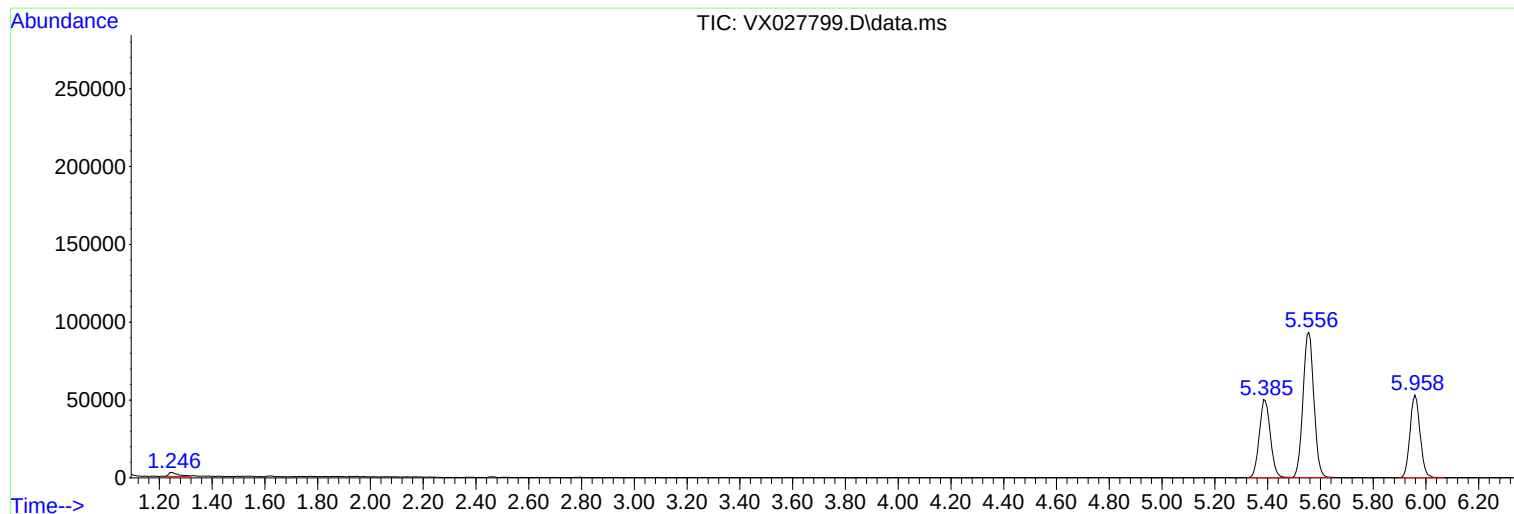

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX033022\  
Data File : VX027799.D  
Acq On : 30 Mar 2022 10:36  
Operator : JC/MD  
Sample : VX0330WBL01  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
VX0330WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X032922W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX033022\  
Data File : VX027799.D  
Acq On : 30 Mar 2022 10:36  
Operator : JC/MD  
Sample : VX0330WBL01  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
VX0330WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X032922W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | --Internal Standard-- |    |      |      |
|------------------|----|---------|-------|----------|-----------------------|----|------|------|
|                  |    |         |       |          | #                     | RT | Resp | Conc |

-----