

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX033022\
Data File : VX027813.D
Acq On : 30 Mar 2022 16:14
Operator : JC/MD
Sample : N2074-19 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TT101D2-20220321

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032922W.M

Title : SW846 8260

Signal : TIC: VX027813.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	21	26	44	rBV2	4217	10958	1.64%	0.354%
2	2.325	198	203	210	rBV3	5926	11663	1.75%	0.377%
3	5.391	693	706	720	rBV2	54593	157542	23.59%	5.093%
4	5.556	722	733	749	rVB	89719	250795	37.55%	8.108%
5	5.958	789	799	815	rBV	58042	152685	22.86%	4.936%
6	6.763	920	931	942	rBV	142620	337330	50.51%	10.905%
7	7.129	982	991	1005	rBV	313620	667895	100.00%	21.592%
8	8.653	1234	1241	1253	rBV	283153	442754	66.29%	14.313%
9	10.055	1465	1471	1484	rBV	307262	399180	59.77%	12.905%
10	11.085	1634	1640	1654	rVB	231054	305794	45.78%	9.886%
11	12.024	1789	1794	1801	rBV	297901	356678	53.40%	11.531%




Sum of corrected areas: 3093274

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX033022\
Data File : VX027813.D
Acq On : 30 Mar 2022 16:14
Operator : JC/MD
Sample : N2074-19 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TT101D2-20220321

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032922W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

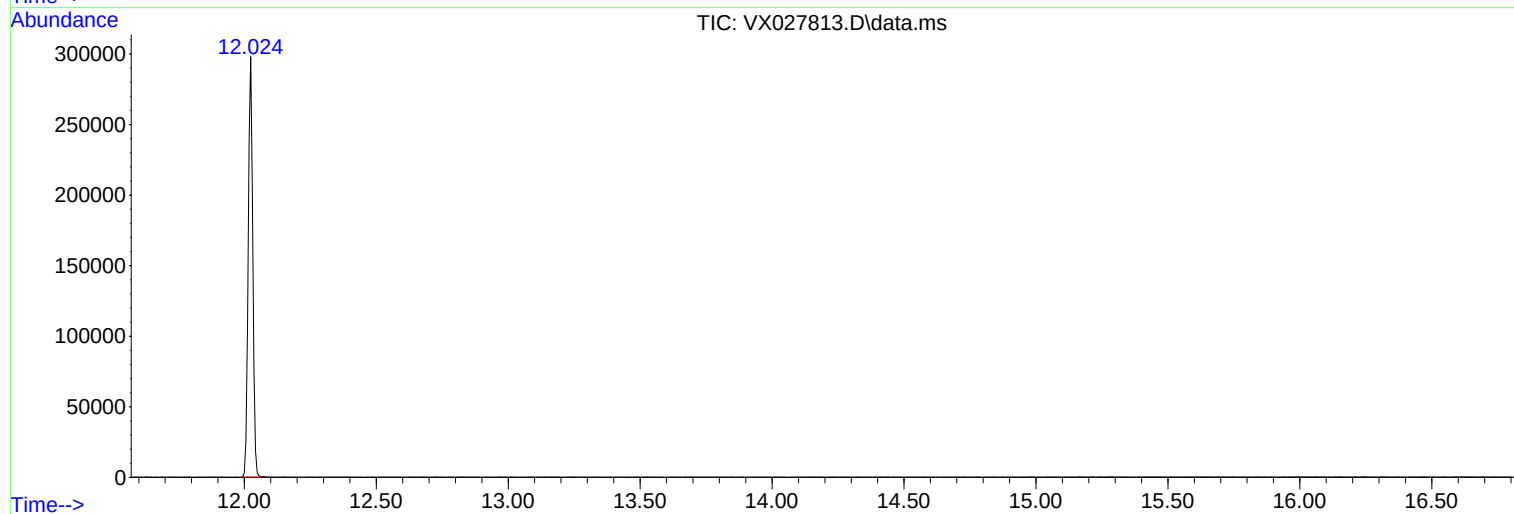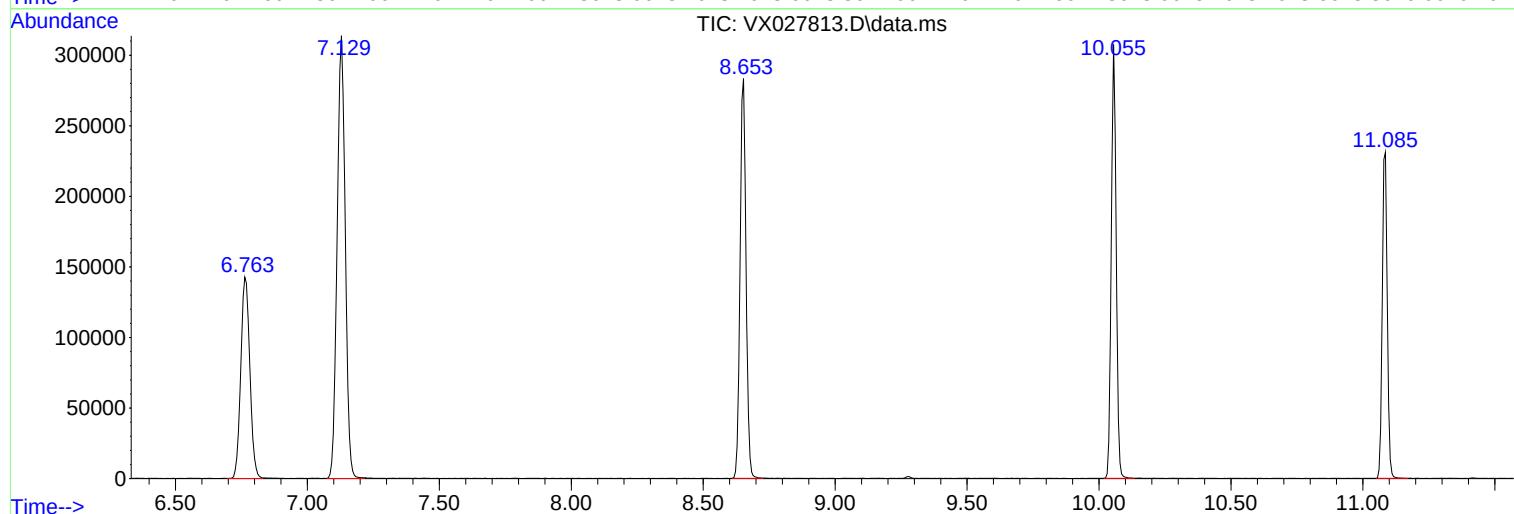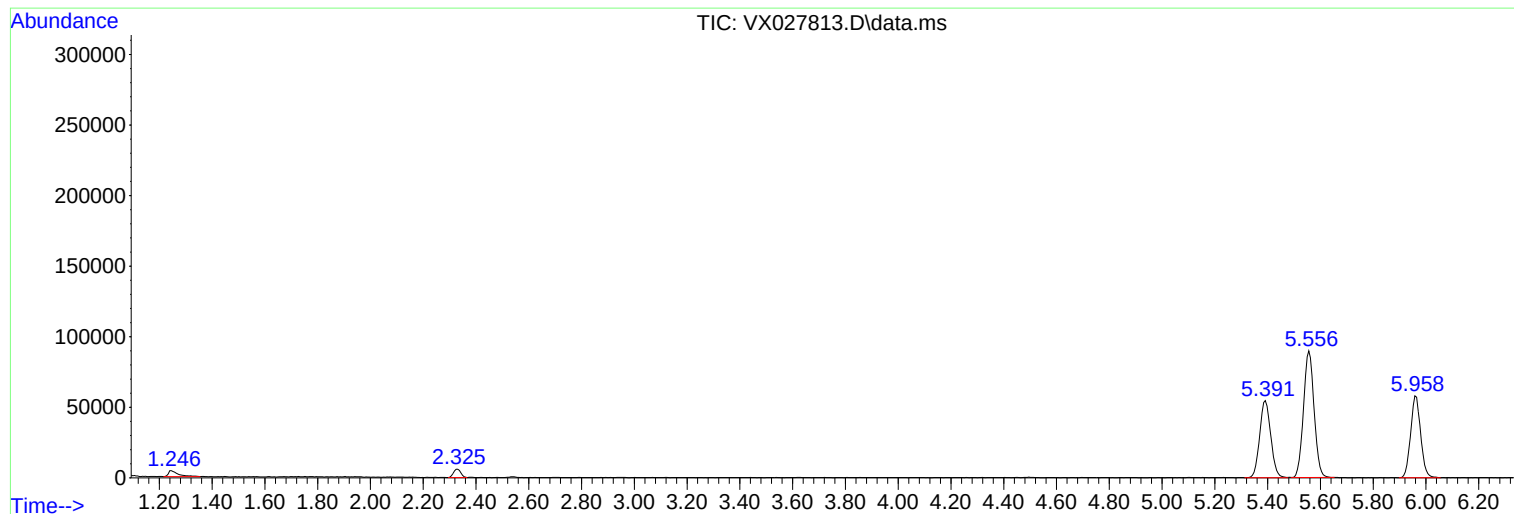

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX033022\
Data File : VX027813.D
Acq On : 30 Mar 2022 16:14
Operator : JC/MD
Sample : N2074-19 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TT101D2-20220321

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032922W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX033022\
Data File : VX027813.D
Acq On : 30 Mar 2022 16:14
Operator : JC/MD
Sample : N2074-19 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TT101D2-20220321

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032922W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------