

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX033022\
Data File : VX027816.D
Acq On : 30 Mar 2022 17:24
Operator : JC/MD
Sample : N2074-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TT180D1-20220318

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032922W.M

Title : SW846 8260

Signal : TIC: VX027816.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.245	19	26	32	rBV	4410	9603	1.93%	0.334%
2	2.324	197	203	209	rBV2	3842	6911	1.39%	0.240%
3	5.391	695	706	723	rBV2	52756	154053	30.90%	5.355%
4	5.555	723	733	752	rVB	88347	249411	50.03%	8.670%
5	5.964	789	800	812	rBV	56033	149751	30.04%	5.206%
6	6.763	921	931	945	rBV	138485	333144	66.83%	11.581%
7	7.128	982	991	1004	rBV	233861	498493	100.00%	17.329%
8	8.652	1234	1241	1255	rVB	280864	437780	87.82%	15.218%
9	10.055	1465	1471	1484	rBV	291246	391970	78.63%	13.626%
10	11.085	1634	1640	1652	rVB	224971	296989	59.58%	10.324%
11	12.024	1789	1794	1802	rBV	280838	348563	69.92%	12.117%




Sum of corrected areas: 2876668

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX033022\
Data File : VX027816.D
Acq On : 30 Mar 2022 17:24
Operator : JC/MD
Sample : N2074-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TT180D1-20220318

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032922W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

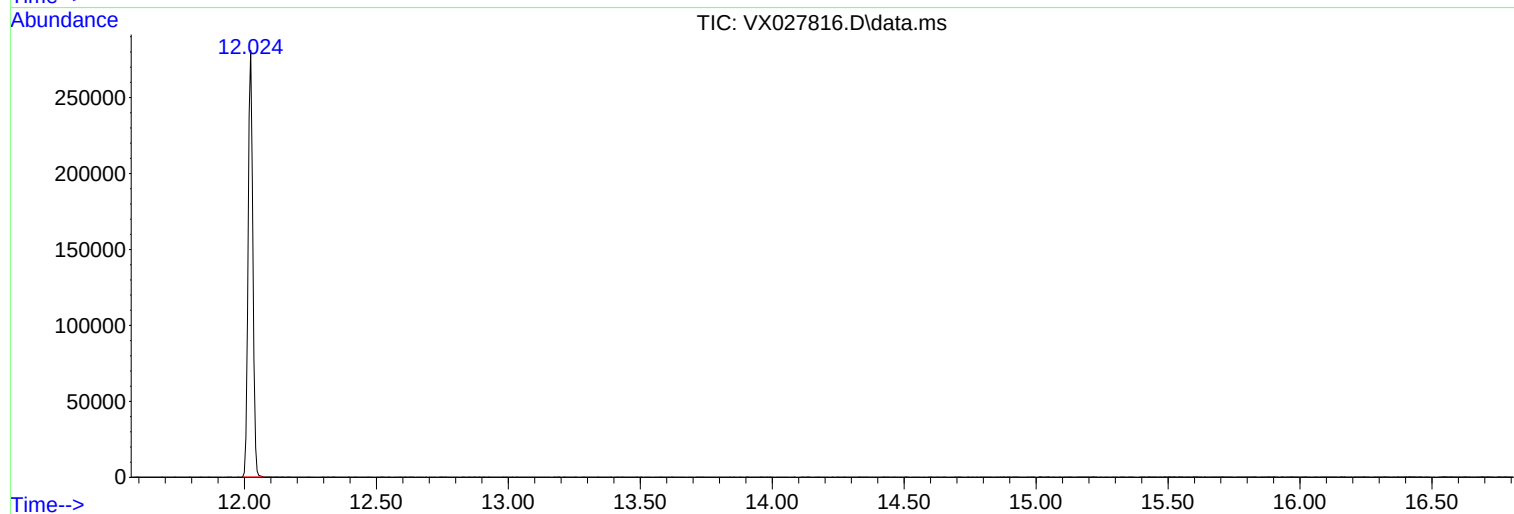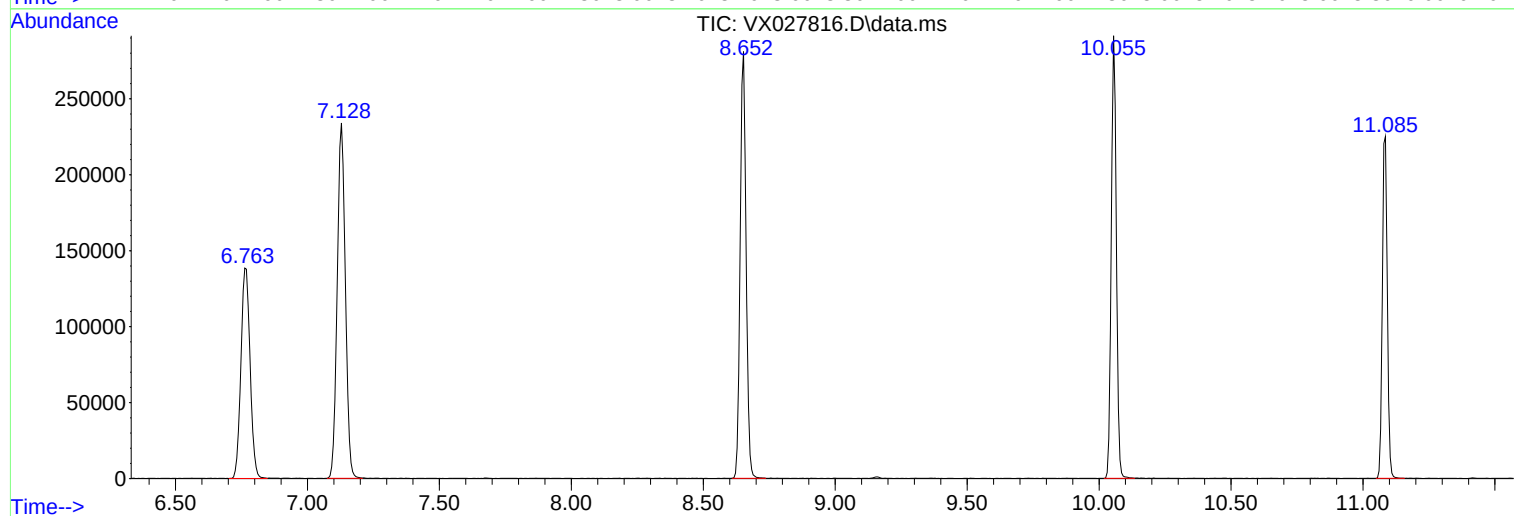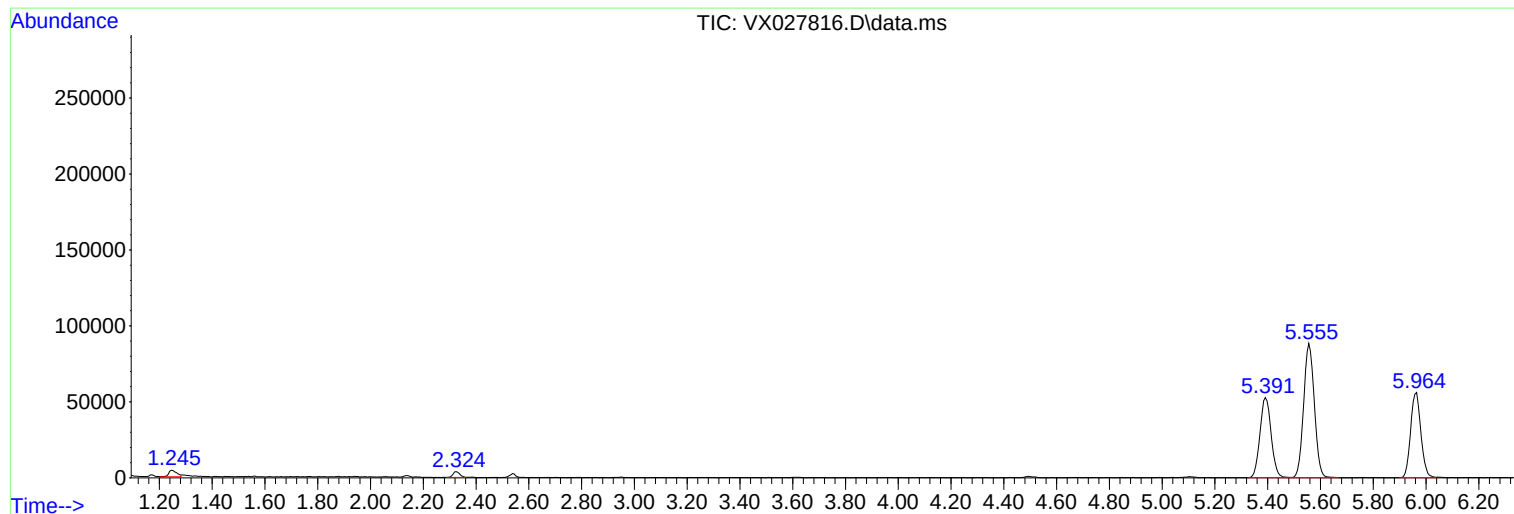

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX033022\
Data File : VX027816.D
Acq On : 30 Mar 2022 17:24
Operator : JC/MD
Sample : N2074-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TT180D1-20220318

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032922W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX033022\
Data File : VX027816.D
Acq On : 30 Mar 2022 17:24
Operator : JC/MD
Sample : N2074-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TT180D1-20220318

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032922W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------