

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX033023\  
Data File : VX034848.D  
Acq On : 30 Mar 2023 13:33  
Operator : JC/MD  
Sample : IBLK  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 10 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
IBLK

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X032923W.M

Title : SW846 8260

Signal : TIC: VX034848.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.385       | 693           | 705         | 718          | rBV      | 167795         | 485819        | 31.87%          | 6.092%        |
| 2         | 5.550       | 720           | 732         | 749          | rVB      | 294696         | 835317        | 54.80%          | 10.475%       |
| 3         | 5.952       | 786           | 798         | 813          | rBV      | 195672         | 532702        | 34.95%          | 6.680%        |
| 4         | 6.763       | 919           | 931         | 949          | rBV      | 464966         | 1122333       | 73.63%          | 14.074%       |
| 5         | 8.647       | 1234          | 1240        | 1250         | rBV      | 973756         | 1524231       | 100.00%         | 19.114%       |
| 6         | 10.055      | 1465          | 1471        | 1489         | rBV      | 960566         | 1309206       | 85.89%          | 16.418%       |
| 7         | 11.079      | 1634          | 1639        | 1653         | rBV      | 777046         | 987896        | 64.81%          | 12.388%       |
| 8         | 12.024      | 1788          | 1794        | 1802         | rBV      | 902872         | 1176884       | 77.21%          | 14.758%       |




Sum of corrected areas: 7974388

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX033023\  
Data File : VX034848.D  
Acq On : 30 Mar 2023 13:33  
Operator : JC/MD  
Sample : IBLK  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 10 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
IBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X032923W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

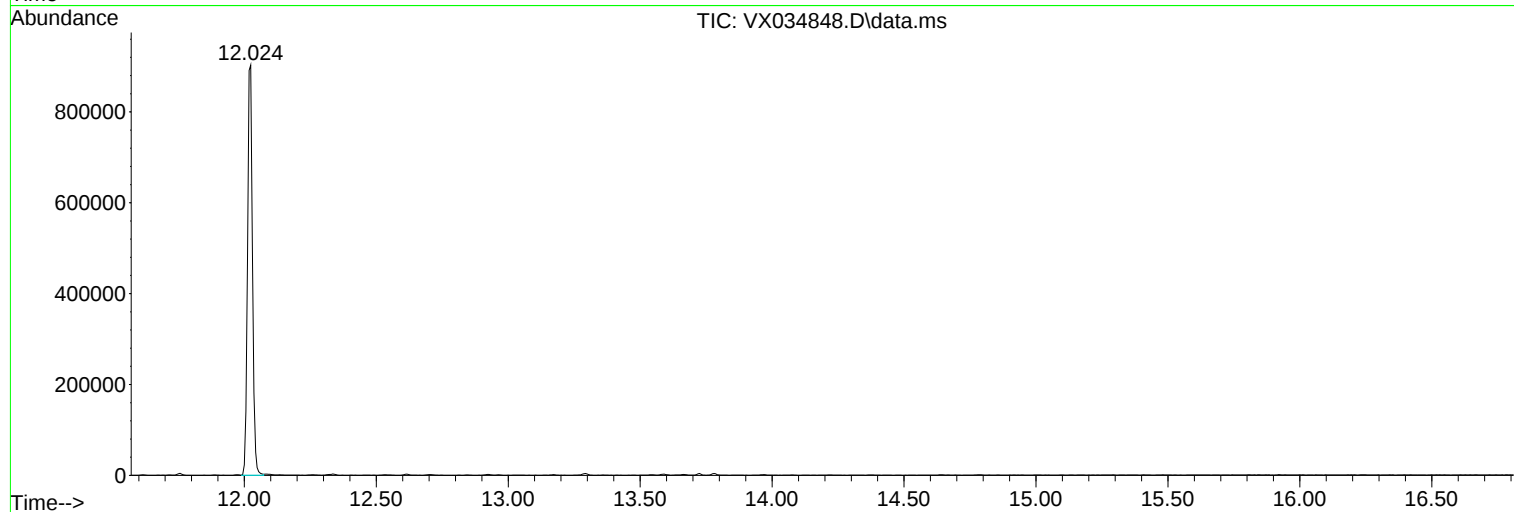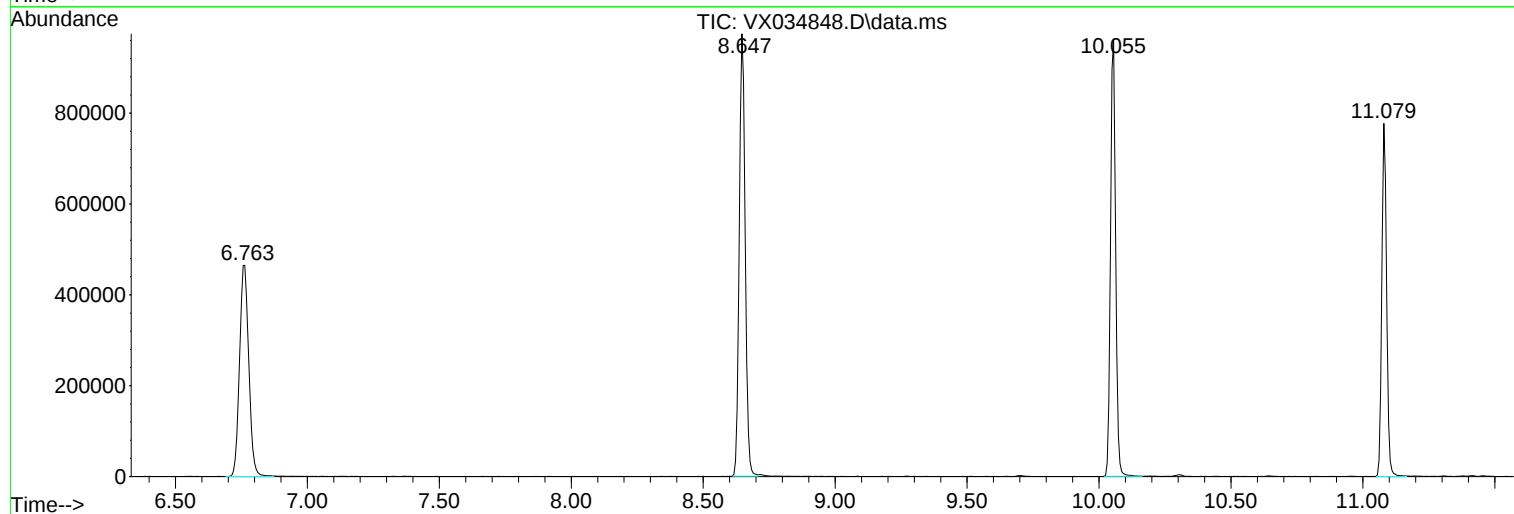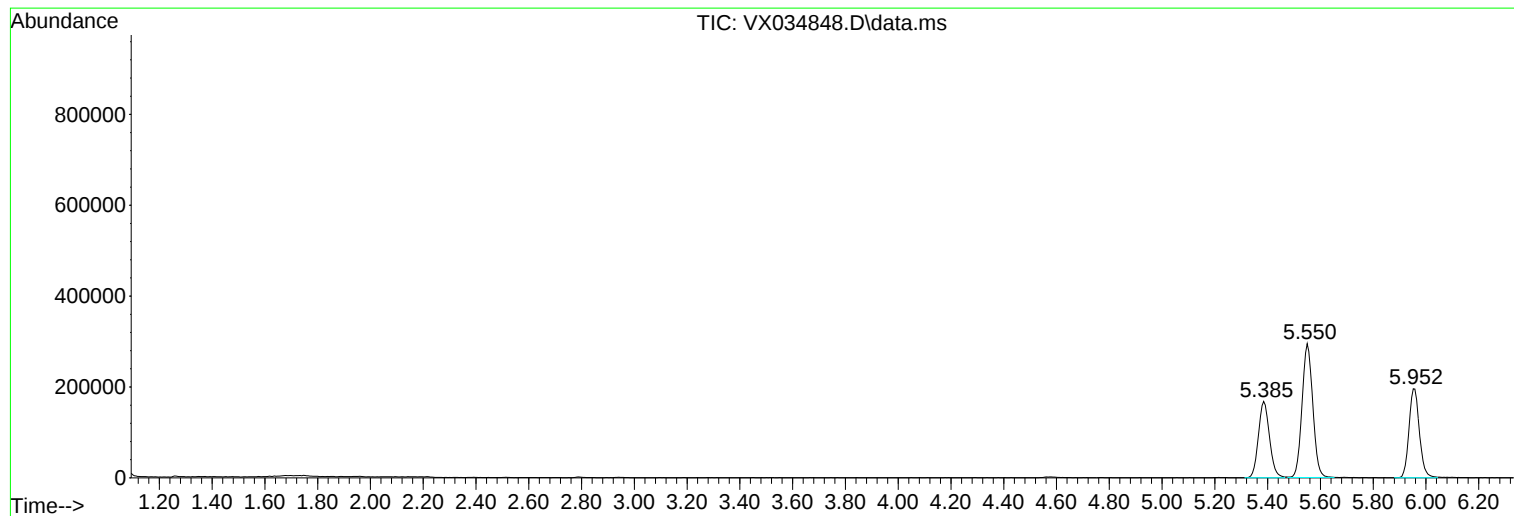

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX033023\  
Data File : VX034848.D  
Acq On : 30 Mar 2023 13:33  
Operator : JC/MD  
Sample : IBLK  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 10 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
IBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X032923W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX033023\  
Data File : VX034848.D  
Acq On : 30 Mar 2023 13:33  
Operator : JC/MD  
Sample : IBLK  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 10 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
IBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X032923W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|