

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX033023\
 Data File : VX034851.D
 Acq On : 30 Mar 2023 14:42
 Operator : JC/MD
 Sample : 02091-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 OF-3

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032923W.M
 Title : SW846 8260

Signal : TIC: VX034851.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.453	56	60	65	rBV	37214	43189	3.16%	0.558%
2	2.294	193	198	205	rVB	9305	14410	1.05%	0.186%
3	2.386	207	213	222	rBV	70804	125888	9.20%	1.626%
4	2.581	235	245	250	rBV2	4783	15823	1.16%	0.204%
5	4.007	471	479	491	rBV2	17403	44818	3.27%	0.579%
6	4.568	562	571	586	rBV	13065	41445	3.03%	0.535%
7	5.385	694	705	720	rBV2	151338	442189	32.31%	5.710%
8	5.550	721	732	748	rVB	259683	751844	54.93%	9.709%
9	5.952	788	798	814	rBV	192541	492273	35.97%	6.357%
10	6.763	921	931	948	rBV	418576	1006858	73.56%	13.002%
11	7.293	1008	1018	1027	rBV7	6458	19202	1.40%	0.248%
12	7.470	1041	1047	1056	rBV	6581	15696	1.15%	0.203%
13	8.574	1222	1228	1234	rBV	61956	101492	7.42%	1.311%
14	8.647	1234	1240	1249	rVV	862757	1368681	100.00%	17.674%
15	9.525	1379	1384	1392	rBV2	15297	25057	1.83%	0.324%
16	10.055	1465	1471	1485	rBV	863449	1177462	86.03%	15.205%
17	10.774	1583	1589	1597	rBV	10387	17400	1.27%	0.225%
18	10.860	1599	1603	1613	rVB3	8680	14300	1.04%	0.185%
19	11.079	1631	1639	1649	rBV	701276	887538	64.85%	11.461%
20	12.018	1788	1793	1807	rBV	822622	1050103	76.72%	13.560%
21	12.585	1882	1886	1897	rBV3	15883	29141	2.13%	0.376%
22	13.140	1972	1977	1984	rBV	32597	43631	3.19%	0.563%
23	14.194	2144	2150	2157	rBV5	6617	15402	1.13%	0.199%




Sum of corrected areas: 7743842

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX033023\
Data File : VX034851.D
Acq On : 30 Mar 2023 14:42
Operator : JC/MD
Sample : 02091-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
OF-3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032923W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

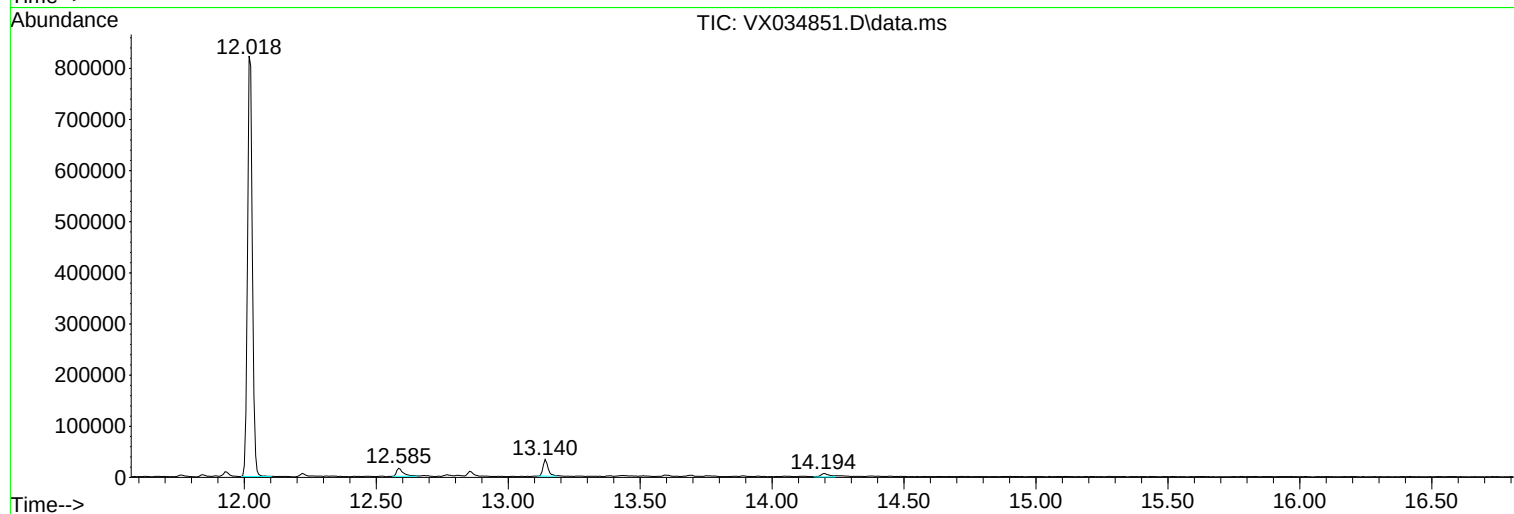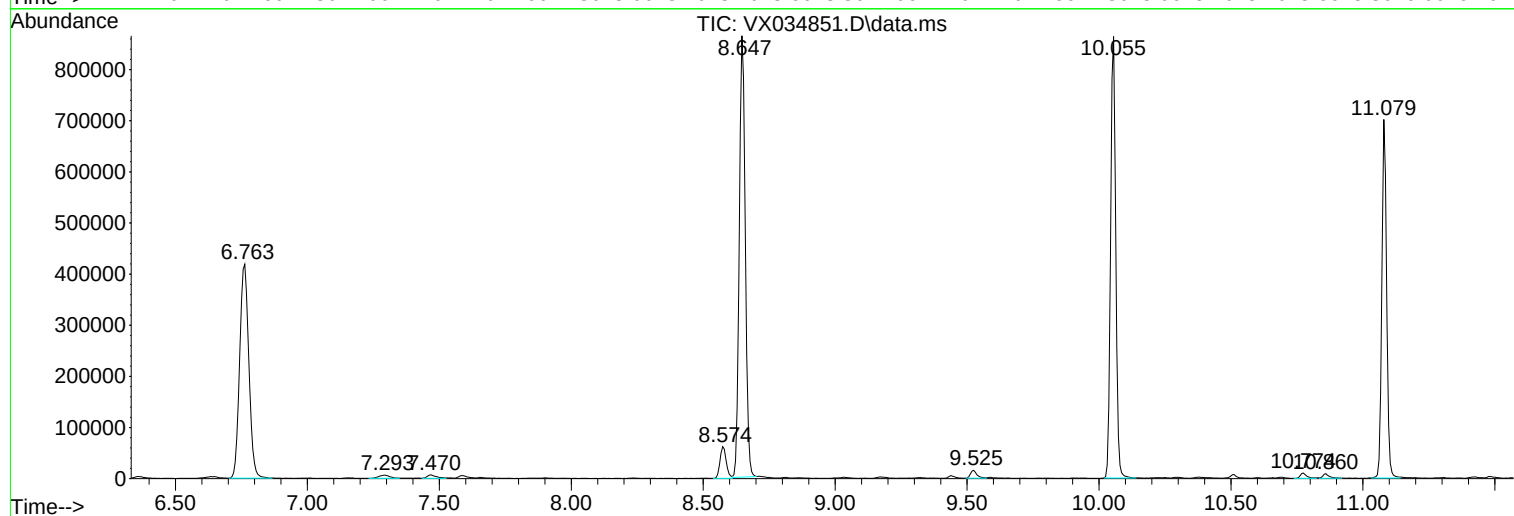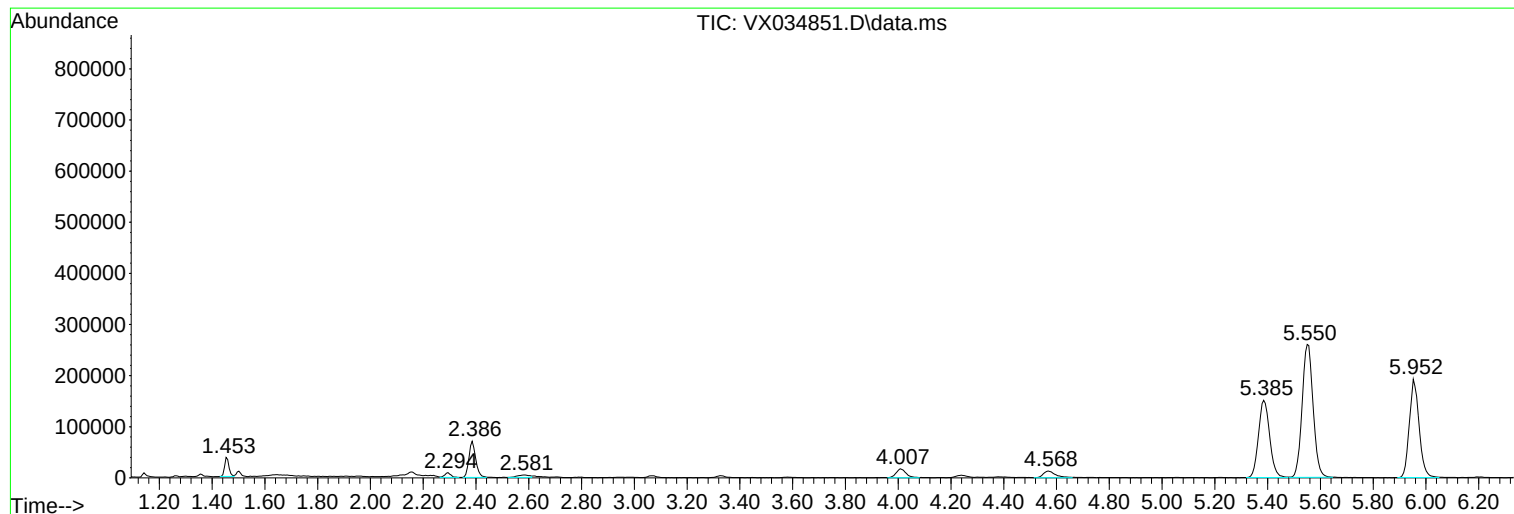

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX033023\
Data File : VX034851.D
Acq On : 30 Mar 2023 14:42
Operator : JC/MD
Sample : 02091-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
OF-3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032923W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX033023\
Data File : VX034851.D
Acq On : 30 Mar 2023 14:42
Operator : JC/MD
Sample : 02091-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
OF-3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032923W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------