

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX033023\
 Data File : VX034852.D
 Acq On : 30 Mar 2023 15:05
 Operator : JC/MD
 Sample : 02074-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TB-01-032323

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032923W.M
 Title : SW846 8260

Signal : TIC: VX034852.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.495	547	559	567	rBV	14142	39937	2.76%	0.511%
2	5.093	644	657	668	rBV3	8302	26487	1.83%	0.339%
3	5.385	692	705	721	rBV2	153983	455769	31.52%	5.828%
4	5.550	721	732	747	rVV	274001	776506	53.70%	9.930%
5	5.952	787	798	814	rBV	190668	502010	34.72%	6.420%
6	6.757	920	930	946	rBV	439422	1048314	72.50%	13.406%
7	7.129	985	991	1000	rVB3	7534	16295	1.13%	0.208%
8	8.647	1233	1240	1256	rBV	944280	1445976	100.00%	18.491%
9	9.275	1337	1343	1351	rBV	48639	73084	5.05%	0.935%
10	9.525	1379	1384	1395	rBV	28418	46752	3.23%	0.598%
11	10.055	1465	1471	1483	rBV	911593	1240366	85.78%	15.862%
12	11.079	1634	1639	1649	rBV	738417	941536	65.11%	12.040%
13	11.933	1774	1779	1785	rBV	12119	18006	1.25%	0.230%
14	12.024	1788	1794	1806	rVV	860239	1119865	77.45%	14.321%
15	12.853	1926	1930	1947	rVB2	15160	22815	1.58%	0.292%
16	13.140	1972	1977	1987	rBV	33194	46180	3.19%	0.591%




Sum of corrected areas: 7819898

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX033023\
Data File : VX034852.D
Acq On : 30 Mar 2023 15:05
Operator : JC/MD
Sample : 02074-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TB-01-032323

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032923W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

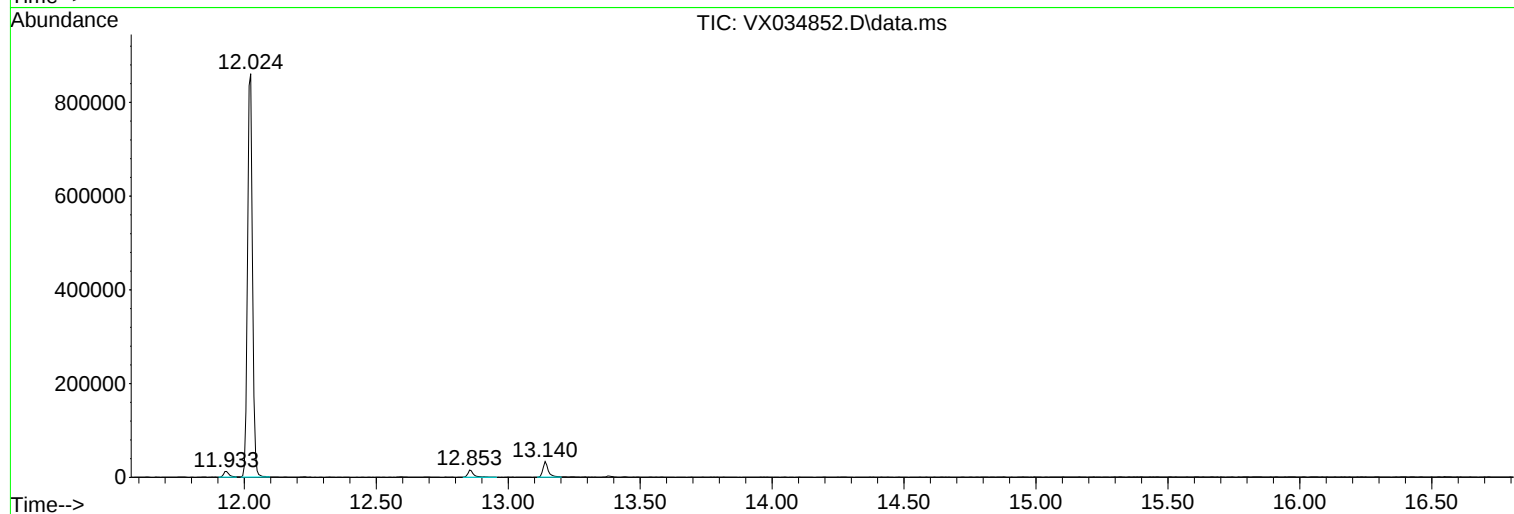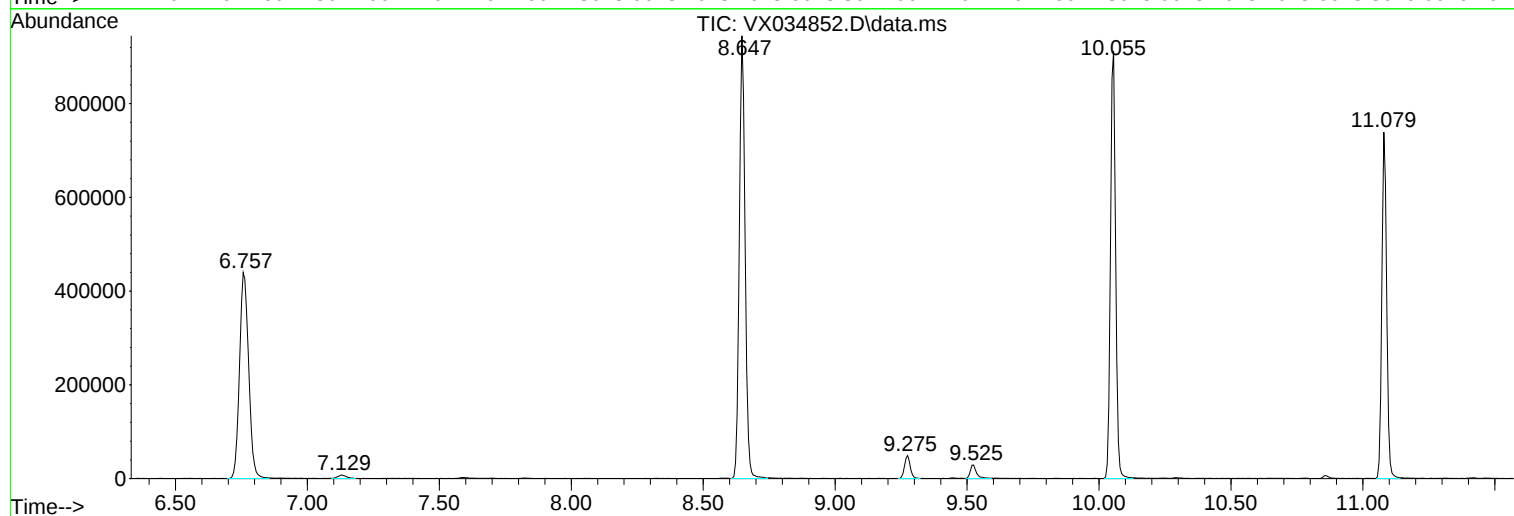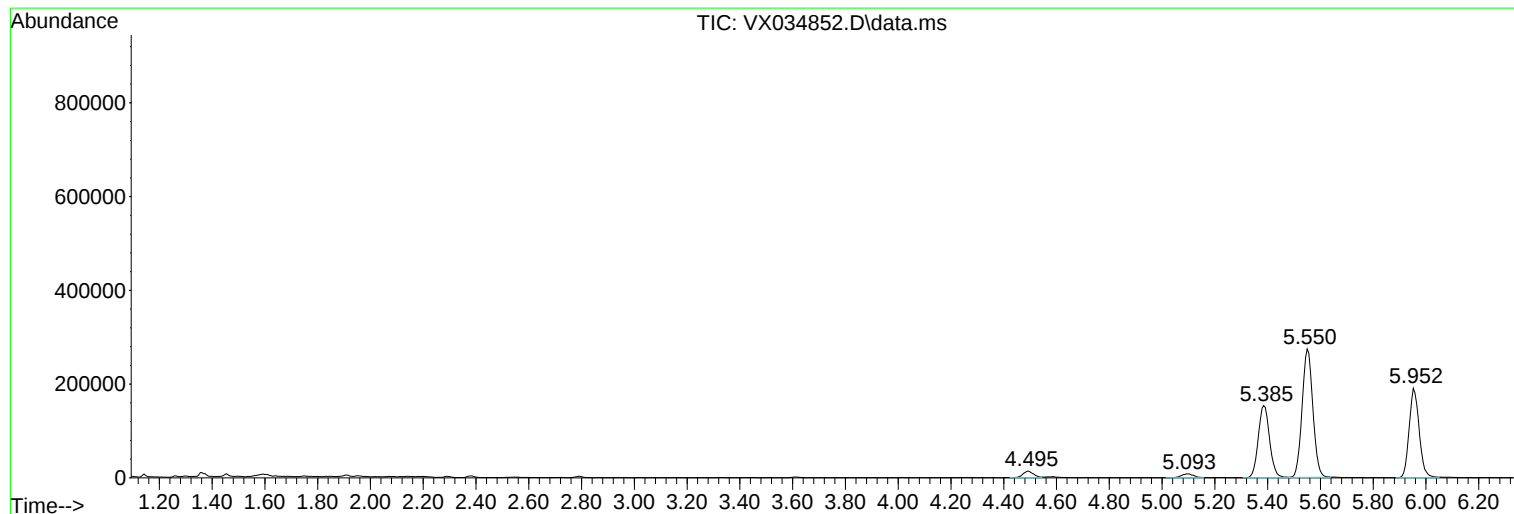

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX033023\
Data File : VX034852.D
Acq On : 30 Mar 2023 15:05
Operator : JC/MD
Sample : 02074-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TB-01-032323

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032923W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX033023\
Data File : VX034852.D
Acq On : 30 Mar 2023 15:05
Operator : JC/MD
Sample : 02074-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TB-01-032323

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032923W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------