

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX033023\
 Data File : VX034854.D
 Acq On : 30 Mar 2023 15:51
 Operator : JC/MD
 Sample : 02074-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EB-01-032323

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032923W.M

Title : SW846 8260

Signal : TIC: VX034854.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.386	207	213	224	rVB2	7611	14821	1.07%	0.204%
2	2.788	273	279	289	rBV	9445	18782	1.36%	0.258%
3	5.385	694	705	719	rBV2	152107	443512	32.02%	6.095%
4	5.550	722	732	748	rVB2	264881	748810	54.06%	10.291%
5	5.952	787	798	813	rBV	181317	486315	35.11%	6.683%
6	6.757	919	930	952	rBV	420562	1017033	73.42%	13.977%
7	8.647	1233	1240	1251	rBV	902942	1385148	100.00%	19.036%
8	10.055	1465	1471	1485	rBV	876160	1195756	86.33%	16.433%
9	11.079	1634	1639	1653	rBV	705625	898516	64.87%	12.348%
10	12.024	1788	1794	1806	rBV	794443	1051304	75.90%	14.448%
11	13.140	1971	1977	1988	rVB2	10595	16558	1.20%	0.228%




Sum of corrected areas: 7276555

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX033023\
Data File : VX034854.D
Acq On : 30 Mar 2023 15:51
Operator : JC/MD
Sample : 02074-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EB-01-032323

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032923W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

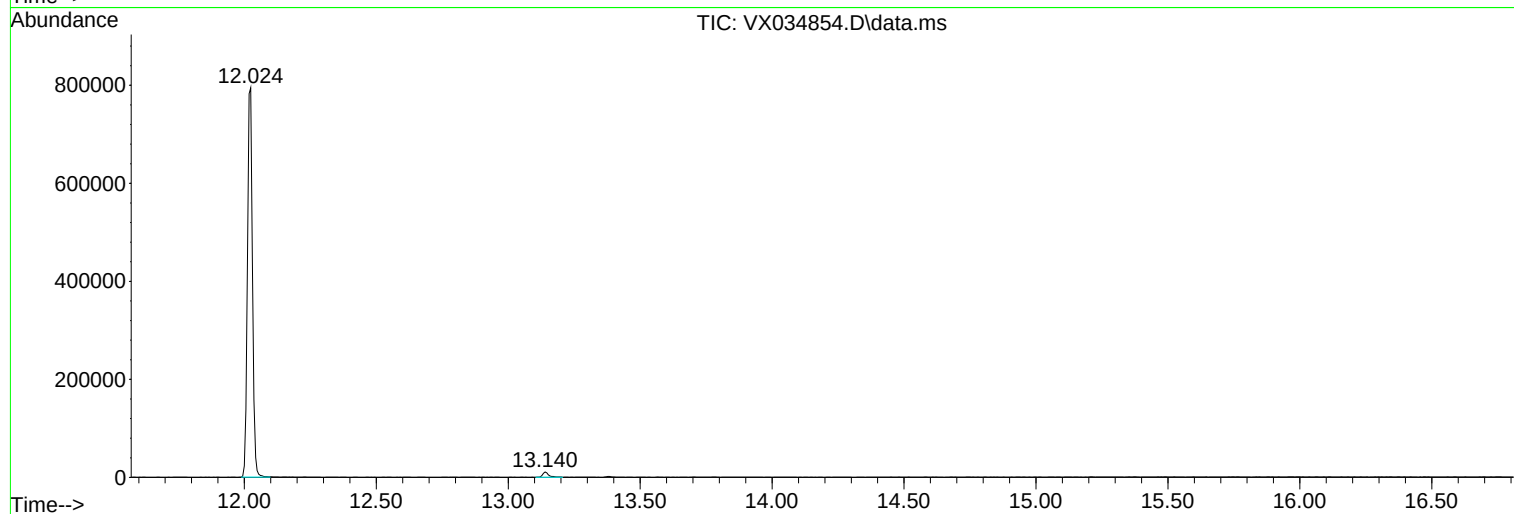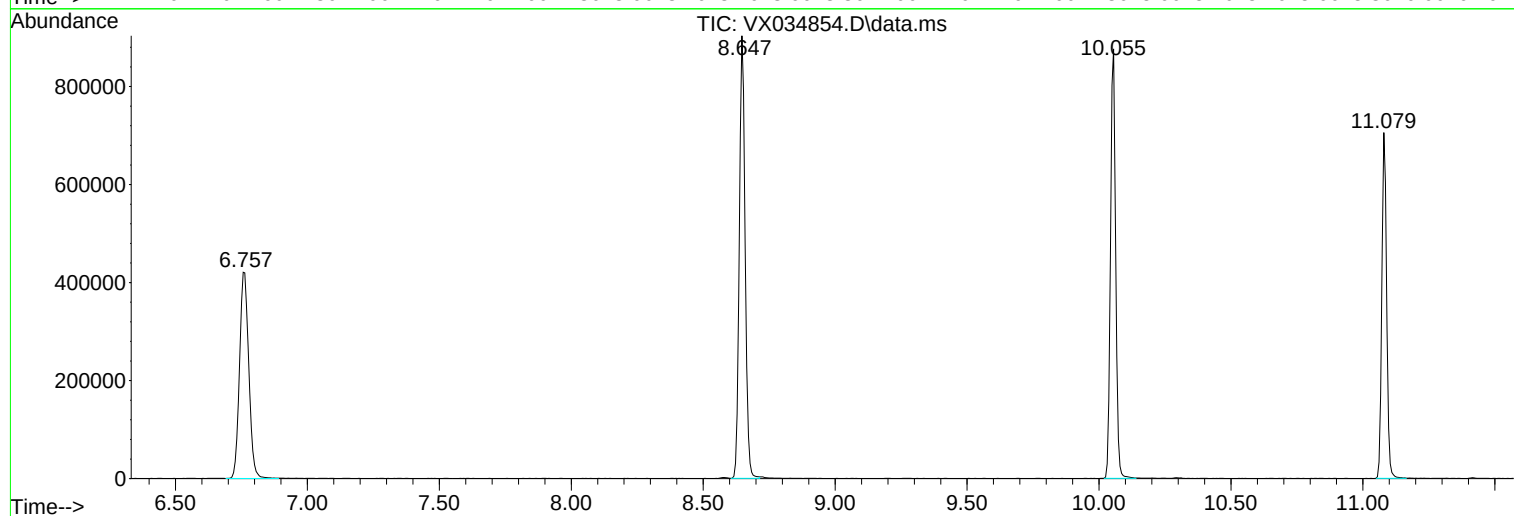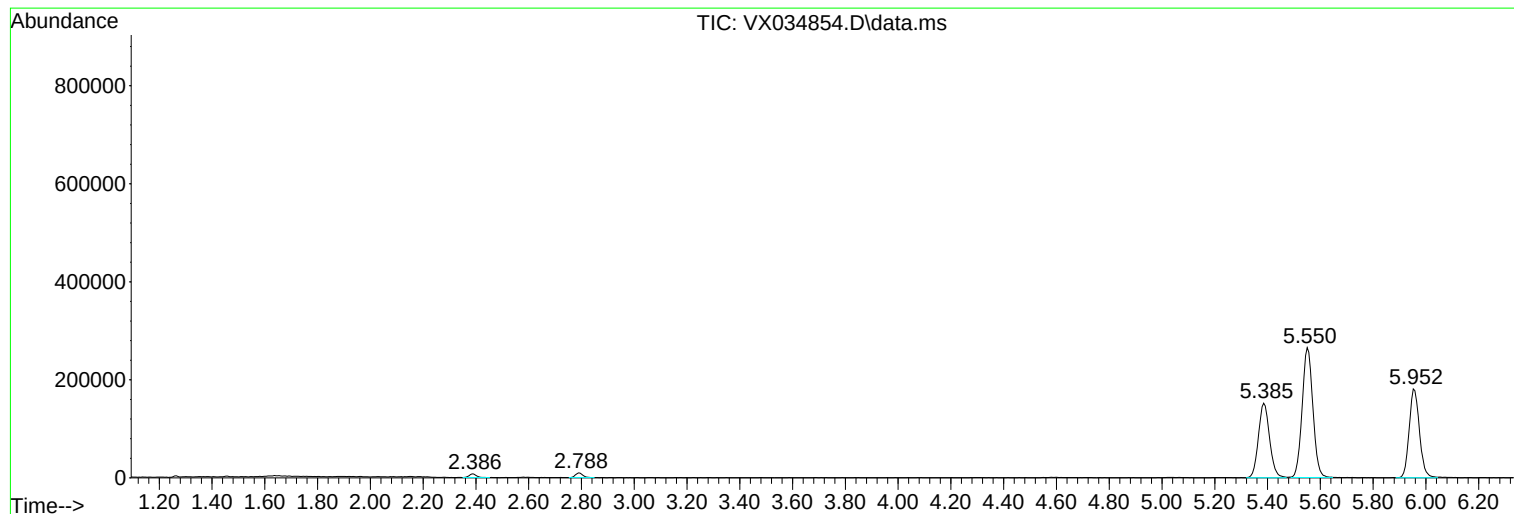

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX033023\
Data File : VX034854.D
Acq On : 30 Mar 2023 15:51
Operator : JC/MD
Sample : 02074-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EB-01-032323

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032923W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX033023\
Data File : VX034854.D
Acq On : 30 Mar 2023 15:51
Operator : JC/MD
Sample : 02074-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EB-01-032323

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032923W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------