

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX033023\  
Data File : VX034857.D  
Acq On : 30 Mar 2023 17:00  
Operator : JC/MD  
Sample : 02096-01  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 19 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-1

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X032923W.M

Title : SW846 8260

Signal : TIC: VX034857.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.385       | 690           | 705         | 721          | rBV2     | 150221         | 440197        | 31.87%          | 6.180%        |
| 2         | 5.550       | 721           | 732         | 750          | rVB      | 260864         | 747429        | 54.12%          | 10.493%       |
| 3         | 5.952       | 788           | 798         | 817          | rBV      | 186556         | 481691        | 34.88%          | 6.762%        |
| 4         | 6.763       | 921           | 931         | 947          | rBV      | 412020         | 1003330       | 72.65%          | 14.085%       |
| 5         | 8.647       | 1233          | 1240        | 1256         | rBV      | 891517         | 1381104       | 100.00%         | 19.389%       |
| 6         | 10.055      | 1465          | 1471        | 1485         | rBV      | 870962         | 1179030       | 85.37%          | 16.552%       |
| 7         | 11.079      | 1634          | 1639        | 1652         | rBV      | 664435         | 874887        | 63.35%          | 12.282%       |
| 8         | 12.024      | 1788          | 1794        | 1806         | rBV      | 792390         | 1015516       | 73.53%          | 14.256%       |




Sum of corrected areas: 7123184

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX033023\  
Data File : VX034857.D  
Acq On : 30 Mar 2023 17:00  
Operator : JC/MD  
Sample : 02096-01  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 19 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X032923W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

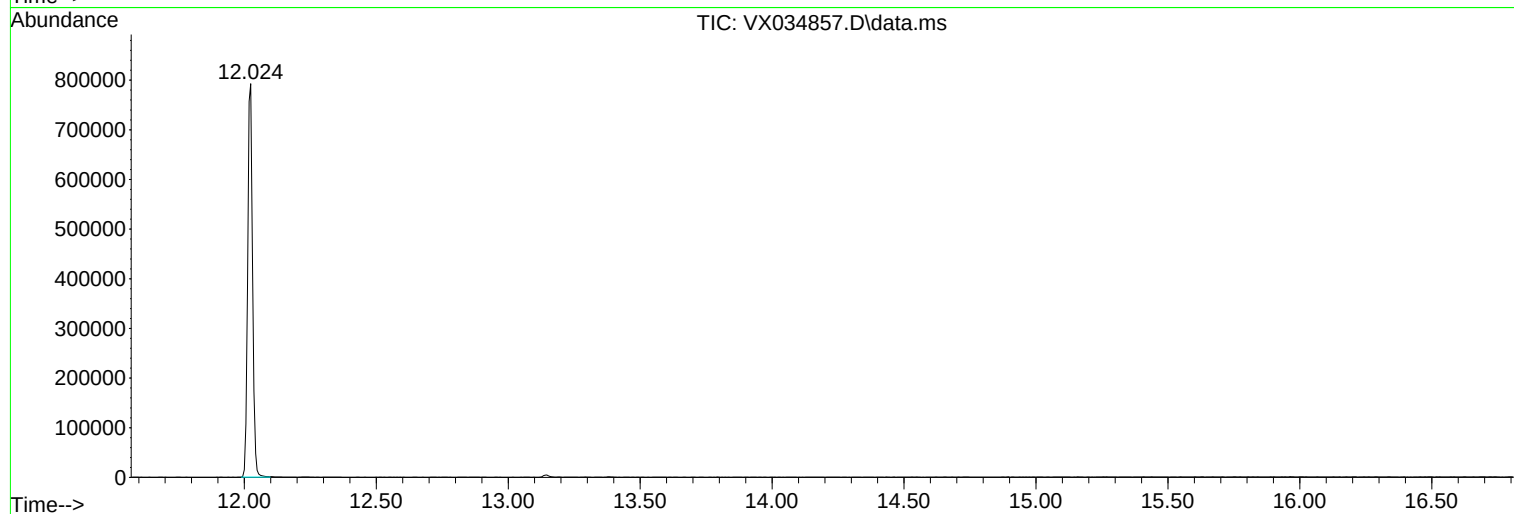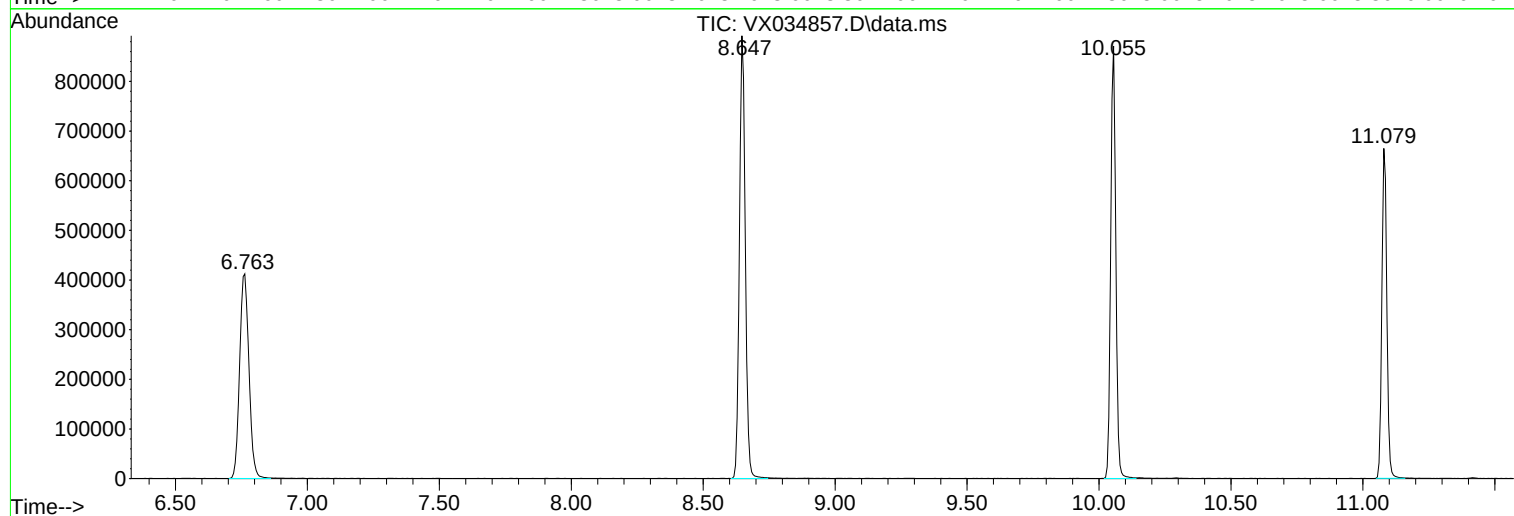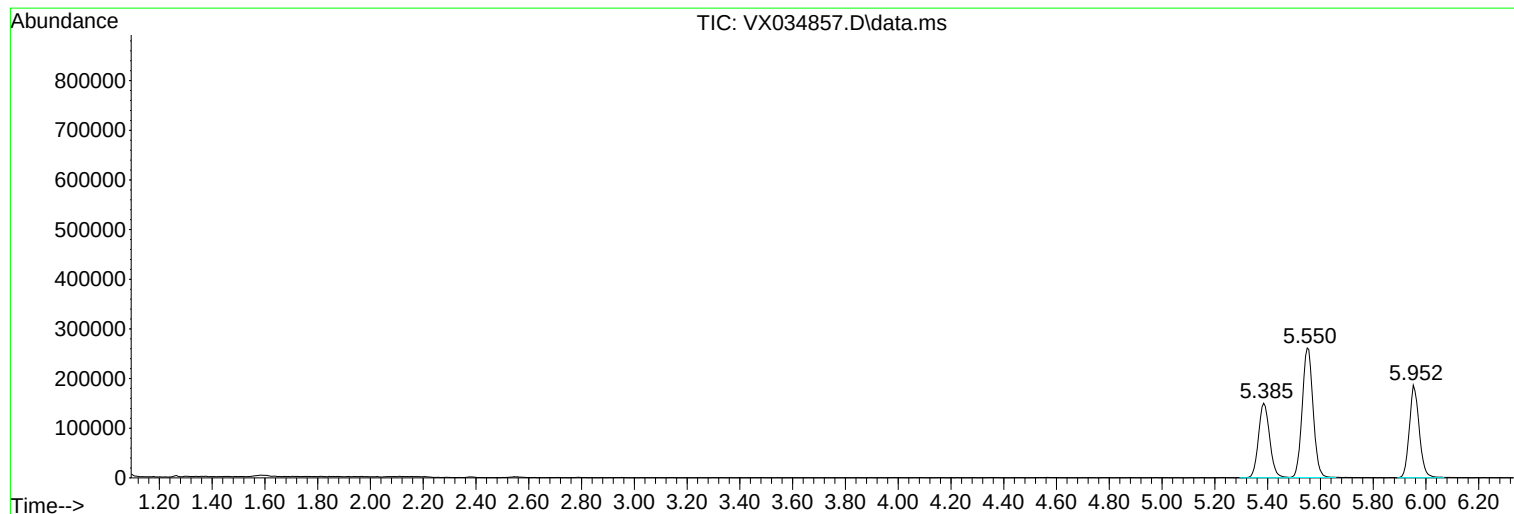

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX033023\  
Data File : VX034857.D  
Acq On : 30 Mar 2023 17:00  
Operator : JC/MD  
Sample : 02096-01  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 19 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X032923W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX033023\  
Data File : VX034857.D  
Acq On : 30 Mar 2023 17:00  
Operator : JC/MD  
Sample : 02096-01  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 19 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X032923W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|