

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX033023\  
Data File : VX034858.D  
Acq On : 30 Mar 2023 17:24  
Operator : JC/MD  
Sample : 02096-03  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 20 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-3

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X032923W.M

Title : SW846 8260

Signal : TIC: VX034858.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.385       | 693           | 705         | 720          | rBV      | 141586         | 410922        | 32.12%          | 6.130%        |
| 2         | 5.550       | 722           | 732         | 748          | rVB      | 241712         | 688242        | 53.79%          | 10.266%       |
| 3         | 5.952       | 789           | 798         | 815          | rBV      | 180694         | 461353        | 36.06%          | 6.882%        |
| 4         | 6.763       | 921           | 931         | 945          | rBV      | 385927         | 937148        | 73.25%          | 13.979%       |
| 5         | 8.647       | 1234          | 1240        | 1256         | rBV      | 814155         | 1279455       | 100.00%         | 19.085%       |
| 6         | 10.055      | 1465          | 1471        | 1485         | rBV      | 804356         | 1107521       | 86.56%          | 16.520%       |
| 7         | 11.079      | 1634          | 1639        | 1654         | rBV      | 645599         | 833033        | 65.11%          | 12.426%       |
| 8         | 12.024      | 1788          | 1794        | 1806         | rBV      | 755364         | 986315        | 77.09%          | 14.712%       |




Sum of corrected areas: 6703989

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX033023\  
Data File : VX034858.D  
Acq On : 30 Mar 2023 17:24  
Operator : JC/MD  
Sample : 02096-03  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 20 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X032923W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

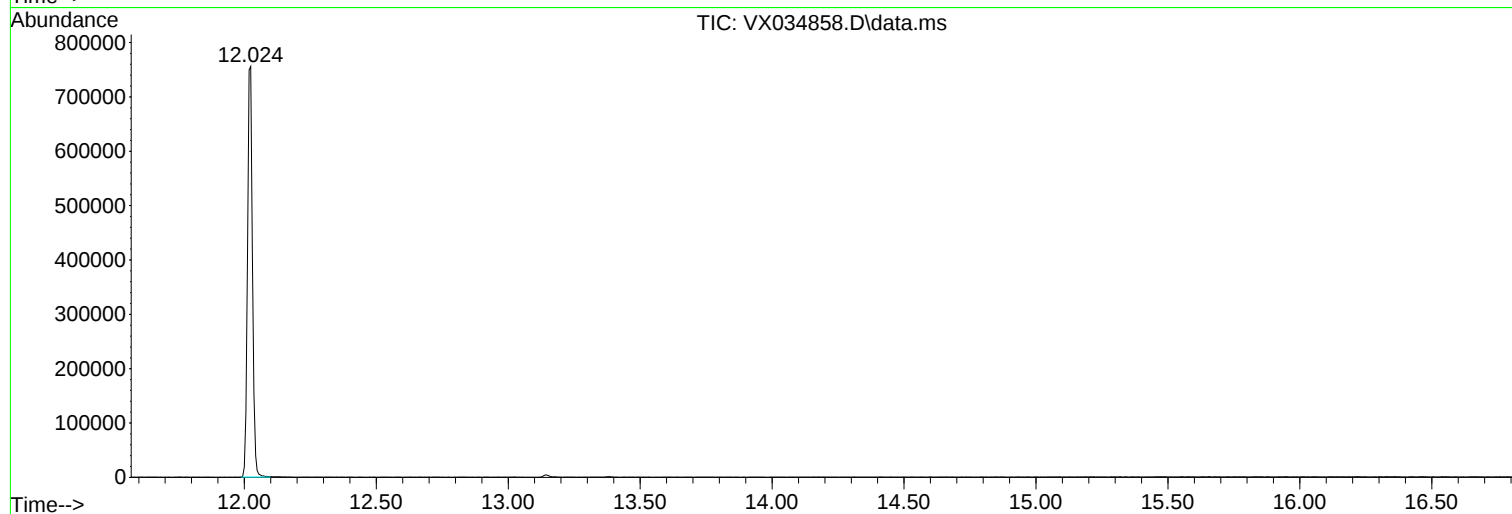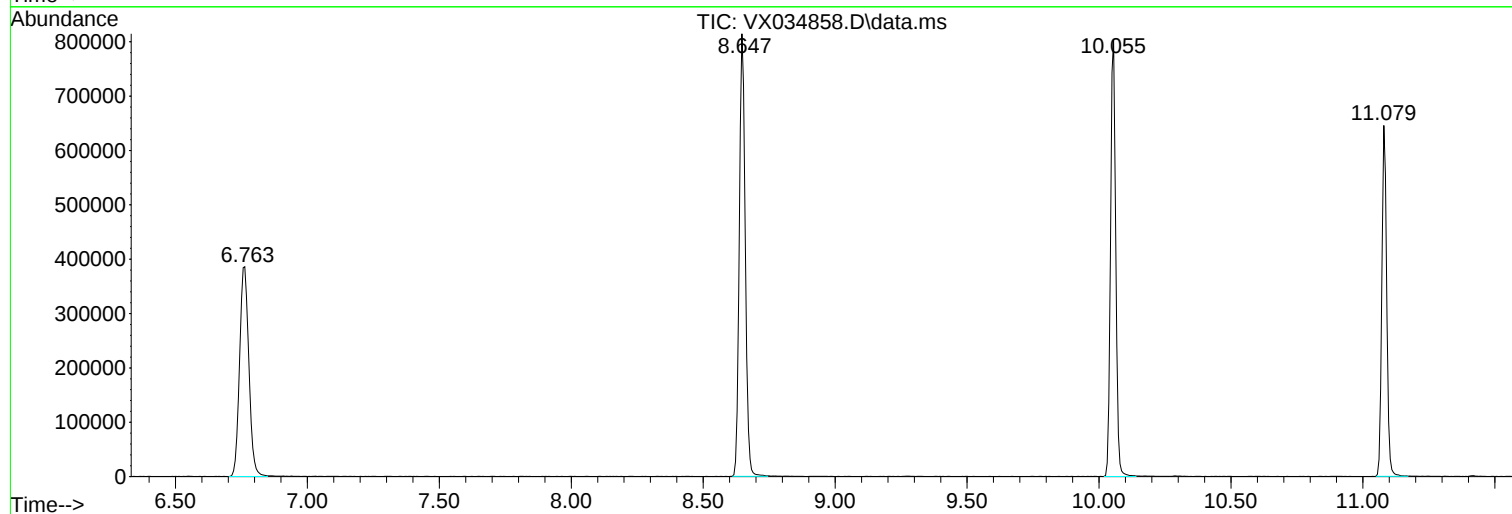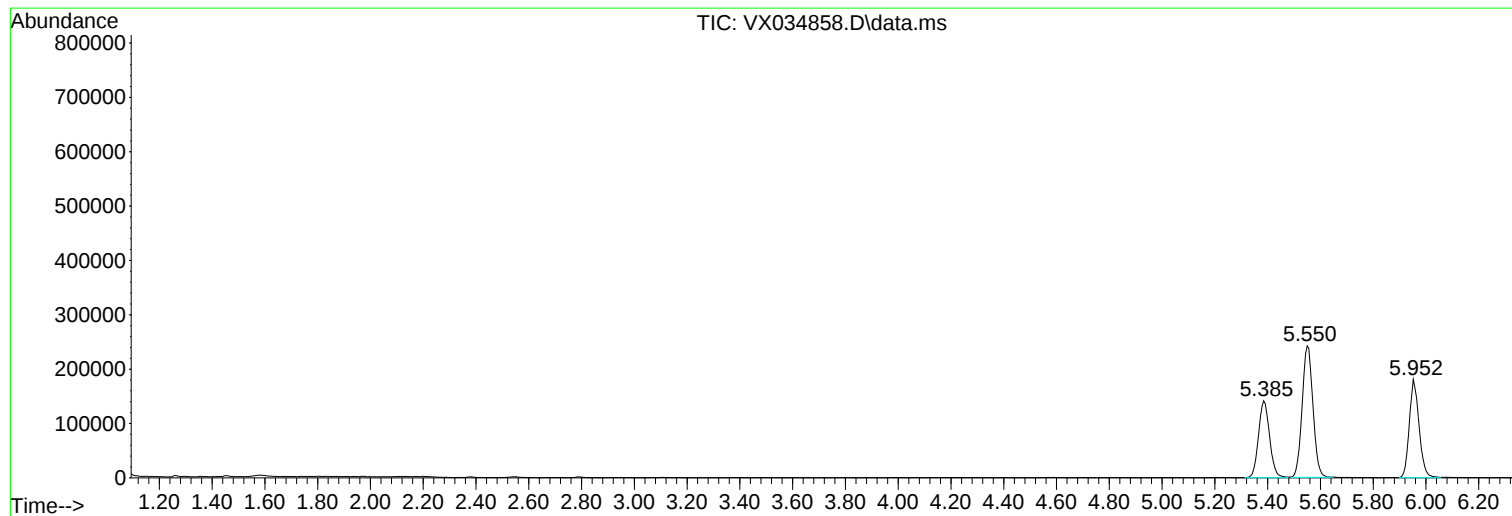

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX033023\  
Data File : VX034858.D  
Acq On : 30 Mar 2023 17:24  
Operator : JC/MD  
Sample : 02096-03  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 20 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X032923W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX033023\  
Data File : VX034858.D  
Acq On : 30 Mar 2023 17:24  
Operator : JC/MD  
Sample : 02096-03  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 20 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X032923W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|