
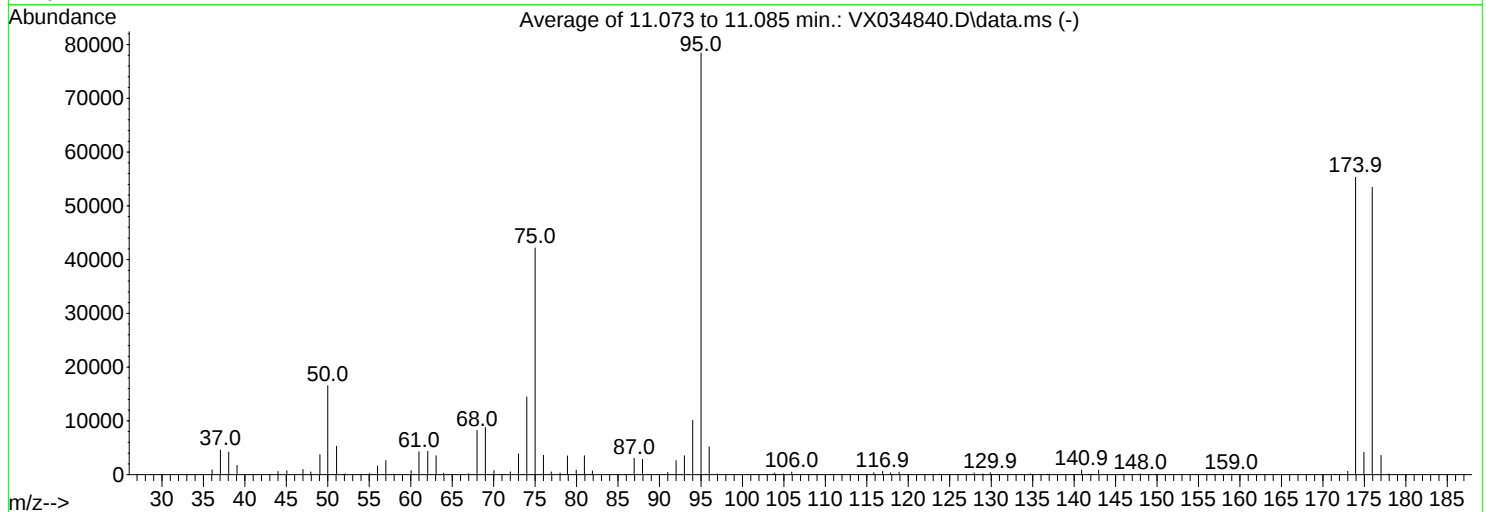


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX033023\
 Data File : VX034840.D
 Acq On : 30 Mar 2023 09:13
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032923W.M
 Title : SW846 8260
 Last Update : Sat Apr 01 01:50:18 2023

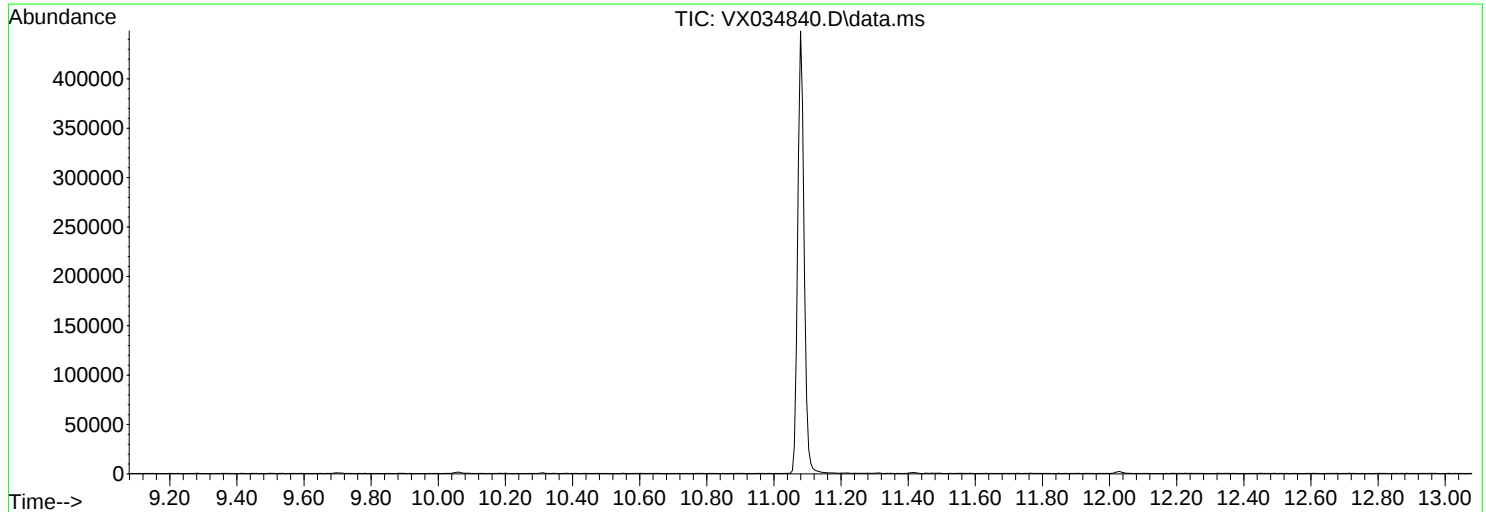

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.1	16548	PASS
75	95	30	60	53.8	42181	PASS
95	95	100	100	100.0	78456	PASS
96	95	5	9	6.6	5158	PASS
173	174	0.00	2	1.1	620	PASS
174	95	50	100	70.5	55339	PASS
175	174	5	9	7.5	4144	PASS
176	174	95	101	96.6	53440	PASS
177	176	5	9	6.7	3582	PASS