

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX033120\
 Data File : VX015451.D
 Acq On : 31 Mar 2020 14:12
 Operator : JC/SP
 Sample : IBLK
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 IBLK

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X032720W.M

Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.064	25	29	42	rBV	3513980	4006767	66.23%	10.557%
2	4.649	607	617	629	rVB2	23070	82080	1.36%	0.216%
3	5.472	740	752	764	rBV	669226	1914178	31.64%	5.043%
4	5.636	767	779	792	rBV	1138124	3238542	53.53%	8.533%
5	6.032	832	844	855	rBV	779439	2038169	33.69%	5.370%
6	6.837	963	976	987	rBV	1808502	4354747	71.98%	11.474%
7	8.697	1275	1281	1298	rVB	3702872	6049973	100.00%	15.940%
8	10.099	1505	1511	1526	rBV	4007588	5514443	91.15%	14.529%
9	11.123	1674	1679	1688	rVB	3627852	4606467	76.14%	12.137%
10	11.794	1785	1789	1793	rVB	76297	90888	1.50%	0.239%
11	12.062	1828	1833	1840	rBV	4870742	5887045	97.31%	15.511%
12	13.330	2038	2041	2049	rVB3	55039	96255	1.59%	0.254%
13	13.818	2117	2121	2129	rVB	50881	74608	1.23%	0.197%


Sum of corrected areas: 37954162

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX033120\
Data File : VX015451.D
Acq On : 31 Mar 2020 14:12
Operator : JC/SP
Sample : IBLK
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X032720W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

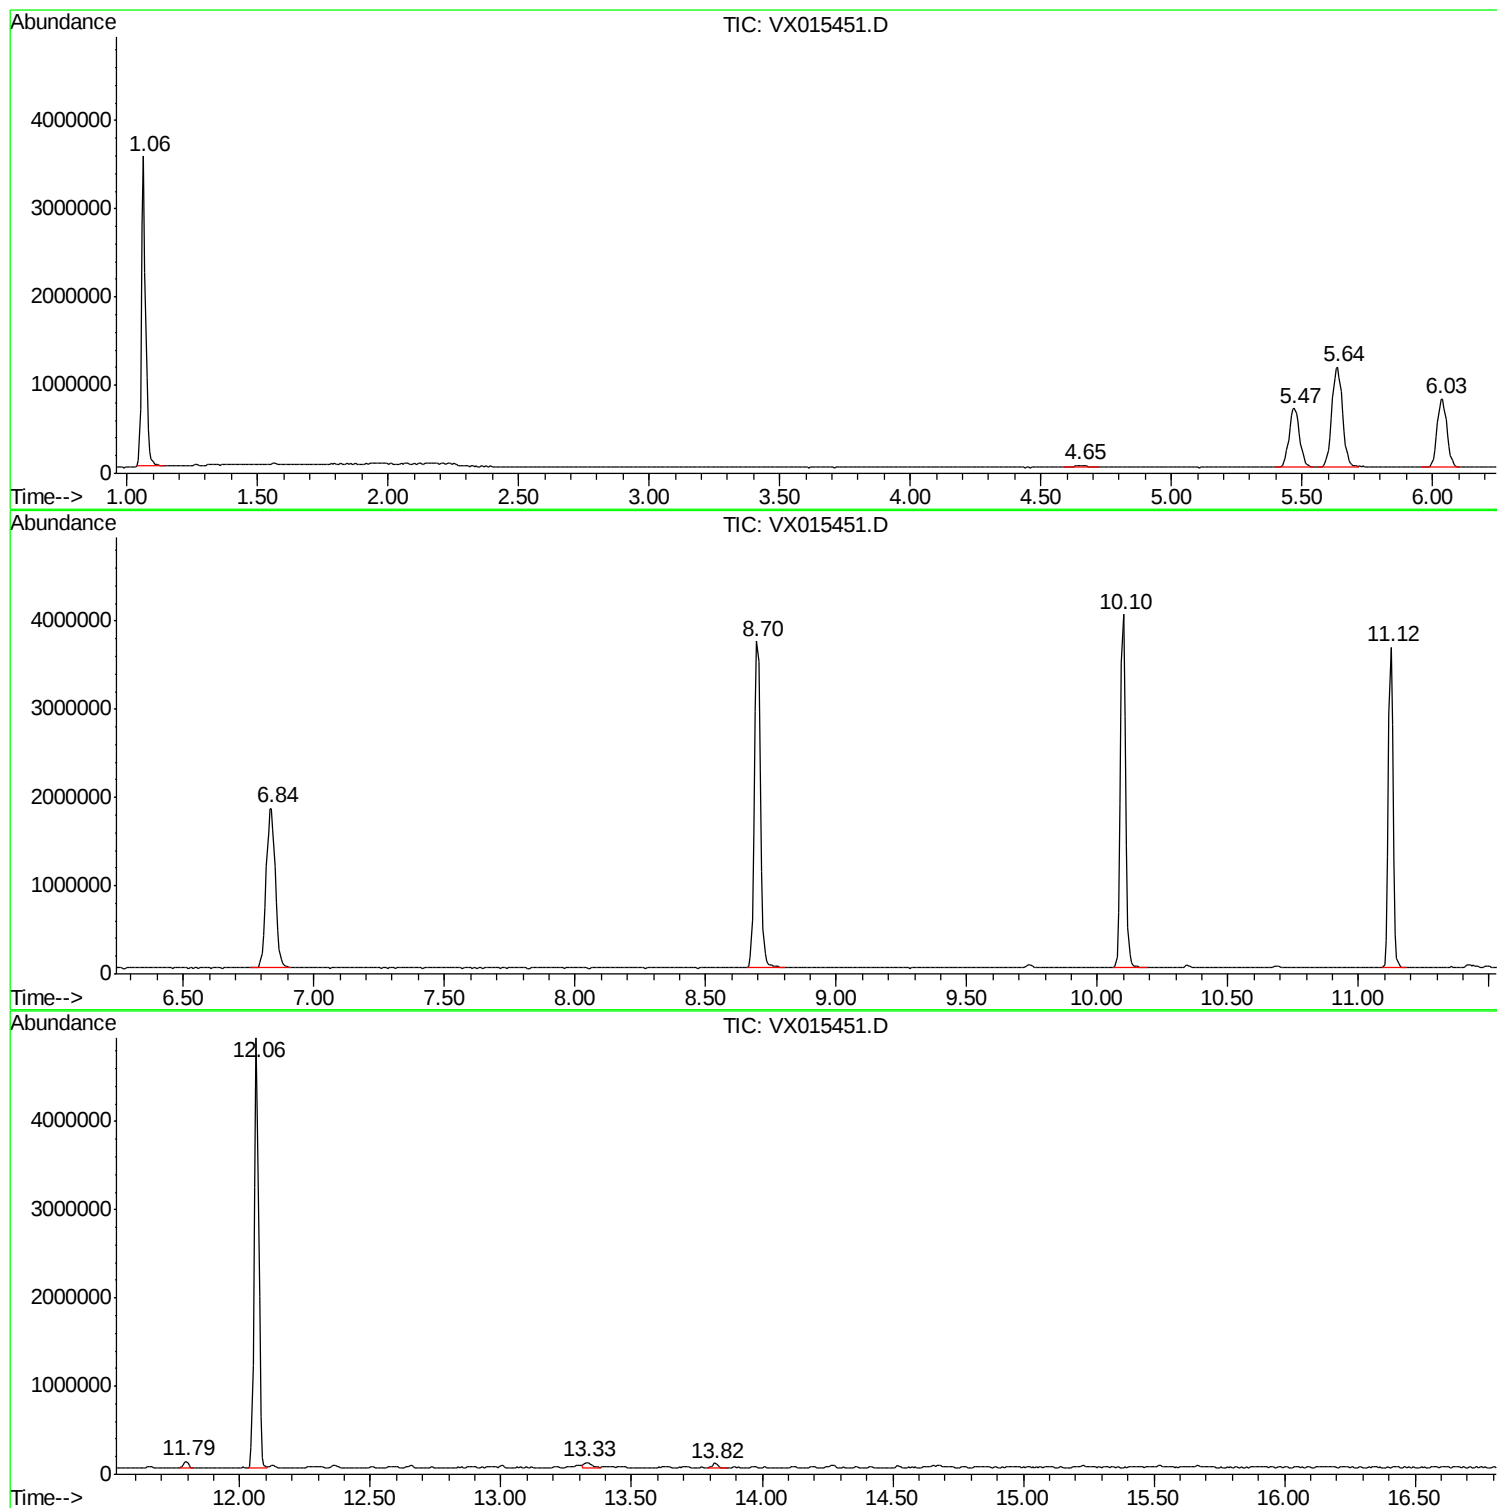

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX033120\
Data File : VX015451.D
Acq On : 31 Mar 2020 14:12
Operator : JC/SP
Sample : IBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X032720W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX033120\
Data File : VX015451.D
Acq On : 31 Mar 2020 14:12
Operator : JC/SP
Sample : IBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X032720W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc