

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX033121\
 Data File : VX021678.D
 Acq On : 31 Mar 2021 12:45
 Operator : JC/MD
 Sample : M1842-14
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 RE123D1-20210324

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M

Title : SW846 8260

Signal : TIC: VX021678.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.593	77	86	89	rBV4	2941	5917	1.58%	0.285%
2	2.593	249	256	260	rBV2	2460	4479	1.20%	0.216%
3	5.470	733	745	758	rBV	48282	134625	36.02%	6.495%
4	5.629	761	772	791	rVB	66145	186594	49.92%	9.002%
5	6.035	831	841	858	rBV	51003	132446	35.43%	6.390%
6	6.835	965	977	989	rBV	111708	268144	71.74%	12.937%
7	7.188	1029	1037	1049	rBV2	16966	36753	9.83%	1.773%
8	8.694	1285	1293	1305	rBV	237387	373783	100.00%	18.033%
9	10.094	1525	1531	1548	rBV	262896	354957	94.96%	17.125%
10	11.118	1700	1705	1717	rVB	207588	268045	71.71%	12.932%
11	12.059	1860	1865	1872	rVB	248743	306986	82.13%	14.811%




Sum of corrected areas: 2072729

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX033121\
Data File : VX021678.D
Acq On : 31 Mar 2021 12:45
Operator : JC/MD
Sample : M1842-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE123D1-20210324

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

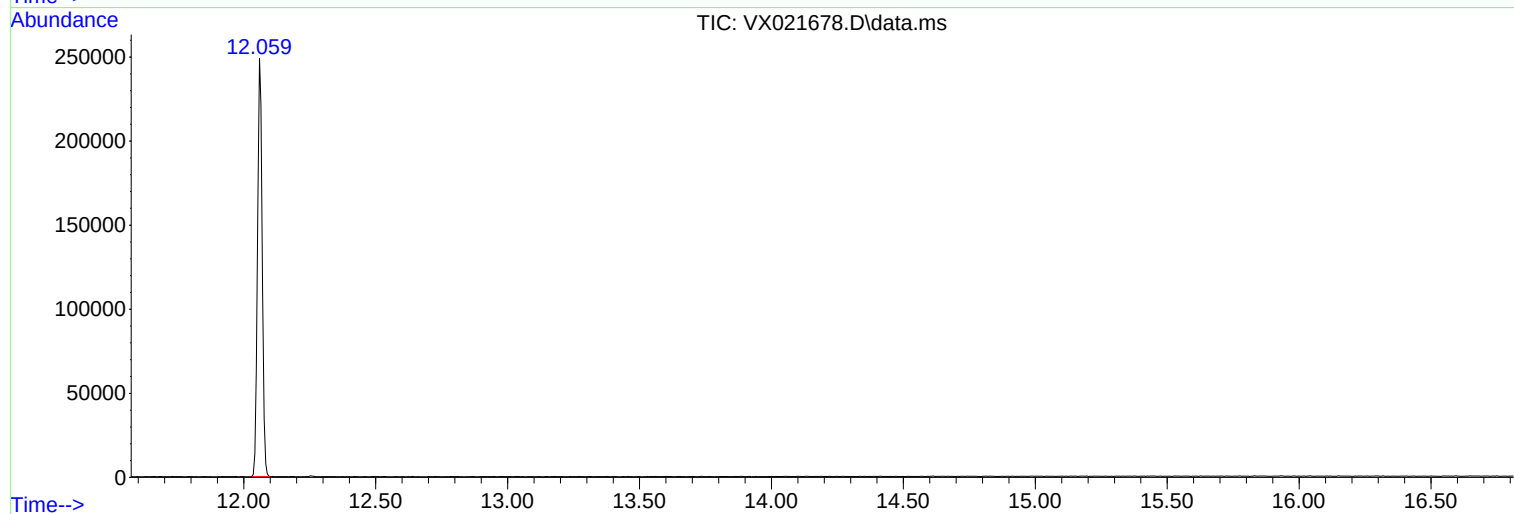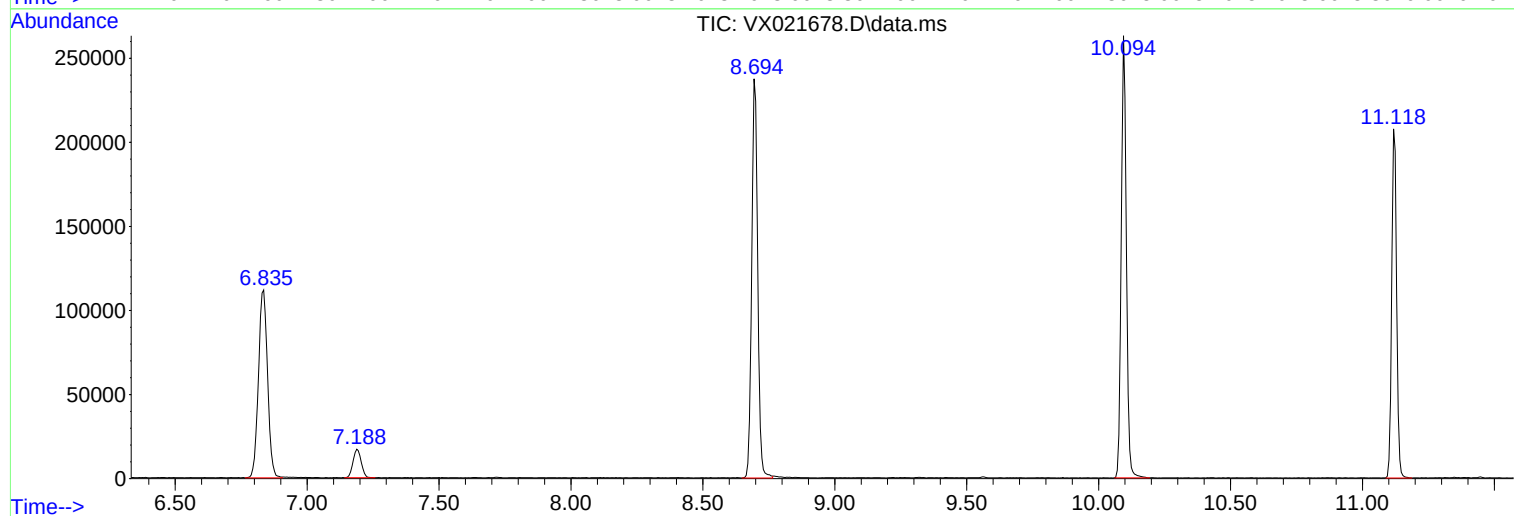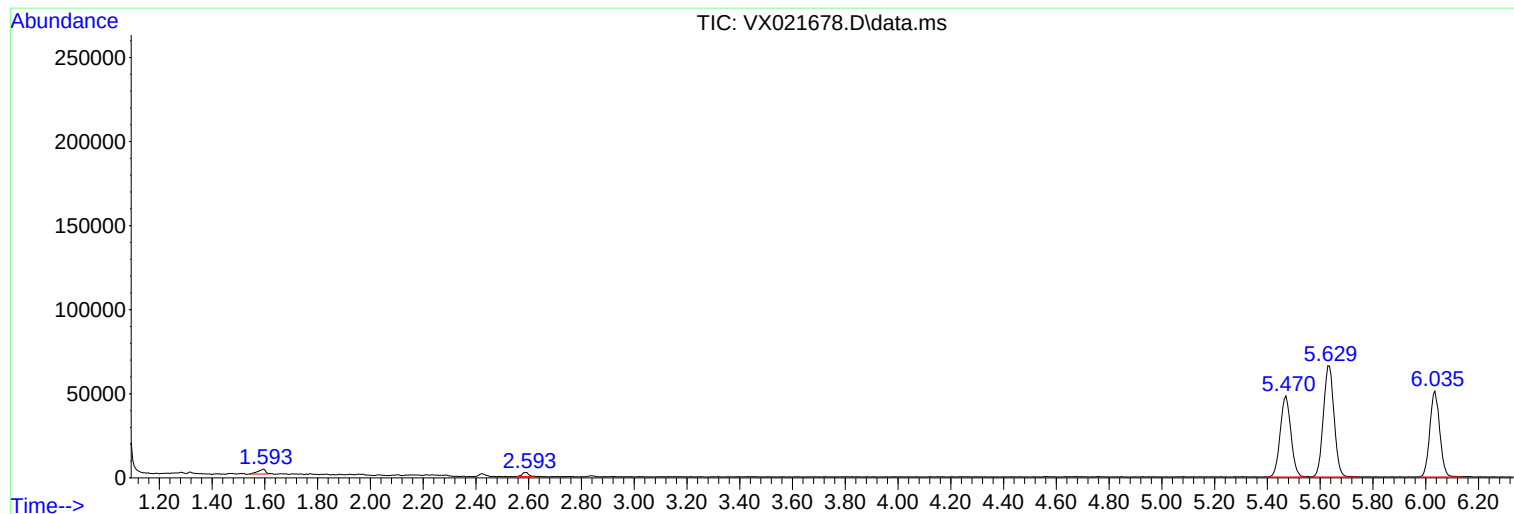

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX033121\
Data File : VX021678.D
Acq On : 31 Mar 2021 12:45
Operator : JC/MD
Sample : M1842-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE123D1-20210324

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX033121\
Data File : VX021678.D
Acq On : 31 Mar 2021 12:45
Operator : JC/MD
Sample : M1842-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE123D1-20210324

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
