

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX033121\
 Data File : VX021679.D
 Acq On : 31 Mar 2021 13:06
 Operator : JC/MD
 Sample : M1842-15
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 RE123D2-20210324

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M

Title : SW846 8260

Signal : TIC: VX021679.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	76	87	89	rBV4	3407	6606	1.75%	0.312%
2	5.470	731	745	756	rBV	48411	136850	36.23%	6.460%
3	5.629	761	772	786	rBV	69061	188670	49.95%	8.906%
4	6.035	828	841	856	rBV2	51933	137341	36.36%	6.483%
5	6.829	967	976	990	rBV	114759	273302	72.36%	12.901%
6	7.188	1031	1037	1048	rVB2	7373	14694	3.89%	0.694%
7	8.694	1286	1293	1306	rBV	240032	377722	100.00%	17.829%
8	9.318	1394	1399	1405	rVB2	9048	13580	3.60%	0.641%
9	10.094	1525	1531	1547	rVB	263489	364917	96.61%	17.225%
10	11.118	1700	1705	1719	rVB	208708	274447	72.66%	12.955%
11	12.059	1860	1865	1875	rVB	262064	330394	87.47%	15.595%




Sum of corrected areas: 2118523

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX033121\
Data File : VX021679.D
Acq On : 31 Mar 2021 13:06
Operator : JC/MD
Sample : M1842-15
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE123D2-20210324

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

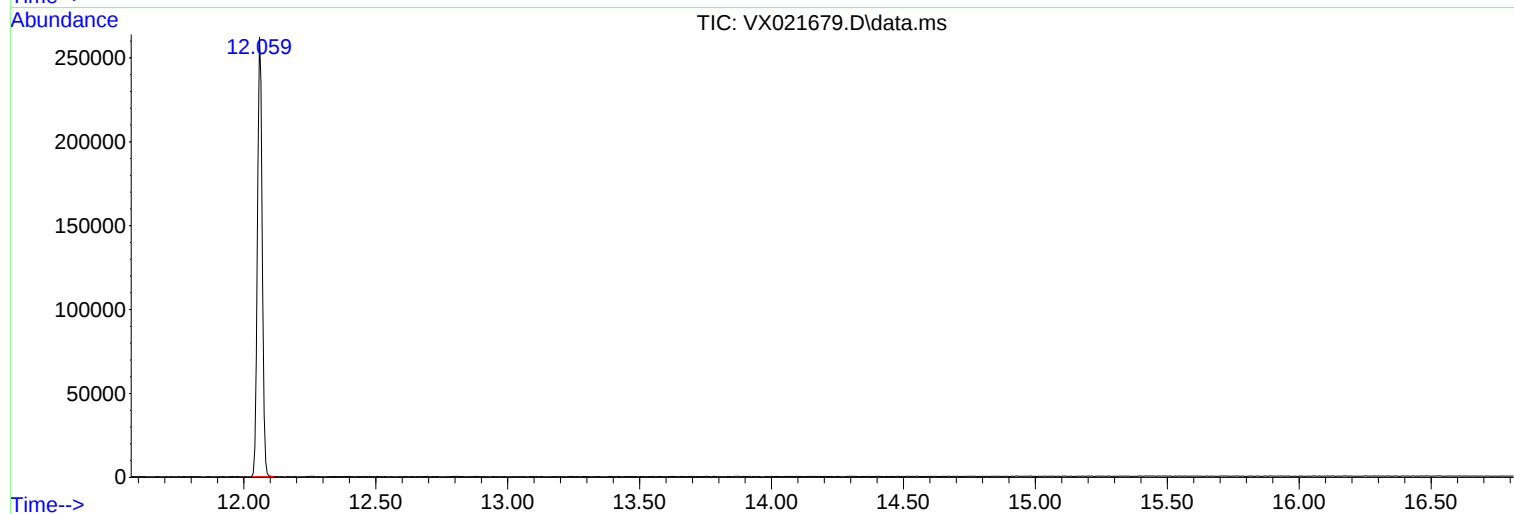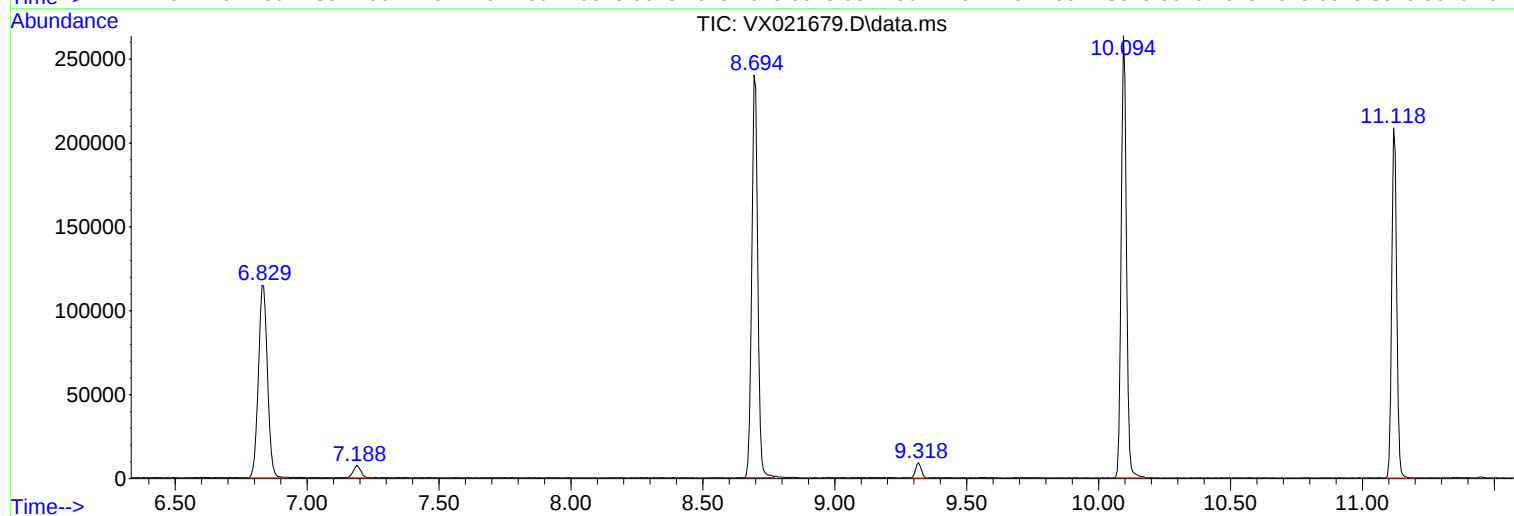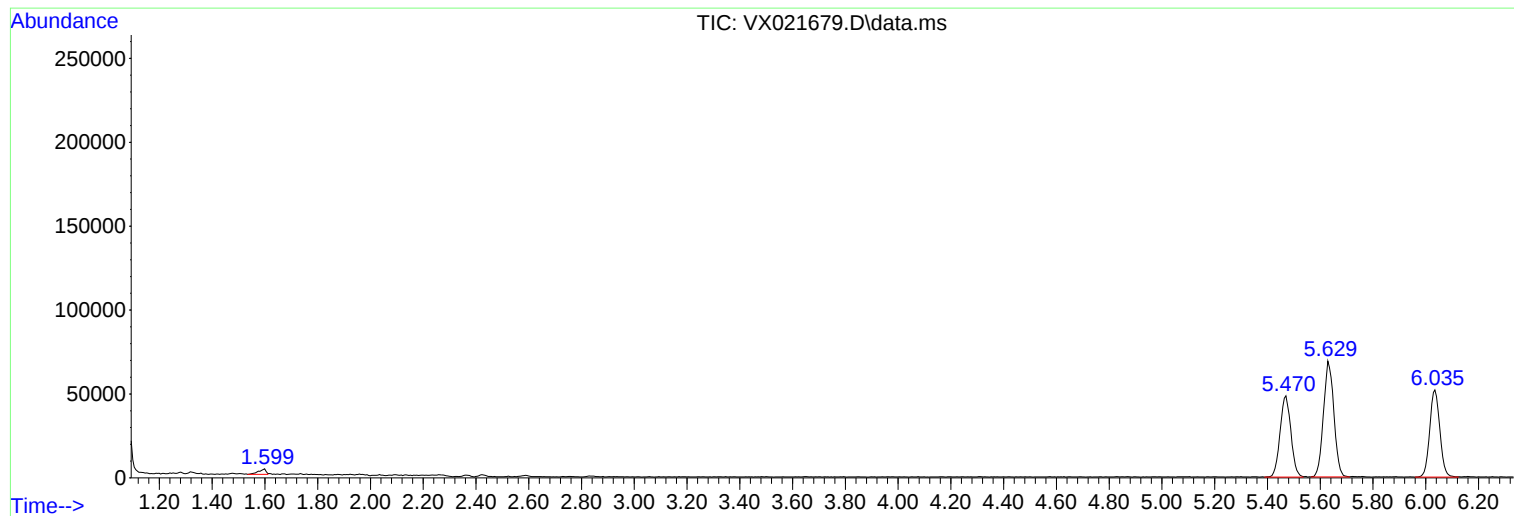

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX033121\
Data File : VX021679.D
Acq On : 31 Mar 2021 13:06
Operator : JC/MD
Sample : M1842-15
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE123D2-20210324

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX033121\
Data File : VX021679.D
Acq On : 31 Mar 2021 13:06
Operator : JC/MD
Sample : M1842-15
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE123D2-20210324

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
