

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX033121\
 Data File : VX021684.D
 Acq On : 31 Mar 2021 14:53
 Operator : JC/MD
 Sample : M1842-20
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW178S-20210324

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M

Title : SW846 8260

Signal : TIC: VX021684.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	80	87	90	rVB5	3037	5846	1.59%	0.284%
2	3.170	347	354	368	rBV2	2949	7403	2.01%	0.360%
3	5.464	734	744	760	rVB	45553	131644	35.80%	6.401%
4	5.635	760	773	787	rBV	64164	181284	49.29%	8.815%
5	6.035	830	841	854	rBV	49196	131897	35.86%	6.414%
6	6.835	966	977	991	rBV	111610	265547	72.21%	12.912%
7	7.194	1031	1038	1042	rBV5	2436	4744	1.29%	0.231%
8	8.700	1286	1294	1305	rBV	232523	367764	100.00%	17.883%
9	10.094	1525	1531	1549	rVB	264888	359084	97.64%	17.460%
10	11.124	1700	1706	1717	rBV	209009	273704	74.42%	13.309%
11	12.059	1860	1865	1873	rBV	262747	327634	89.09%	15.931%




Sum of corrected areas: 2056551

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX033121\
Data File : VX021684.D
Acq On : 31 Mar 2021 14:53
Operator : JC/MD
Sample : M1842-20
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW178S-20210324

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

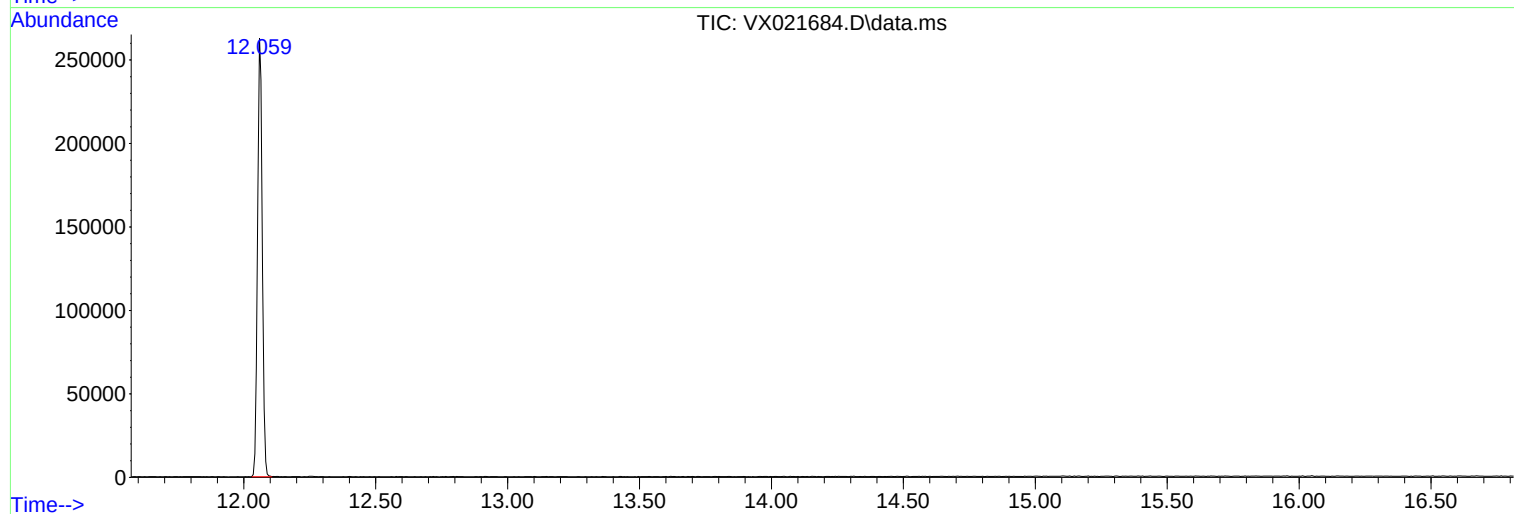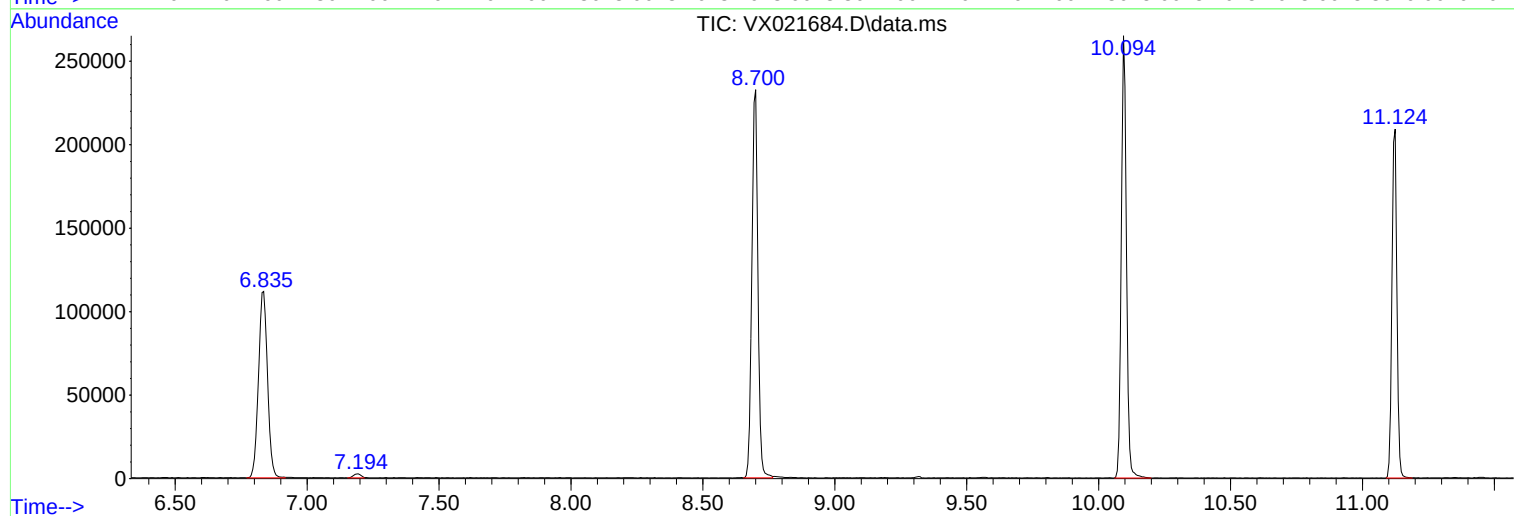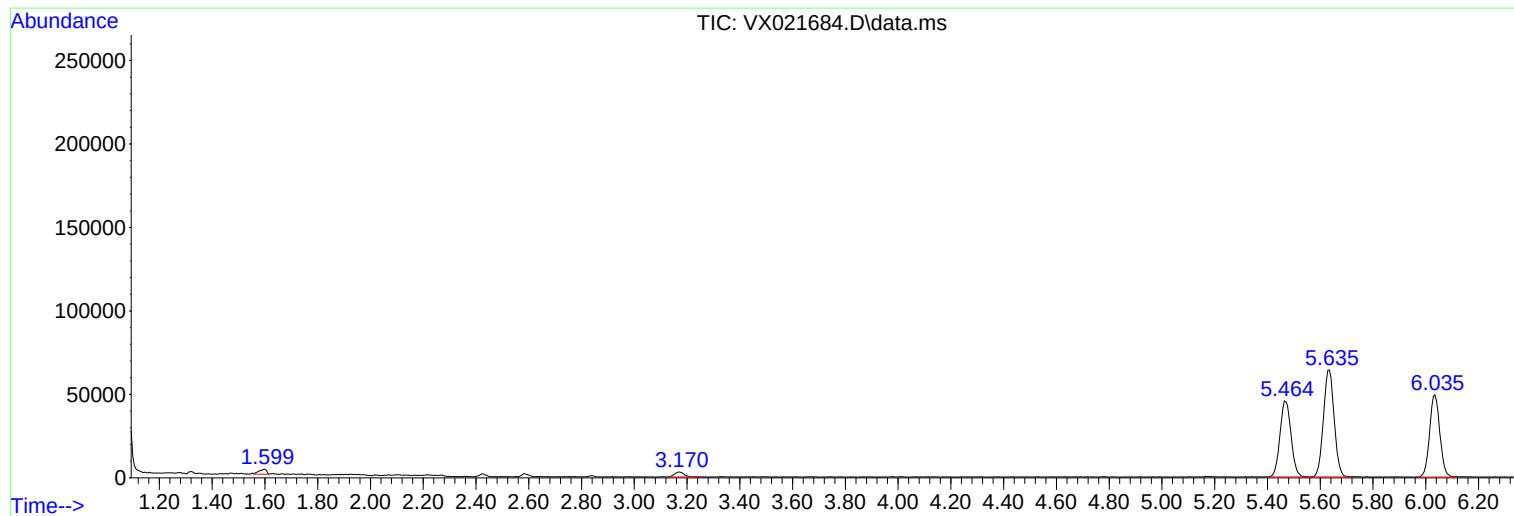

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX033121\
Data File : VX021684.D
Acq On : 31 Mar 2021 14:53
Operator : JC/MD
Sample : M1842-20
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW178S-20210324

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX033121\
Data File : VX021684.D
Acq On : 31 Mar 2021 14:53
Operator : JC/MD
Sample : M1842-20
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW178S-20210324

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
