

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX033121\
 Data File : VX021690.D
 Acq On : 31 Mar 2021 17:01
 Operator : JC/MD
 Sample : M1842-20
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW178S-20210324

Integration Parameters: RTEINT.P

Integrator: RTE

Smoother: ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M

Title : SW846 8260

Signal : TIC: VX021690.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	78	87	90	rBV4	2839	5873	1.66%	0.304%
2	2.587	247	255	263	rBV	3519	7131	2.02%	0.370%
3	3.170	344	354	361	rBV2	3133	7222	2.05%	0.374%
4	5.464	733	744	757	rBV	44352	126772	35.90%	6.572%
5	5.629	761	772	786	rBV2	64382	175490	49.69%	9.097%
6	6.029	830	840	853	rBV	48762	127686	36.16%	6.619%
7	6.829	966	976	992	rBV	104773	250534	70.94%	12.988%
8	8.694	1286	1293	1315	rBV	226837	353154	100.00%	18.307%
9	10.094	1525	1531	1546	rVB	242947	334259	94.65%	17.328%
10	11.118	1700	1705	1715	rBV	191532	253843	71.88%	13.159%
11	12.059	1860	1865	1874	rBV	226077	287071	81.29%	14.882%




Sum of corrected areas: 1929035

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX033121\
Data File : VX021690.D
Acq On : 31 Mar 2021 17:01
Operator : JC/MD
Sample : M1842-20
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW178S-20210324

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

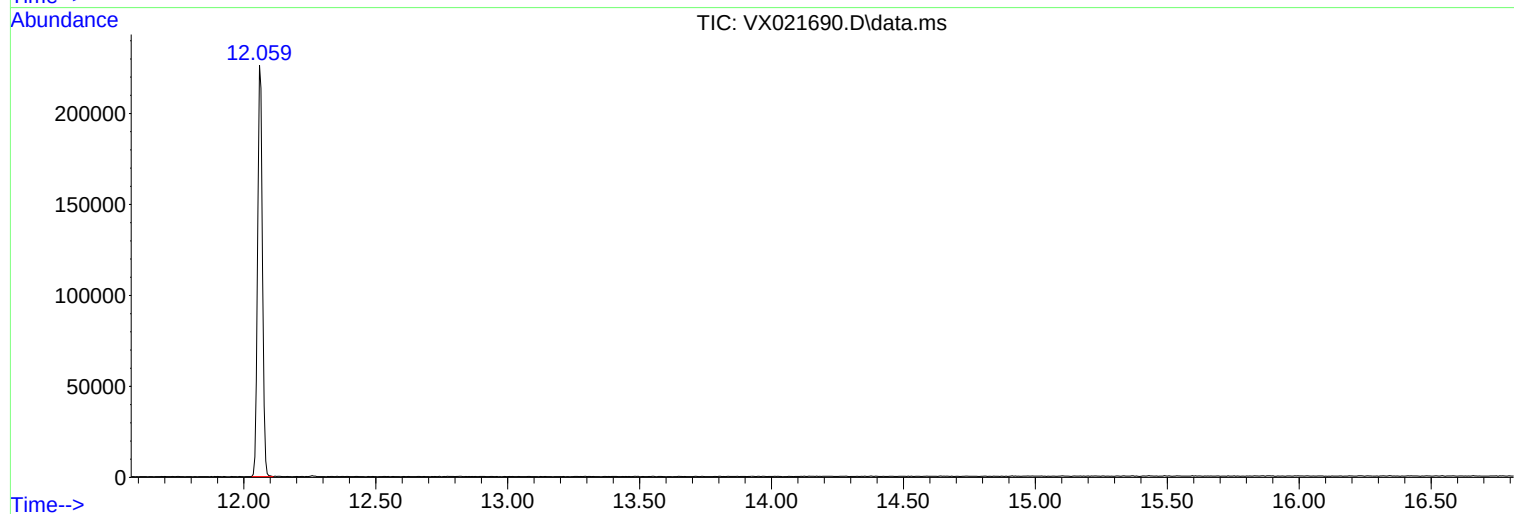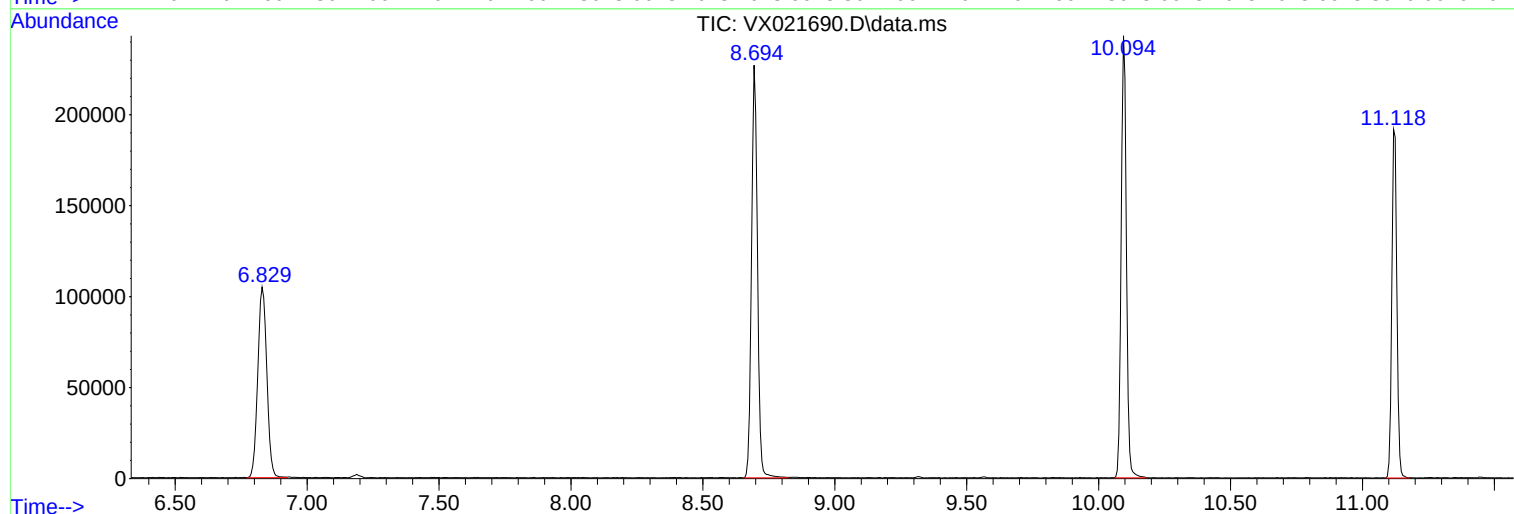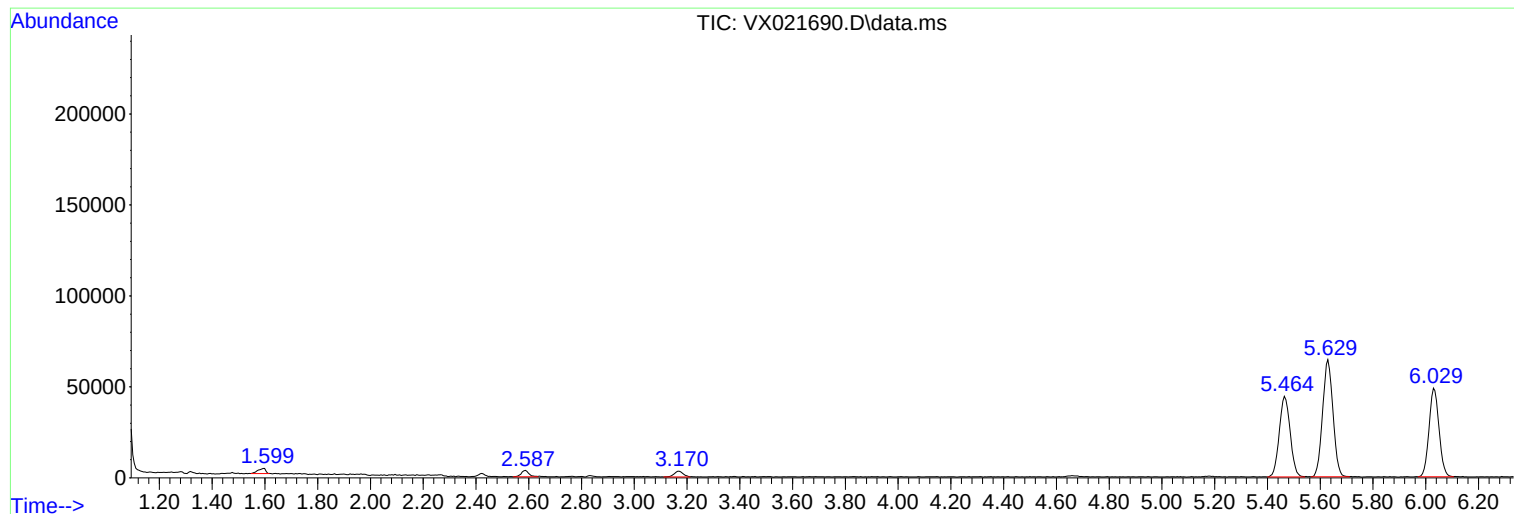

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX033121\
Data File : VX021690.D
Acq On : 31 Mar 2021 17:01
Operator : JC/MD
Sample : M1842-20
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW178S-20210324

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX033121\
Data File : VX021690.D
Acq On : 31 Mar 2021 17:01
Operator : JC/MD
Sample : M1842-20
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW178S-20210324

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------