
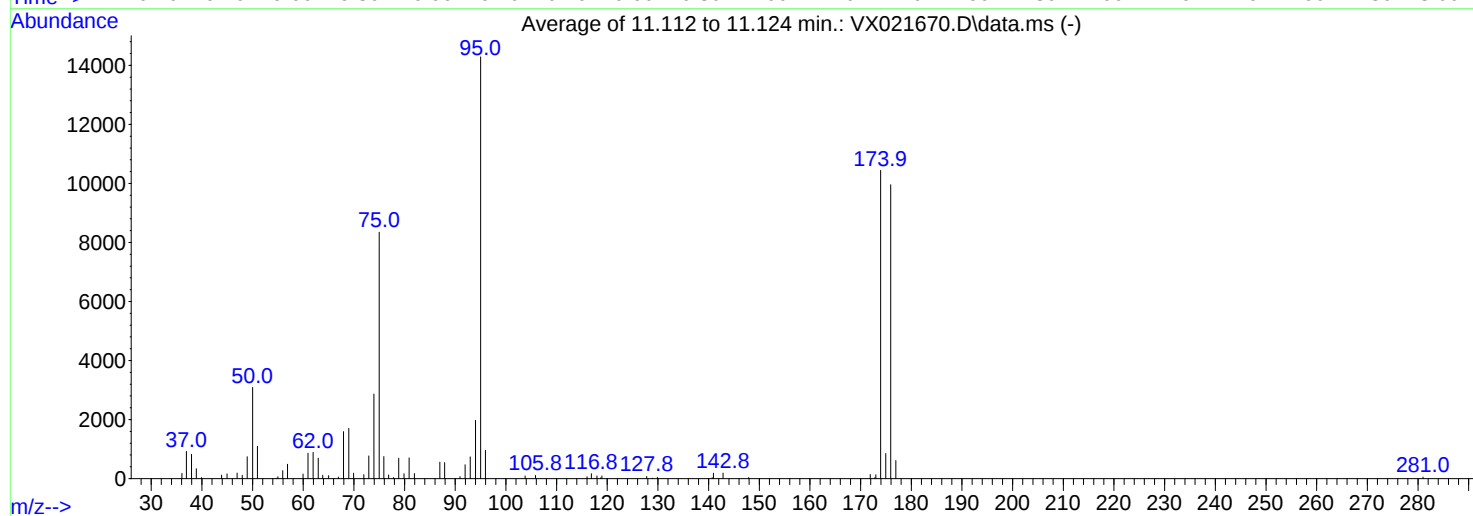


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX033121\
 Data File : VX021670.D
 Acq On : 31 Mar 2021 08:48
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M
 Title : SW846 8260
 Last Update : Wed Mar 24 12:25:26 2021

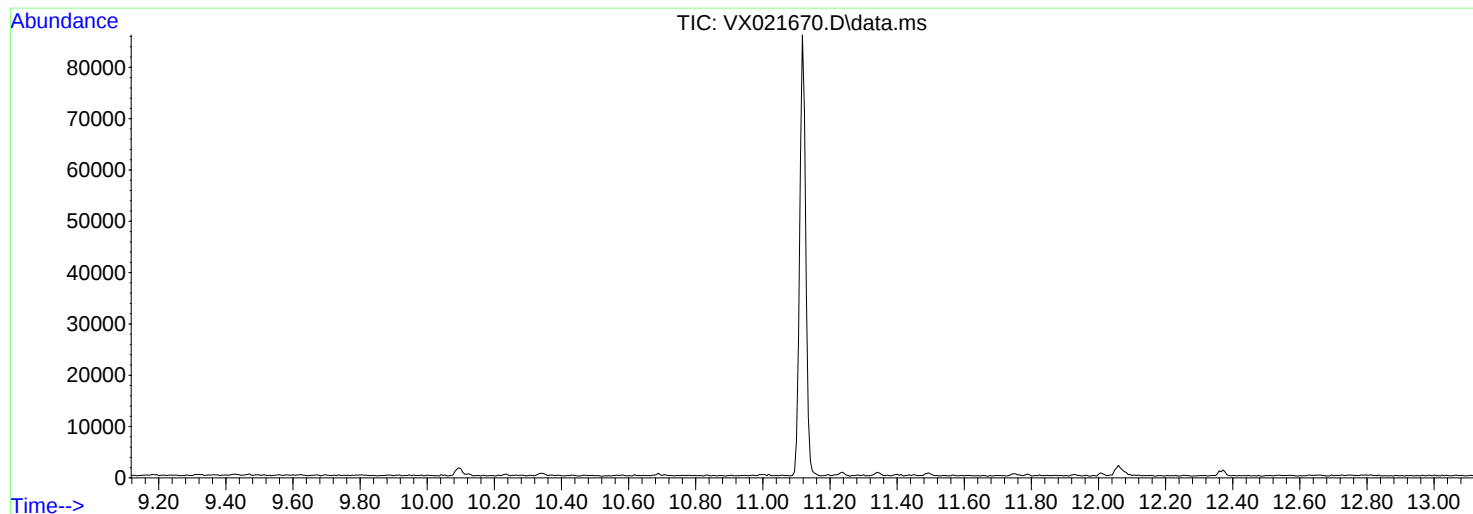

AutoFind: Scans 1704, 1705, 1706; Background Corrected with Scan 1698

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.6	3088	PASS
75	95	30	60	58.4	8349	PASS
95	95	100	100	100.0	14289	PASS
96	95	5	9	6.7	957	PASS
173	174	0.00	2	1.2	129	PASS
174	95	50	100	73.1	10444	PASS
175	174	5	9	8.1	851	PASS
176	174	95	101	95.3	9955	PASS
177	176	5	9	6.2	615	PASS