

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX033122\
Data File : VX027842.D
Acq On : 31 Mar 2022 12:57
Operator : JC/MD
Sample : N2041-05RE
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE117D1-20220317RE

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032922W.M

Title : SW846 8260

Signal : TIC: VX027842.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	20	26	32	rBV3	3144	6834	1.81%	0.303%
2	2.544	230	239	249	rBV	4987	9253	2.46%	0.410%
3	5.391	695	706	723	rBV2	46381	132552	35.20%	5.879%
4	5.556	723	733	747	rVV2	80087	229033	60.82%	10.157%
5	5.958	788	799	815	rVB	45761	122335	32.49%	5.425%
6	6.763	922	931	945	rBV	115213	280542	74.50%	12.442%
7	7.129	981	991	1006	rBV	141552	300758	79.86%	13.338%
8	8.653	1234	1241	1250	rBV	237851	376585	100.00%	16.701%
9	10.055	1465	1471	1480	rBV	240172	315111	83.68%	13.975%
10	11.085	1634	1640	1652	rBV	171457	227340	60.37%	10.082%
11	12.024	1789	1794	1803	rVB	211441	254501	67.58%	11.287%




Sum of corrected areas: 2254844

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX033122\
Data File : VX027842.D
Acq On : 31 Mar 2022 12:57
Operator : JC/MD
Sample : N2041-05RE
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE117D1-20220317RE

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032922W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

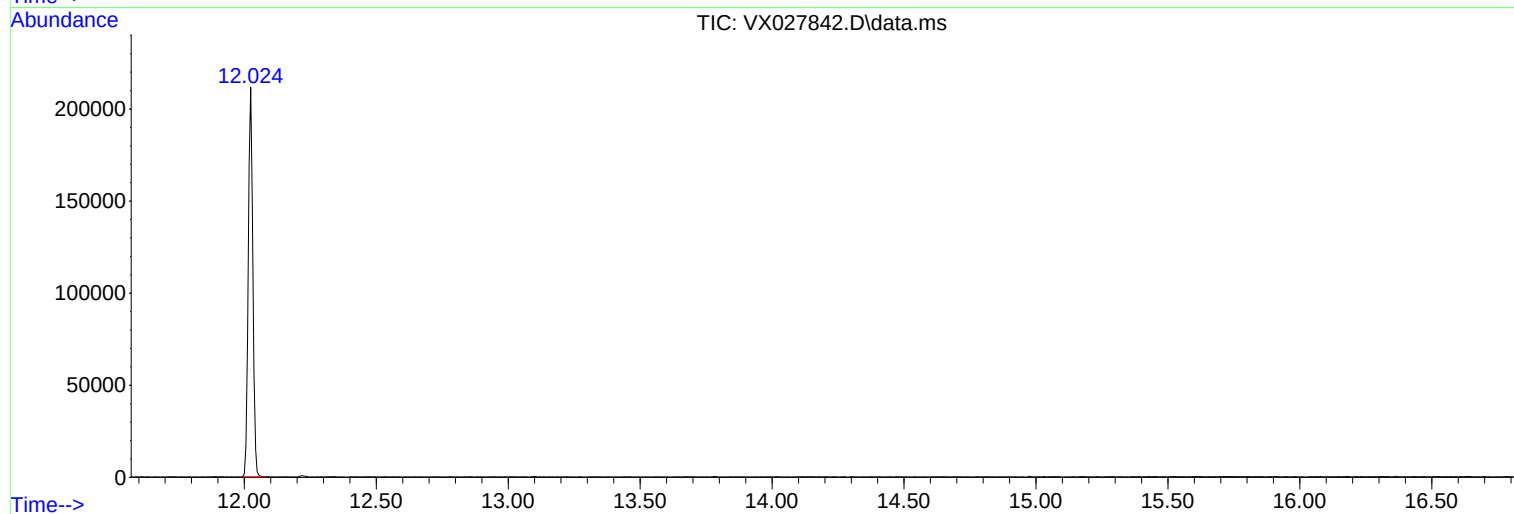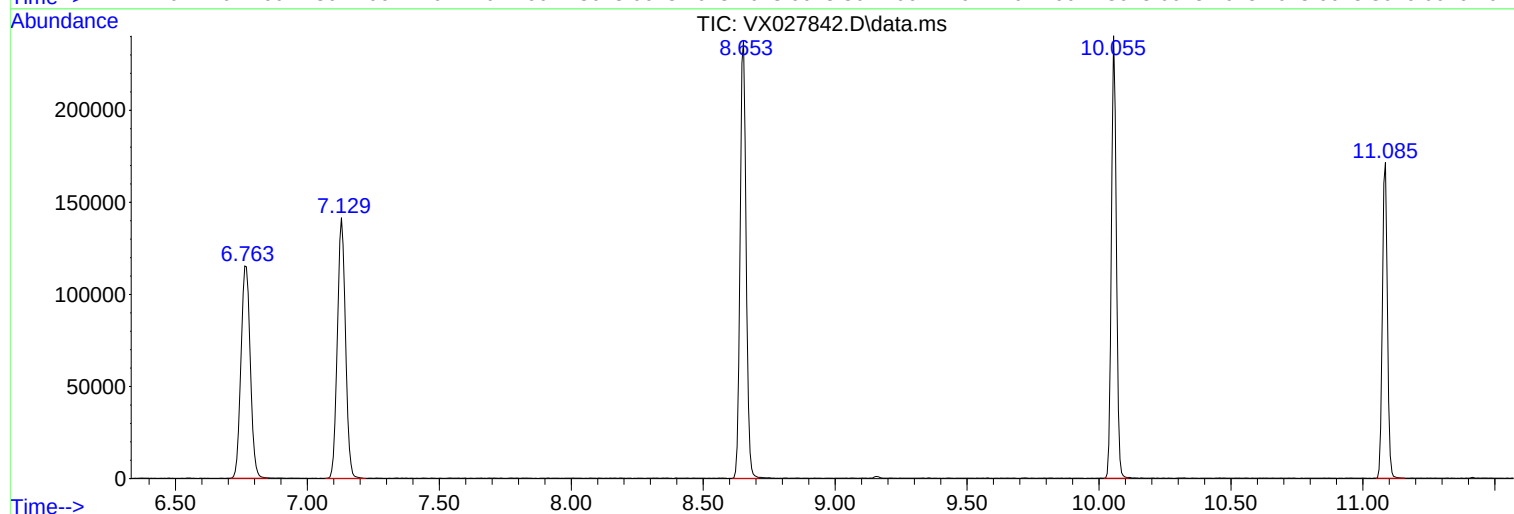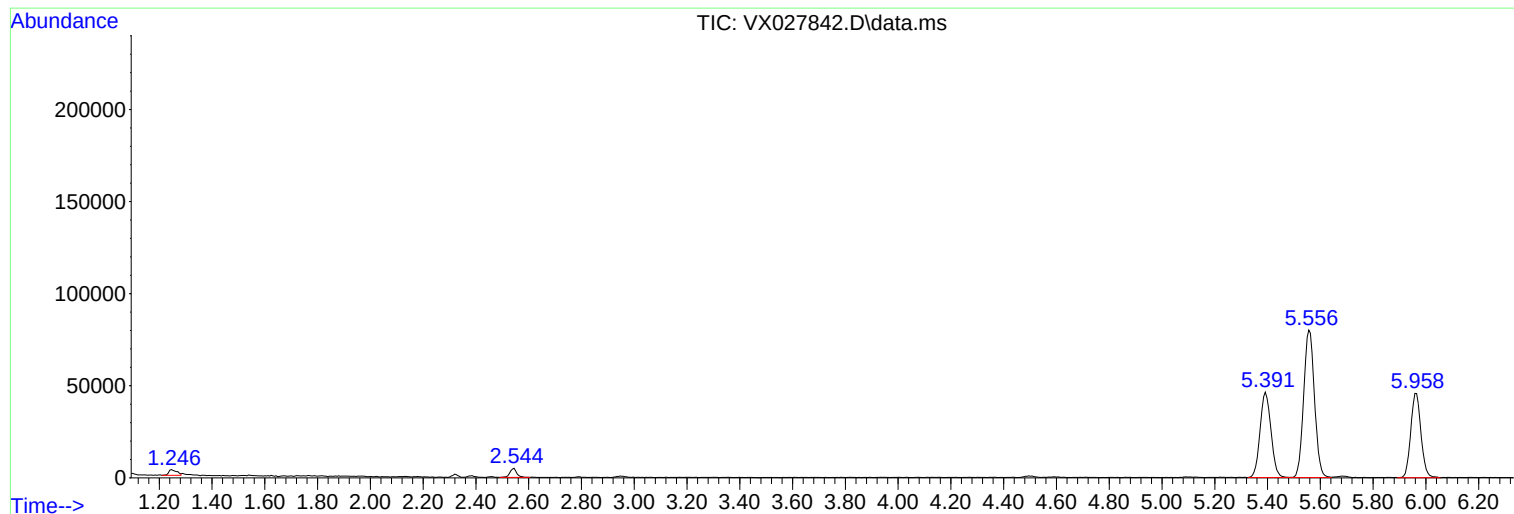

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX033122\
Data File : VX027842.D
Acq On : 31 Mar 2022 12:57
Operator : JC/MD
Sample : N2041-05RE
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE117D1-20220317RE

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032922W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX033122\
Data File : VX027842.D
Acq On : 31 Mar 2022 12:57
Operator : JC/MD
Sample : N2041-05RE
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE117D1-20220317RE

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032922W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc