

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX033122\
 Data File : VX027843.D
 Acq On : 31 Mar 2022 13:20
 Operator : JC/MD
 Sample : N2041-23
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 FB-01-20220318

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032922W.M

Title : SW846 8260

Signal : TIC: VX027843.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	22	26	27	rBV2	3496	4023	1.04%	0.186%
2	1.270	27	30	41	rVB	8694	10994	2.84%	0.508%
3	2.386	207	213	219	rBV	2718	4617	1.19%	0.213%
4	2.538	230	238	250	rBV	7359	14261	3.69%	0.658%
5	5.391	695	706	720	rBV2	50564	146711	37.93%	6.773%
6	5.556	723	733	750	rVB2	83317	236865	61.25%	10.935%
7	5.964	789	800	814	rBV	48533	125438	32.43%	5.791%
8	6.769	922	932	947	rBV	118926	288526	74.60%	13.320%
9	8.653	1234	1241	1250	rBV	249676	386748	100.00%	17.855%
10	10.055	1465	1471	1480	rBV	261554	354882	91.76%	16.384%
11	11.085	1634	1640	1654	rVB	208639	269295	69.63%	12.432%
12	12.024	1789	1794	1802	rBV	268302	323704	83.70%	14.944%




Sum of corrected areas: 2166064

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX033122\
Data File : VX027843.D
Acq On : 31 Mar 2022 13:20
Operator : JC/MD
Sample : N2041-23
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FB-01-20220318

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032922W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

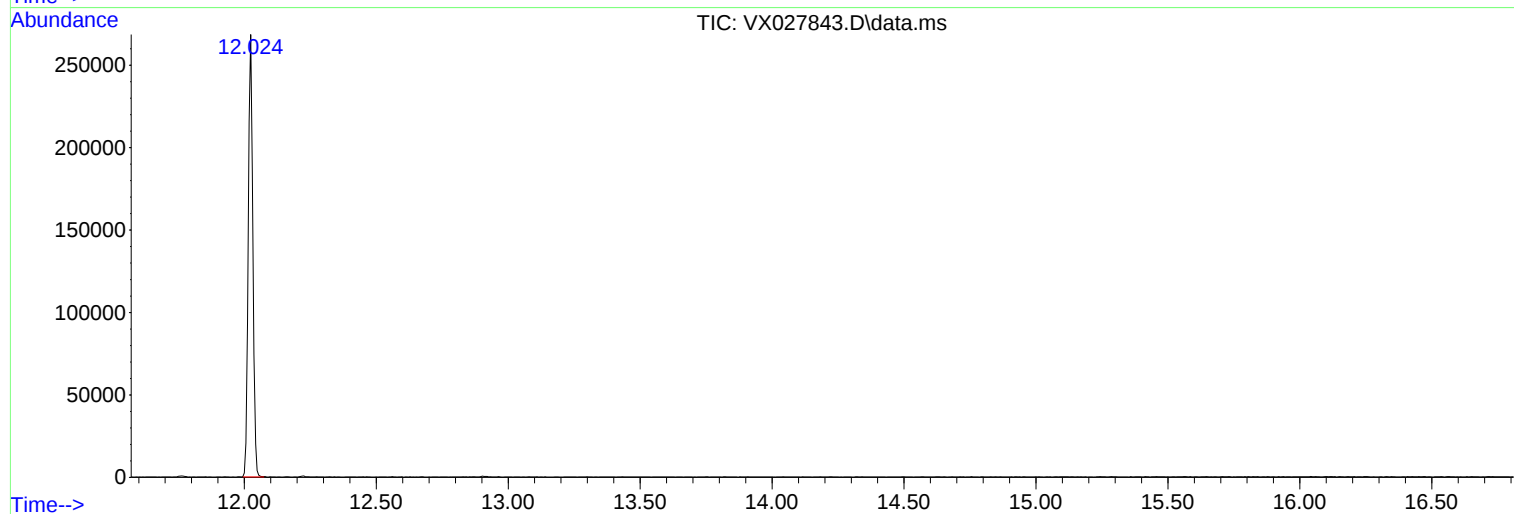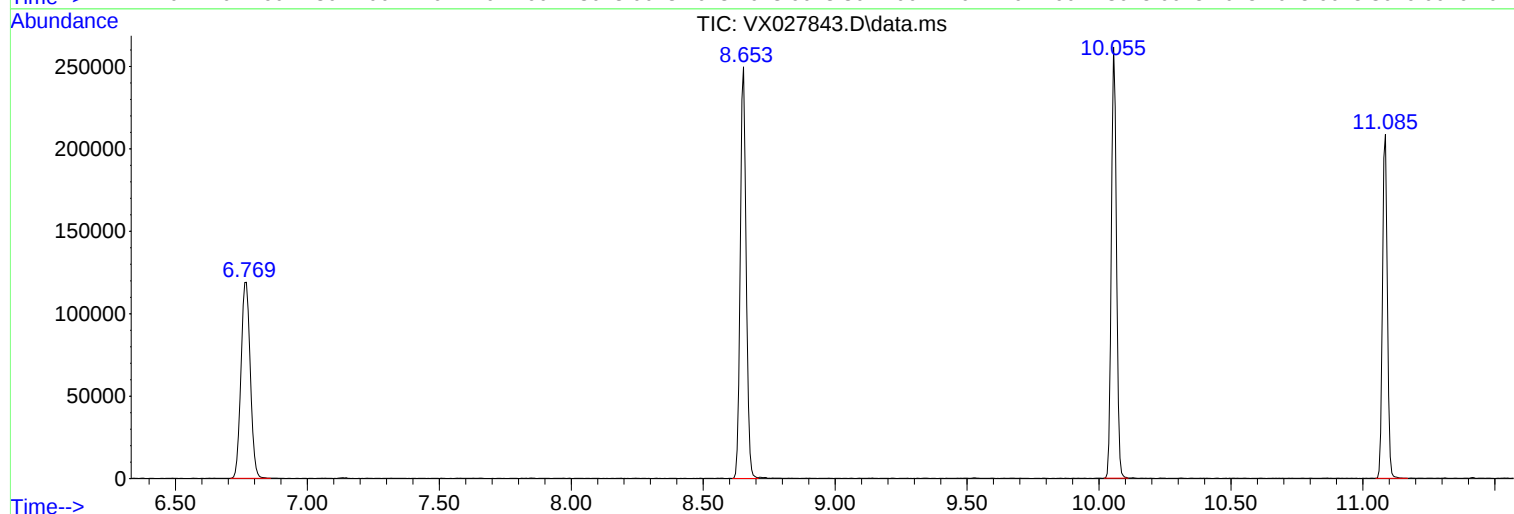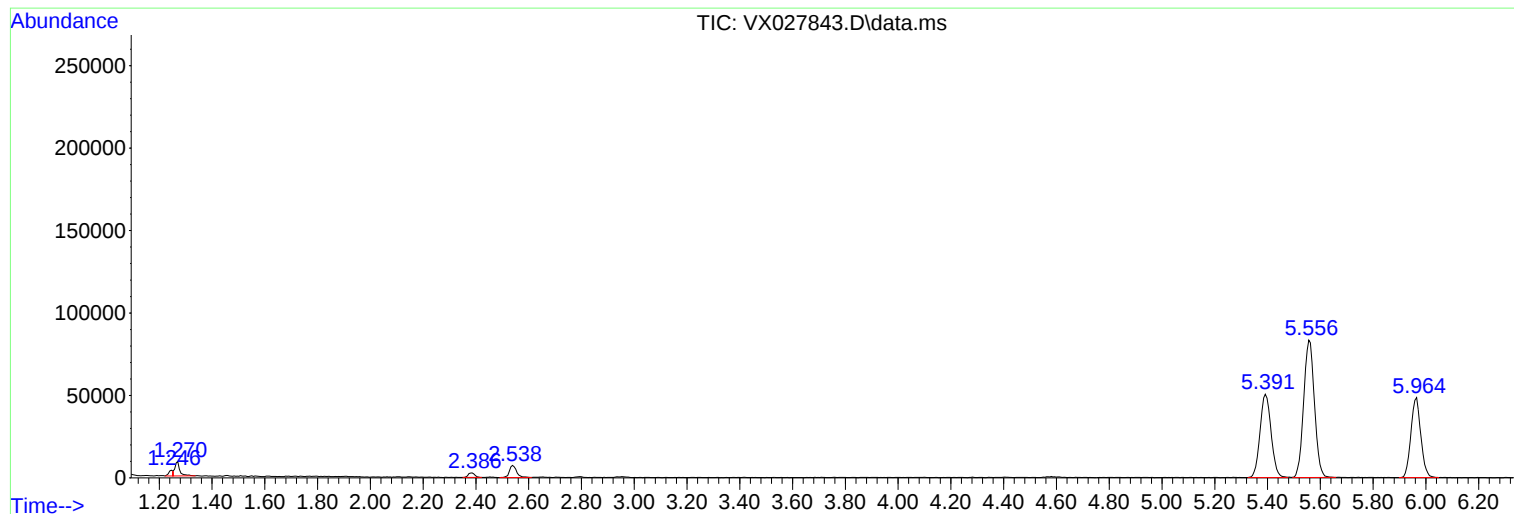

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX033122\
Data File : VX027843.D
Acq On : 31 Mar 2022 13:20
Operator : JC/MD
Sample : N2041-23
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FB-01-20220318

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032922W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX033122\
Data File : VX027843.D
Acq On : 31 Mar 2022 13:20
Operator : JC/MD
Sample : N2041-23
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FB-01-20220318

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032922W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc