

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX033122\
 Data File : VX027853.D
 Acq On : 31 Mar 2022 17:17
 Operator : JC/MD
 Sample : N2074-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TT180D-20220318

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032922W.M

Title : SW846 8260

Signal : TIC: VX027853.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	22	26	38	rBV2	4046	8699	2.08%	0.384%
2	2.538	234	238	243	rBV	3679	6552	1.56%	0.289%
3	5.391	694	706	718	rBV	50848	146336	34.92%	6.458%
4	5.556	722	733	747	rVV	81615	227917	54.39%	10.058%
5	5.958	790	799	811	rBV	52976	134919	32.19%	5.954%
6	6.763	922	931	944	rBV	133003	315673	75.33%	13.931%
7	7.135	985	992	999	rVB3	6079	13368	3.19%	0.590%
8	8.653	1234	1241	1251	rBV	271838	419080	100.00%	18.494%
9	10.055	1465	1471	1482	rBV	288465	381149	90.95%	16.820%
10	11.085	1634	1640	1651	rBV	217091	284475	67.88%	12.554%
11	12.024	1789	1794	1802	rBV	269792	327838	78.23%	14.468%




Sum of corrected areas: 2266006

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX033122\
Data File : VX027853.D
Acq On : 31 Mar 2022 17:17
Operator : JC/MD
Sample : N2074-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TT180D-20220318

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032922W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

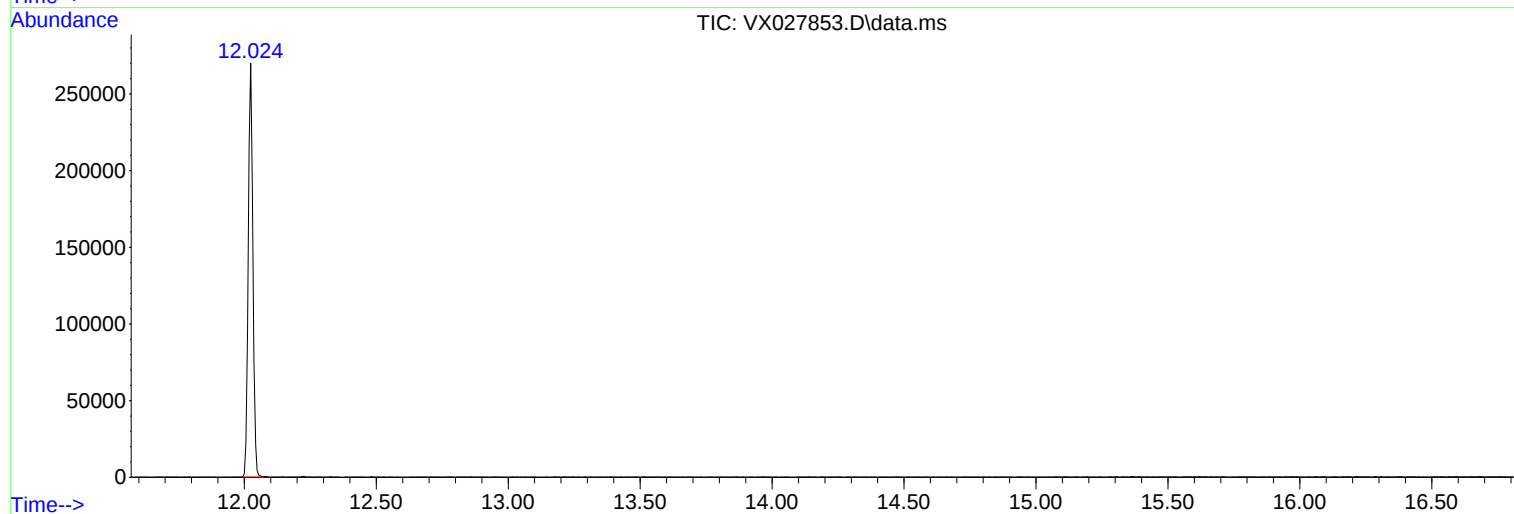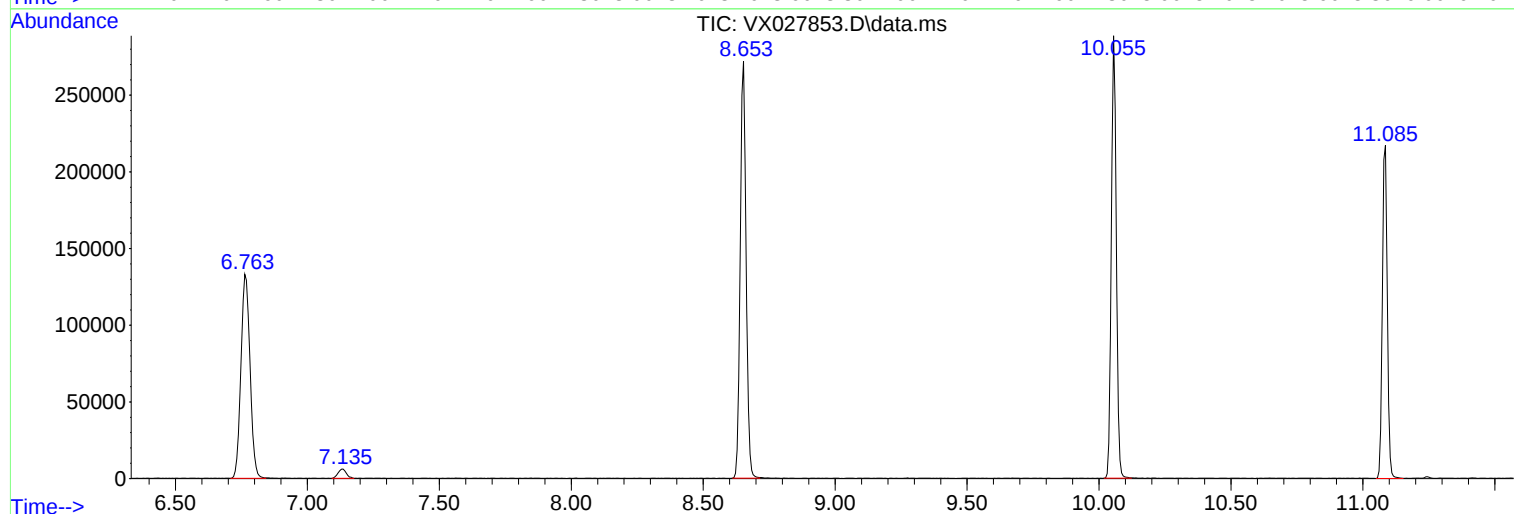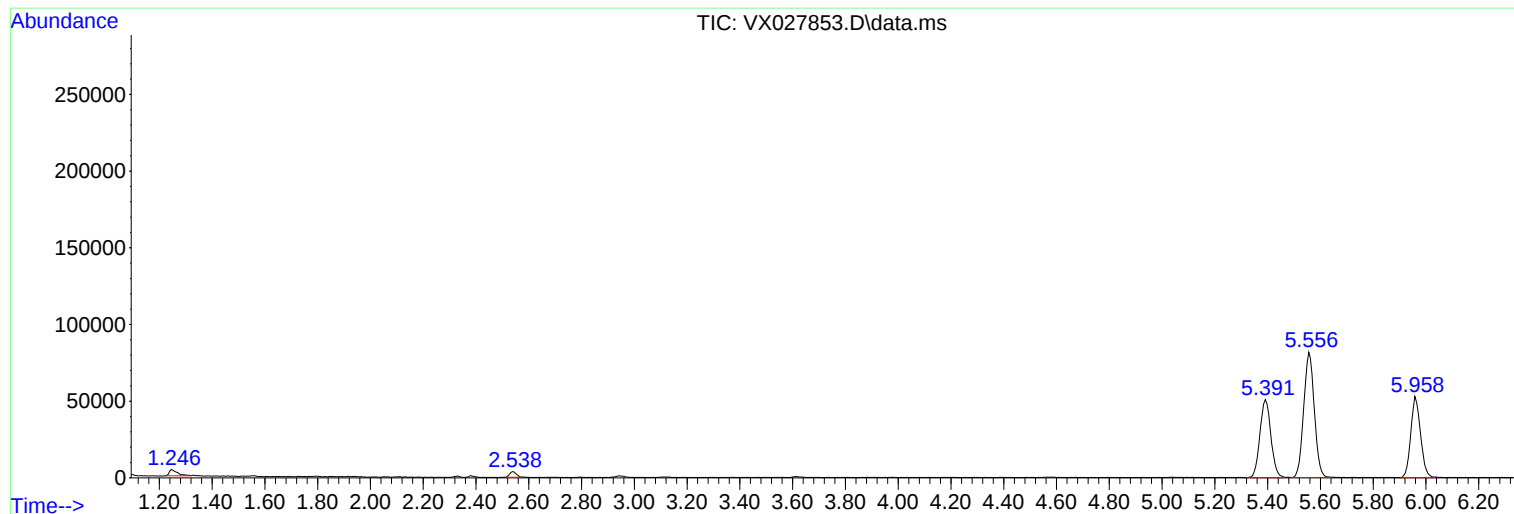

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX033122\
Data File : VX027853.D
Acq On : 31 Mar 2022 17:17
Operator : JC/MD
Sample : N2074-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TT180D-20220318

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032922W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX033122\
Data File : VX027853.D
Acq On : 31 Mar 2022 17:17
Operator : JC/MD
Sample : N2074-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TT180D-20220318

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032922W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------