

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX033122\
 Data File : VX027854.D
 Acq On : 31 Mar 2022 17:40
 Operator : JC/MD
 Sample : N2074-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 RE131D1-20220319

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032922W.M
 Title : SW846 8260

Signal : TIC: VX027854.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.495	551	559	568	rBV4	5499	14747	1.16%	0.400%
2	5.391	695	706	719	rBV2	52750	153049	12.02%	4.156%
3	5.556	722	733	749	rVV2	83119	240221	18.86%	6.523%
4	5.964	789	800	813	rBV	53943	147283	11.56%	3.999%
5	6.763	921	931	944	rBV	131265	313997	24.65%	8.527%
6	7.129	982	991	1013	rBV	602842	1273570	100.00%	34.584%
7	8.653	1234	1241	1251	rBV	274570	427400	33.56%	11.606%
8	9.275	1335	1343	1351	rBV	75138	107022	8.40%	2.906%
9	10.055	1465	1471	1479	rBV	282363	381704	29.97%	10.365%
10	11.085	1634	1640	1649	rVB	221607	287352	22.56%	7.803%
11	12.024	1789	1794	1805	rVB	274487	336210	26.40%	9.130%




Sum of corrected areas: 3682555

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX033122\
Data File : VX027854.D
Acq On : 31 Mar 2022 17:40
Operator : JC/MD
Sample : N2074-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE131D1-20220319

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032922W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

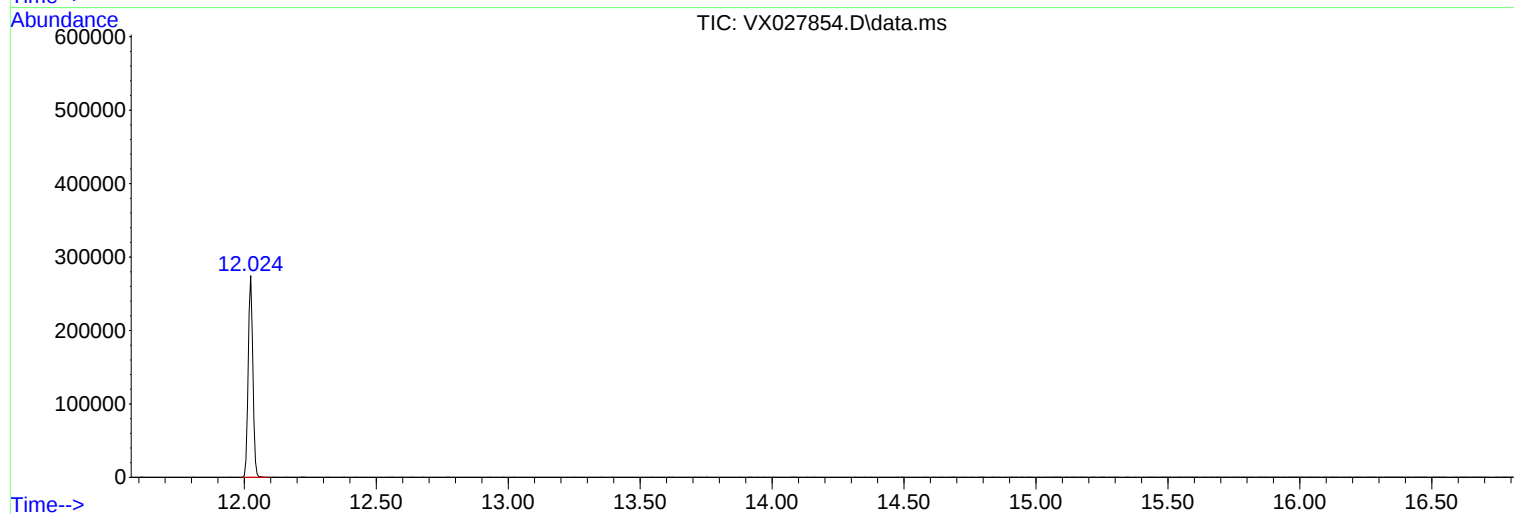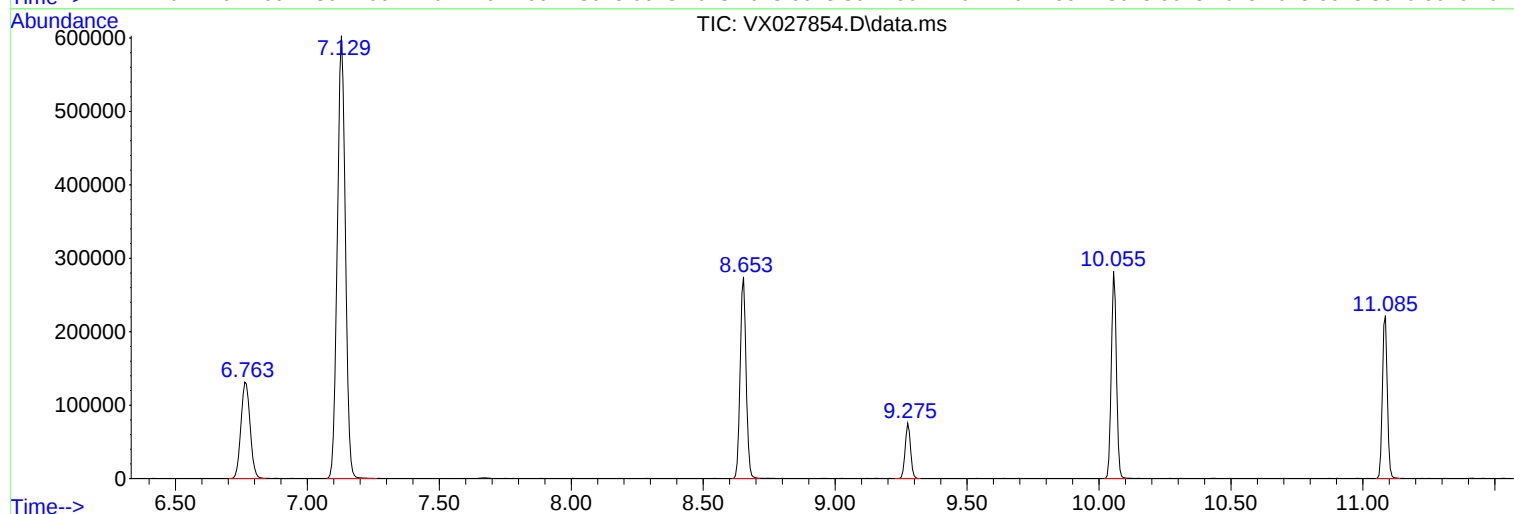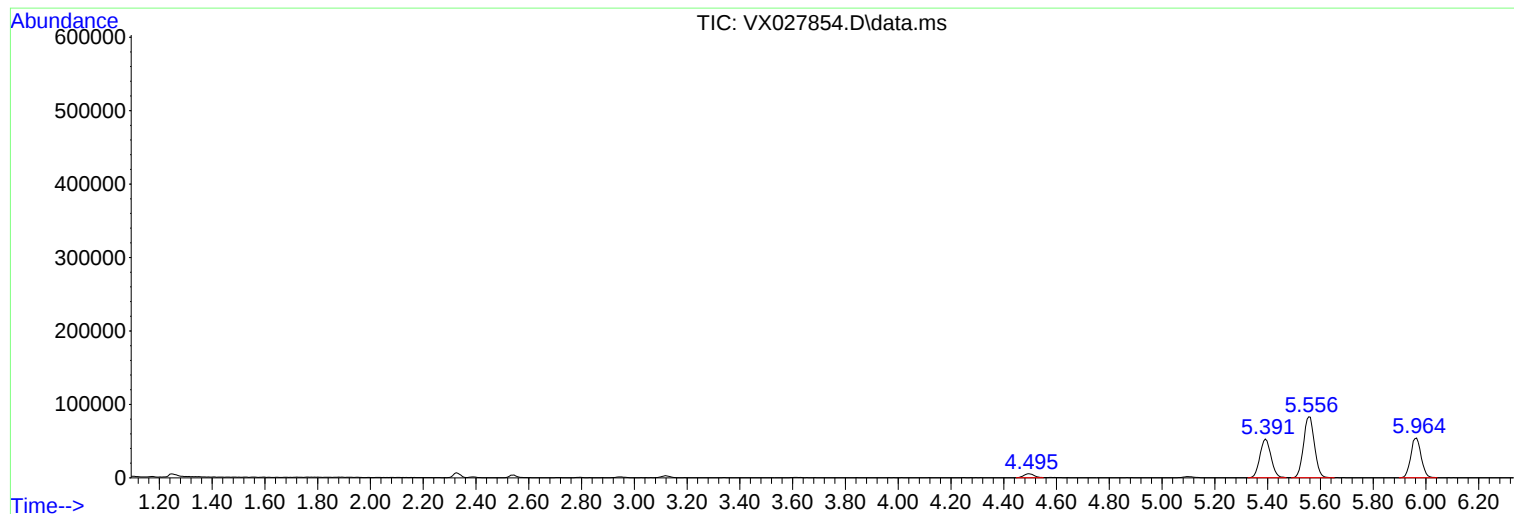

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX033122\
Data File : VX027854.D
Acq On : 31 Mar 2022 17:40
Operator : JC/MD
Sample : N2074-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE131D1-20220319

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032922W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX033122\
Data File : VX027854.D
Acq On : 31 Mar 2022 17:40
Operator : JC/MD
Sample : N2074-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE131D1-20220319

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032922W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
