

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX033122\
 Data File : VX027870.D
 Acq On : 01 Apr 2022 00:49
 Operator : JC/MD
 Sample : N2074-13
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 RE122D3-20220321

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032922W.M

Title : SW846 8260

Signal : TIC: VX027870.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	22	26	32	rBV	3943	8131	1.84%	0.335%
2	2.538	230	238	246	rBV	6550	11838	2.68%	0.488%
3	5.391	695	706	721	rBV2	53394	155954	35.35%	6.423%
4	5.556	721	733	750	rVB2	88394	249802	56.61%	10.288%
5	5.958	788	799	813	rBV	60231	162732	36.88%	6.702%
6	6.763	920	931	946	rBV	140648	334921	75.91%	13.794%
7	7.129	985	991	999	rVB2	5094	10365	2.35%	0.427%
8	8.653	1233	1241	1250	rBV	281491	441230	100.00%	18.173%
9	10.055	1465	1471	1484	rBV	291426	397613	90.11%	16.376%
10	11.079	1634	1639	1649	rBV	229122	303241	68.73%	12.489%
11	12.024	1789	1794	1802	rBV	296485	352162	79.81%	14.504%




Sum of corrected areas: 2427989

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX033122\
Data File : VX027870.D
Acq On : 01 Apr 2022 00:49
Operator : JC/MD
Sample : N2074-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE122D3-20220321

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032922W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

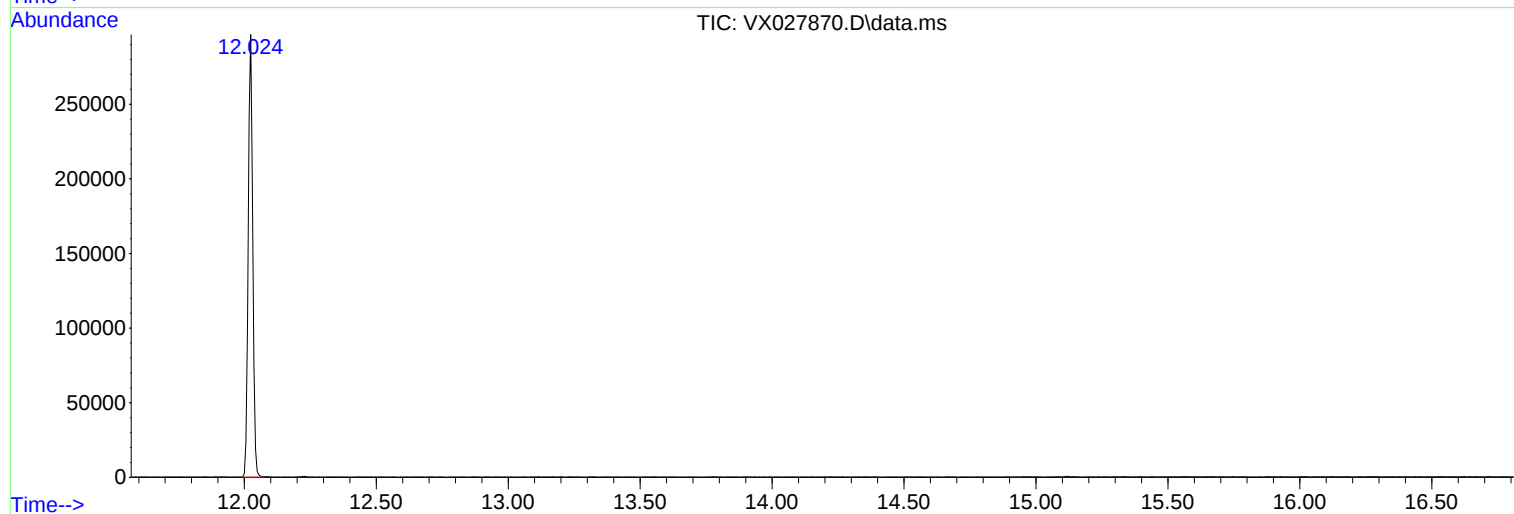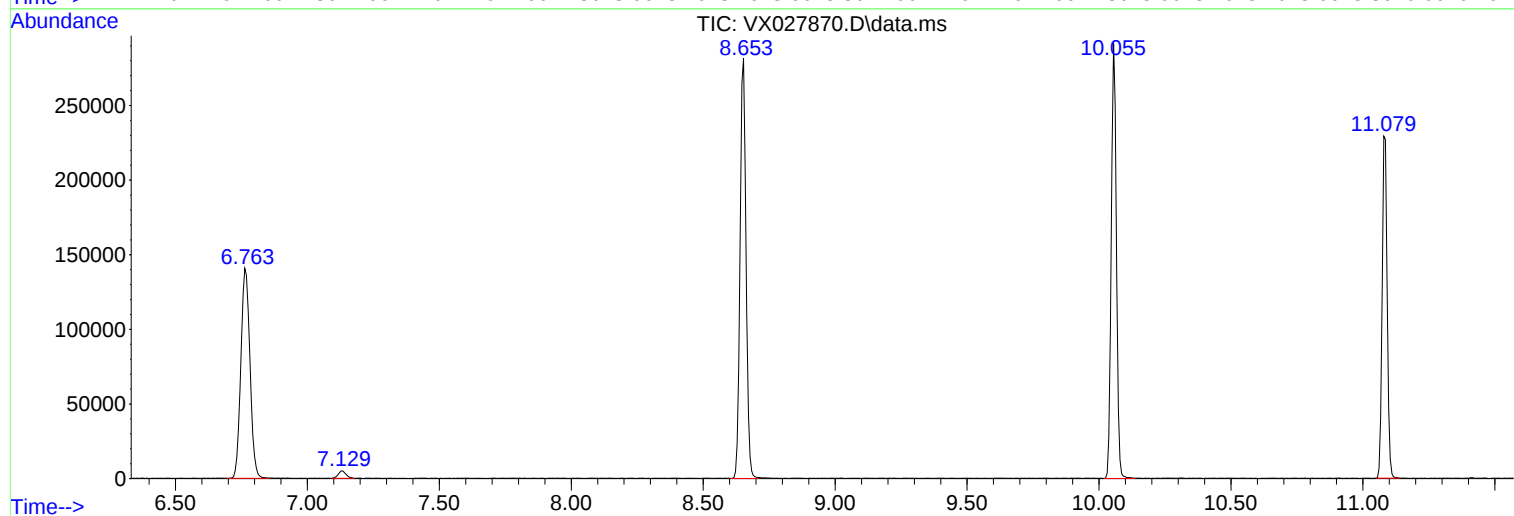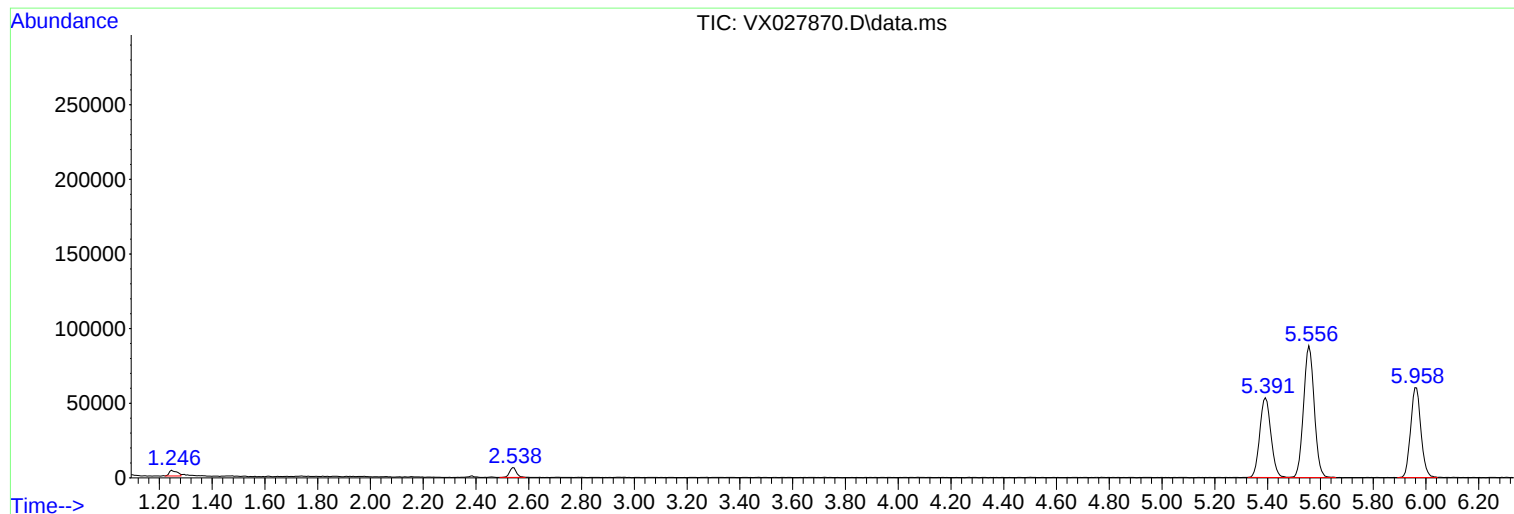

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX033122\
Data File : VX027870.D
Acq On : 01 Apr 2022 00:49
Operator : JC/MD
Sample : N2074-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE122D3-20220321

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032922W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX033122\
Data File : VX027870.D
Acq On : 01 Apr 2022 00:49
Operator : JC/MD
Sample : N2074-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE122D3-20220321

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032922W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------