


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX033122\
 Data File : VX027864.D
 Acq On : 31 Mar 2022 21:59
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032922W.M
 Title : SW846 8260
 Last Update : Wed Mar 30 04:39:27 2022

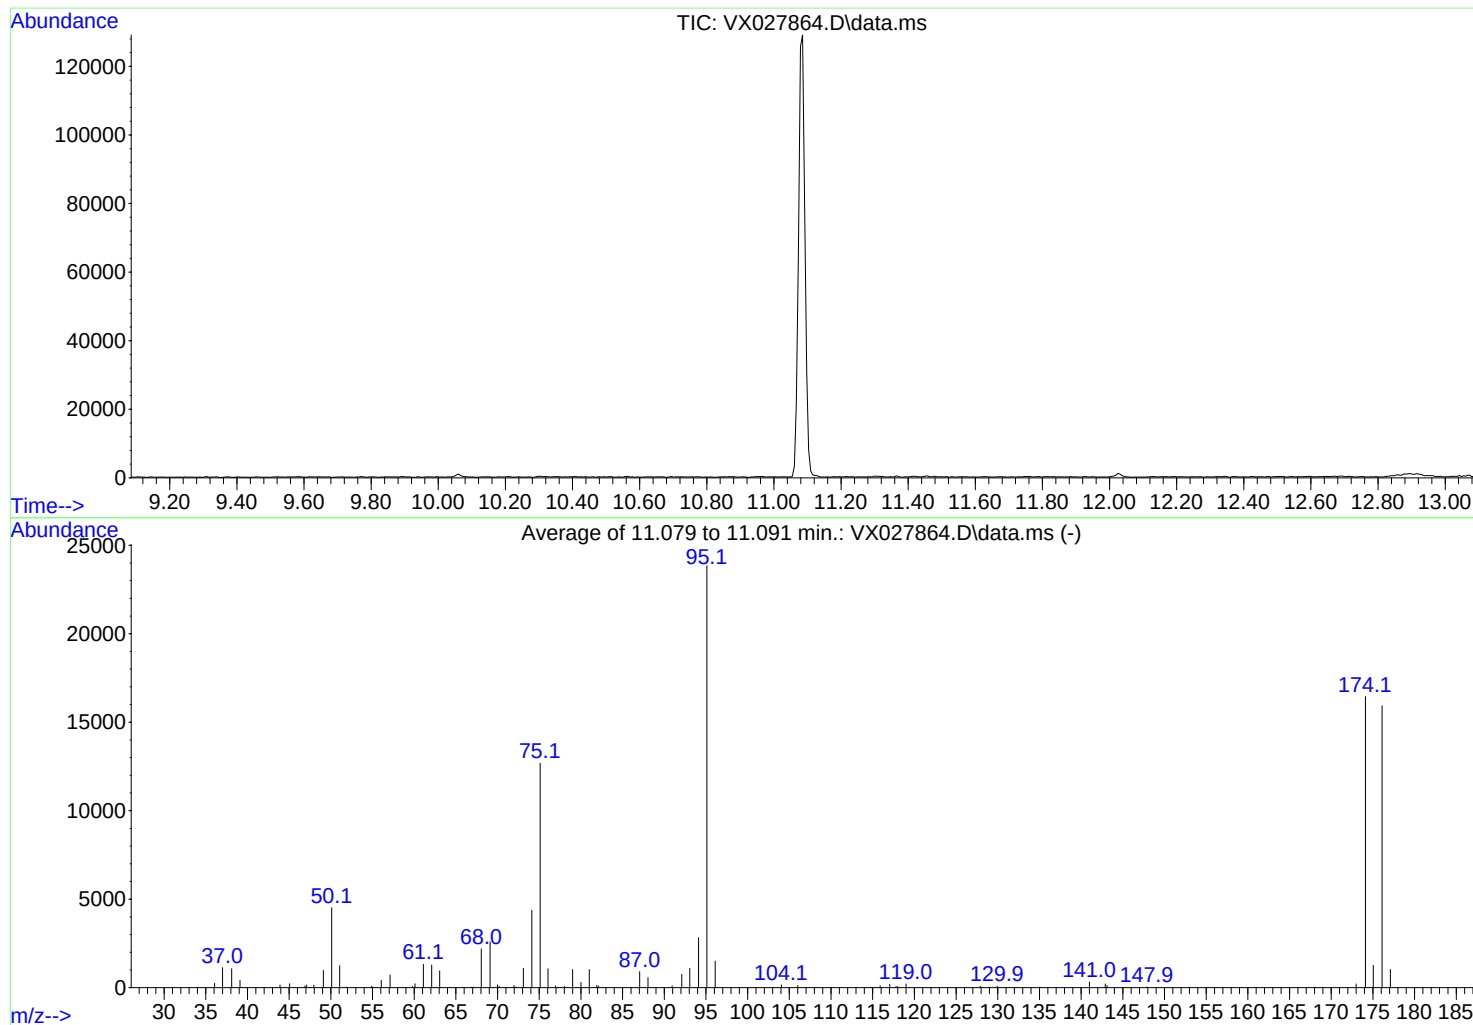

AutoFind: Scans 1639, 1640, 1641; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.9	4516	PASS
75	95	30	60	53.2	12690	PASS
95	95	100	100	100.0	23836	PASS
96	95	5	9	6.3	1505	PASS
173	174	0.00	2	1.2	204	PASS
174	95	50	100	69.0	16452	PASS
175	174	5	9	7.6	1255	PASS
176	174	95	101	96.9	15935	PASS
177	176	5	9	6.4	1020	PASS