

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX033123\
 Data File : VX034906.D
 Acq On : 01 Apr 2023 06:33
 Operator : JC/MD
 Sample : 02137-13
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TRIP-BLANK-1

Quant Time: Apr 03 02:10:31 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032923W.M
 Quant Title : SW846 8260
 QLast Update : Sat Apr 01 01:50:18 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	266891	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	456884	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	410070	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	180822	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	207177	50.757	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	101.520%
35) Dibromofluoromethane	5.385	113	143904	47.620	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	95.240%
50) Toluene-d8	8.647	98	551877	49.478	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	98.960%
62) 4-Bromofluorobenzene	11.079	95	209760	48.597	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	97.200%


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX033123\
Data File : VX034906.D
Acq On : 01 Apr 2023 06:33
Operator : JC/MD
Sample : 02137-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TRIP-BLANK-1

Quant Time: Apr 03 02:10:31 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032923W.M
Quant Title : SW846 8260
QLast Update : Sat Apr 01 01:50:18 2023
Response via : Initial Calibration




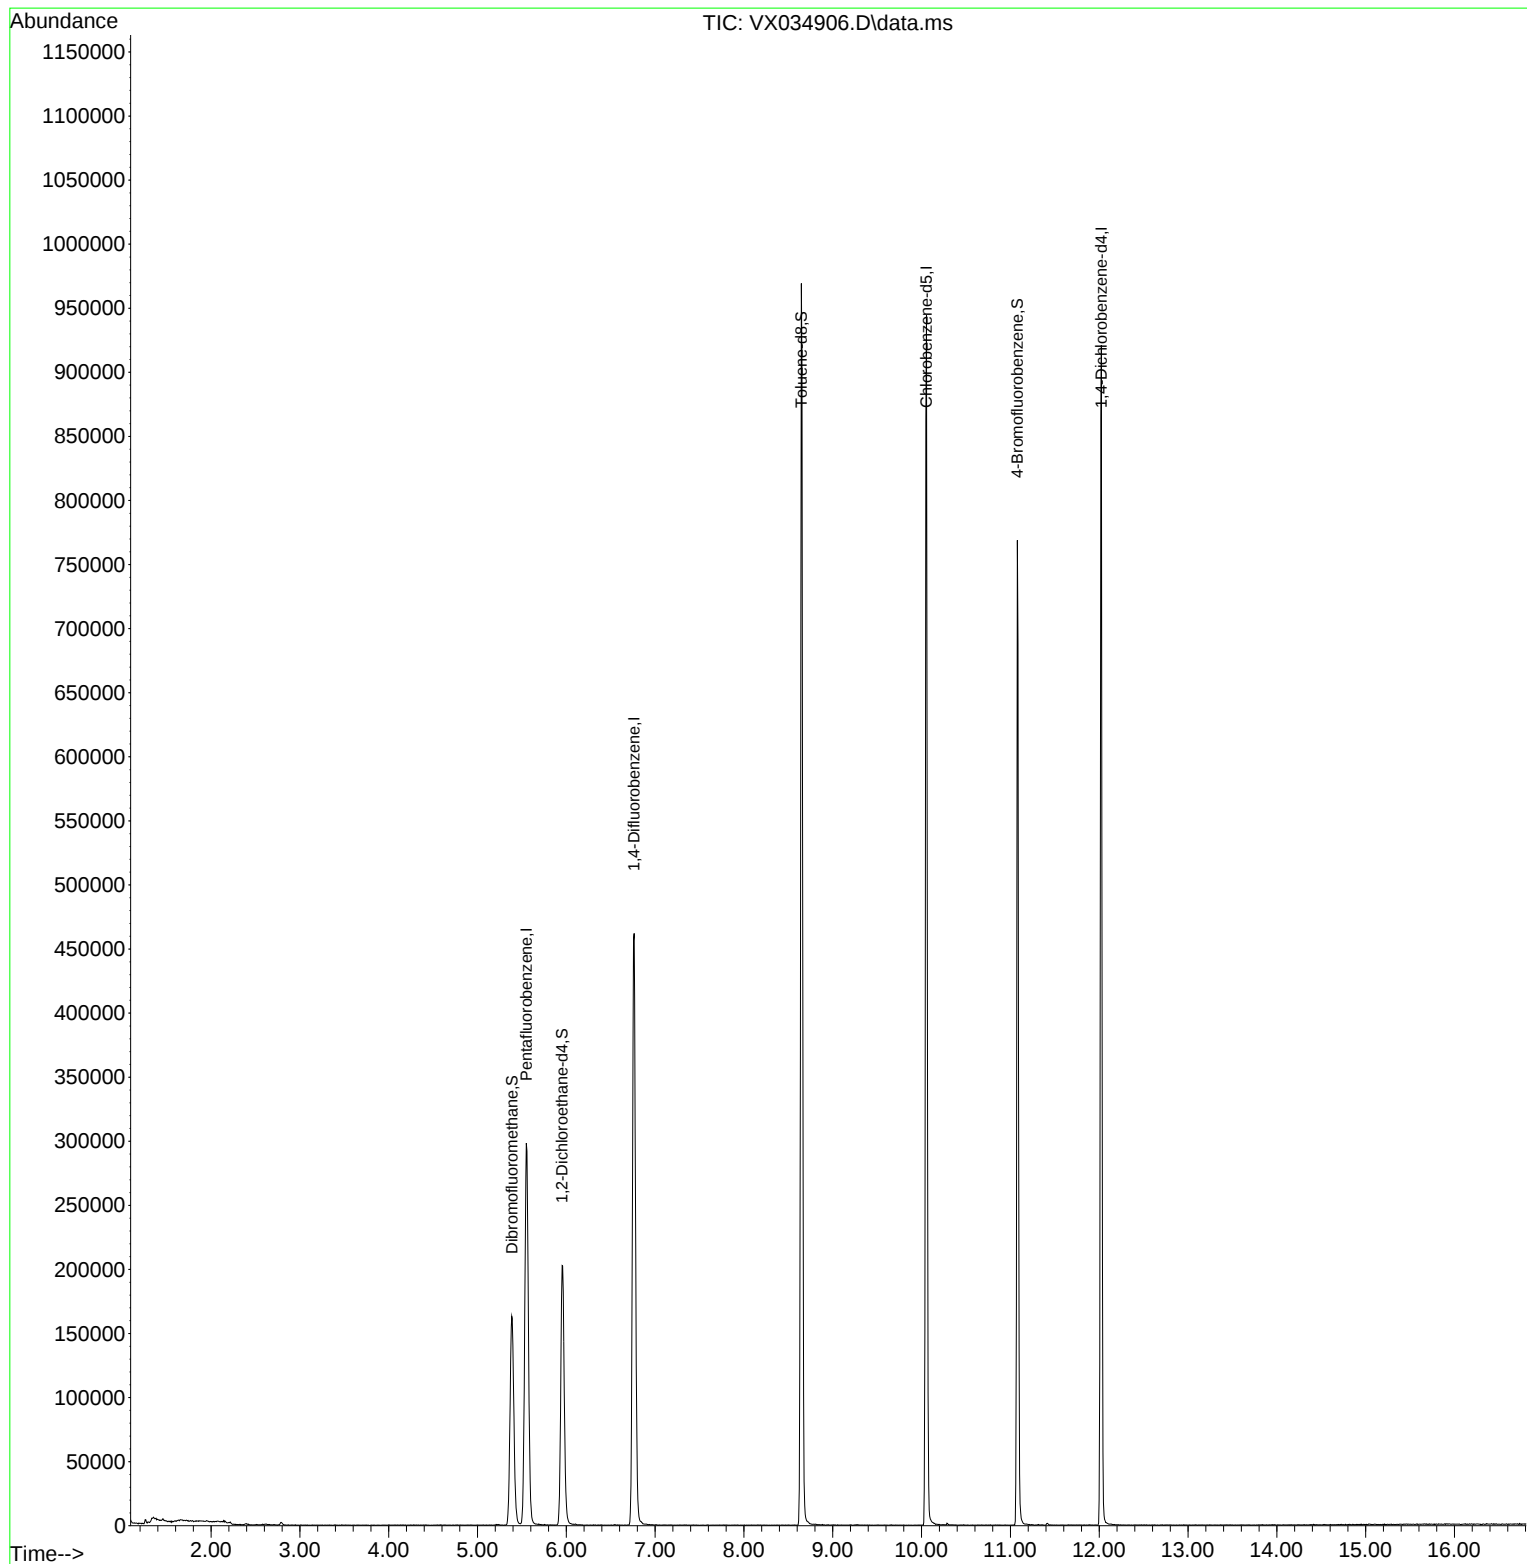




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX034906.D
Acq: 01 Apr 2023 06:33




Instrument :
MSVOA_X
ClientSampleId :
TRIP-BLANK-1


Tgt Ion:168 Resp: 266891
Ion Ratio Lower Upper
168 100
99 64.6 45.7 68.5

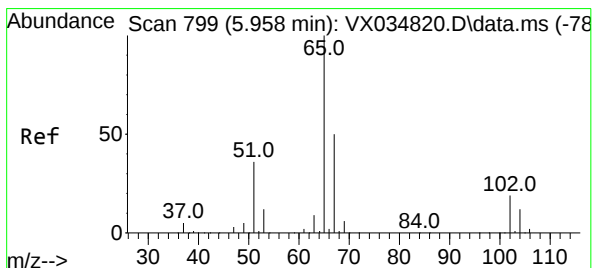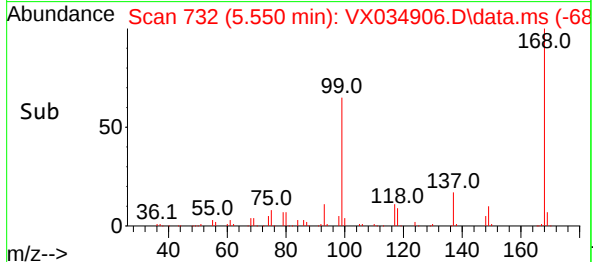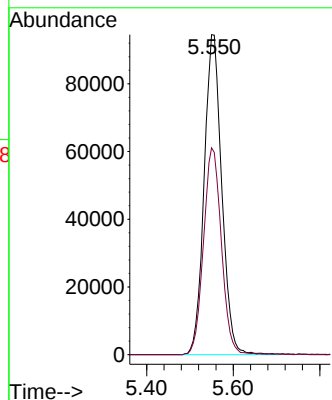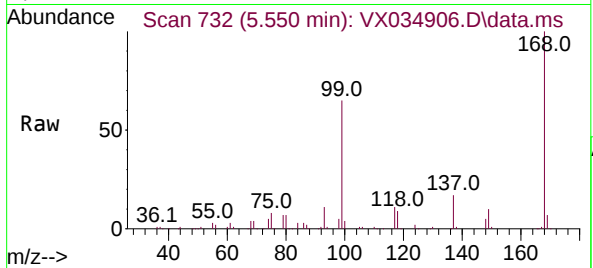

#33
1,2-Dichloroethane-d4
Concen: 50.757 ug/l
RT: 5.952 min Scan# 798
Delta R.T. -0.006 min
Lab File: VX034906.D
Acq: 01 Apr 2023 06:33

Tgt Ion: 65 Resp: 207177
Ion Ratio Lower Upper
65 100
67 50.1 0.0 104.0


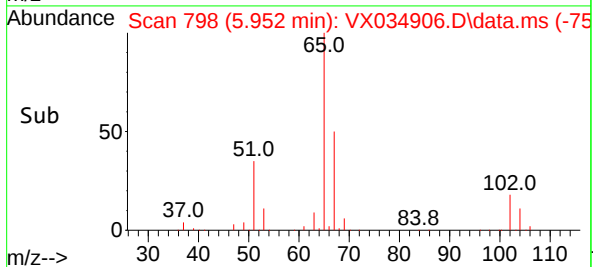
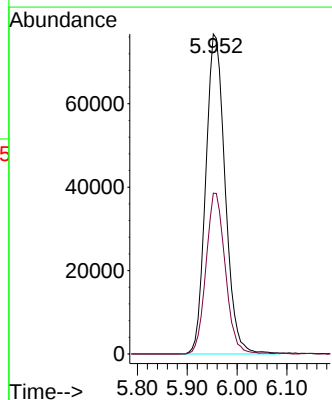
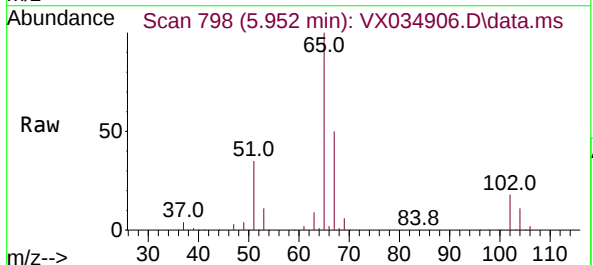


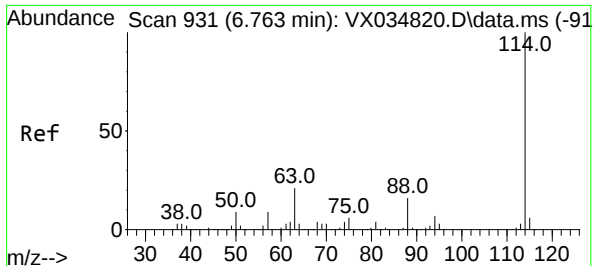

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 911
Delta R.T. 0.000 min
Lab File: VX034906.D
Acq: 01 Apr 2023 06:33




Instrument :
MSVOA_X
ClientSampleId :
TRIP-BLANK-1


Tgt Ion:114 Resp: 456884
Ion Ratio Lower Upper
114 100
63 23.0 0.0 42.2
88 17.2 0.0 33.2

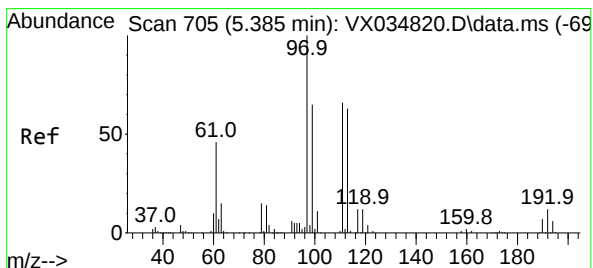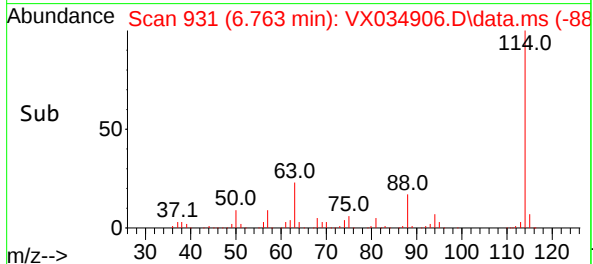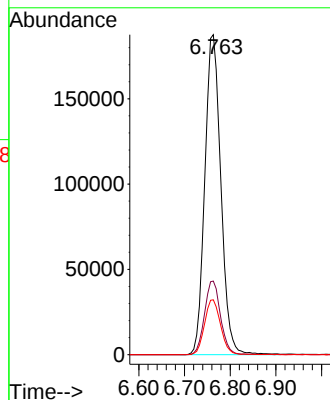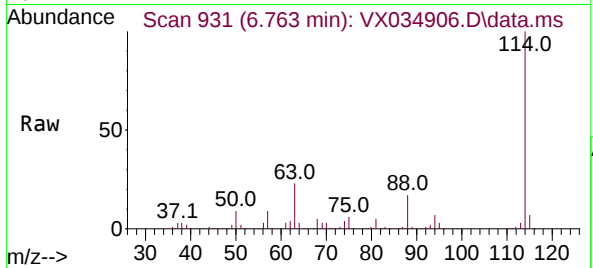

#35
Dibromofluoromethane
Concen: 47.620 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.000 min
Lab File: VX034906.D
Acq: 01 Apr 2023 06:33

Tgt Ion:113 Resp: 143904
Ion Ratio Lower Upper
113 100
111 102.6 83.7 125.5
192 18.6 15.4 23.2


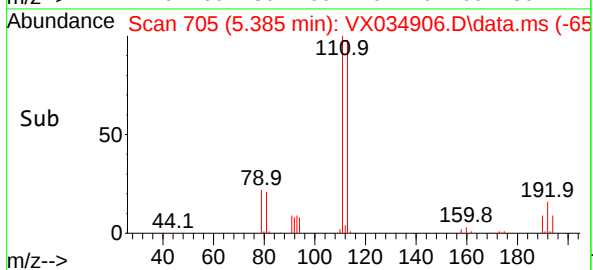
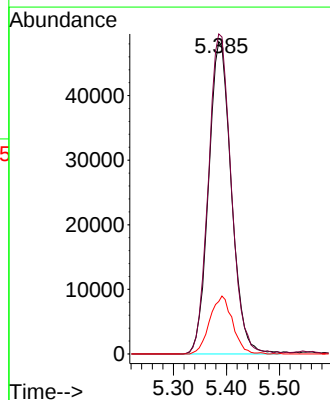
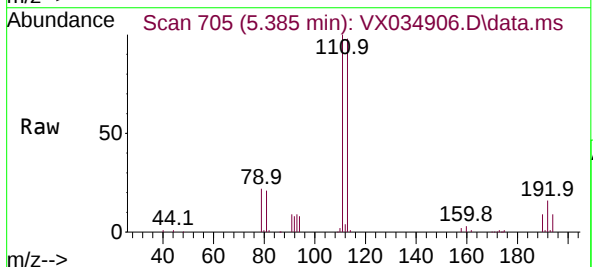


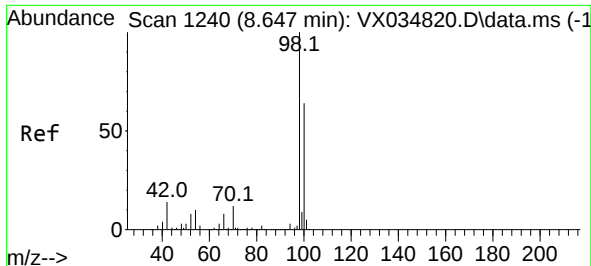

#50
Toluene-d8
Concen: 49.478 ug/l
RT: 8.647 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX034906.D
Acq: 01 Apr 2023 06:33




Instrument :
MSVOA_X
ClientSampleId :
TRIP-BLANK-1


Tgt Ion: 98 Resp: 551877
Ion Ratio Lower Upper
98 100
100 66.3 52.5 78.7

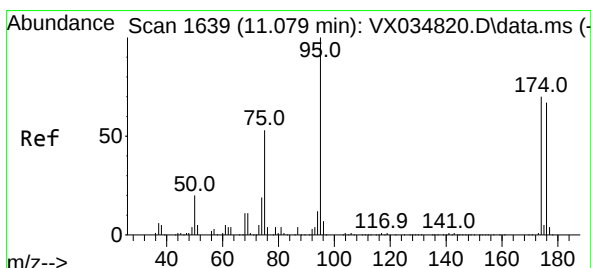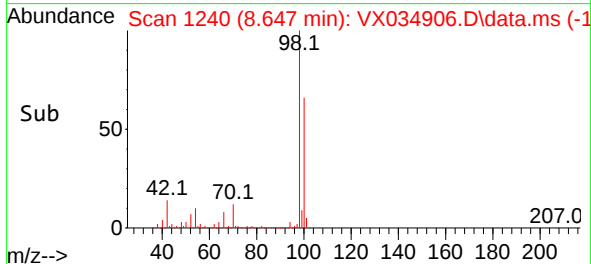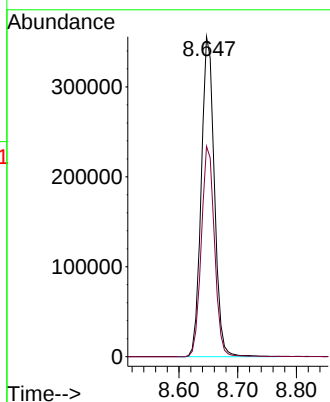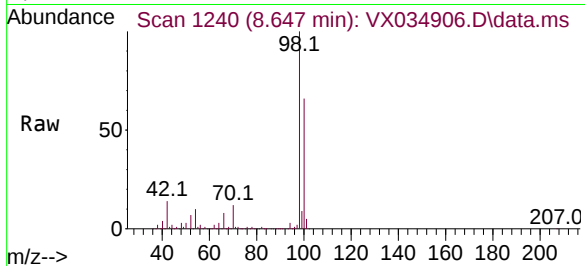

#62
4-Bromofluorobenzene
Concen: 48.597 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX034906.D
Acq: 01 Apr 2023 06:33

Tgt Ion: 95 Resp: 209760
Ion Ratio Lower Upper
95 100
174 70.3 0.0 147.4
176 68.3 0.0 140.6


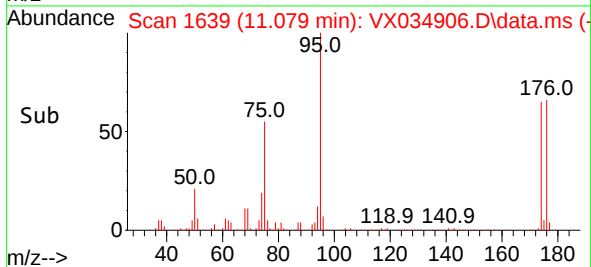
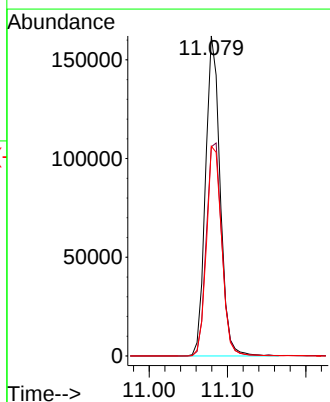
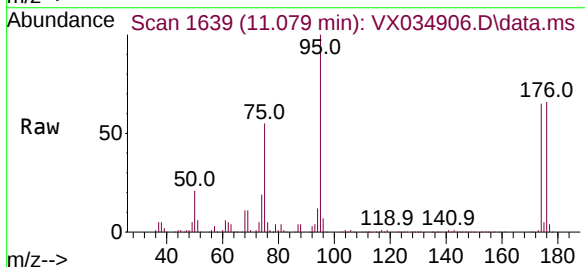


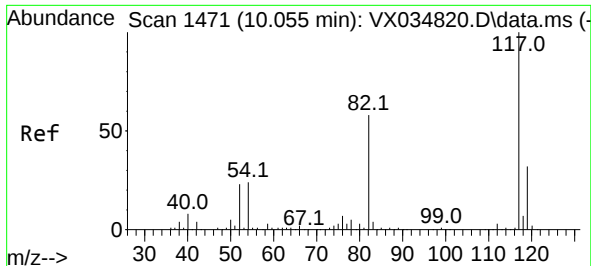

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX034906.D
Acq: 01 Apr 2023 06:33

Instrument :
MSVOA_X
ClientSampleId :
TRIP-BLANK-1

Tgt Ion:117 Resp: 410070
Ion Ratio Lower Upper
117 100
82 59.0 45.0 67.4
119 31.9 26.0 39.0

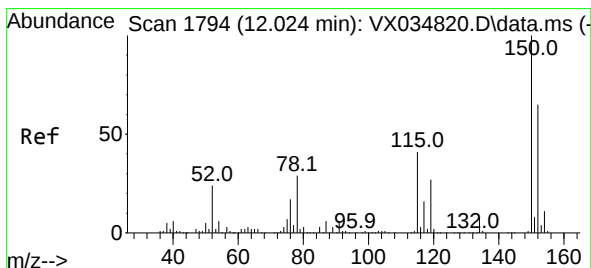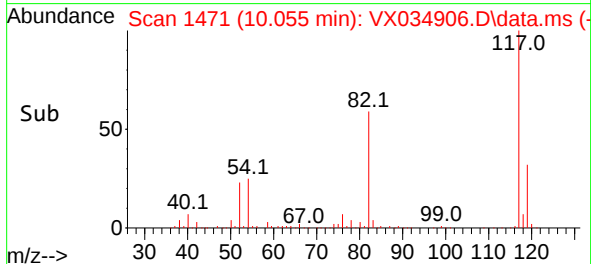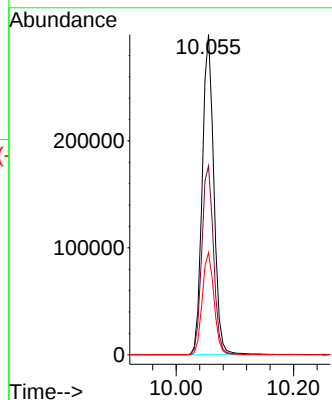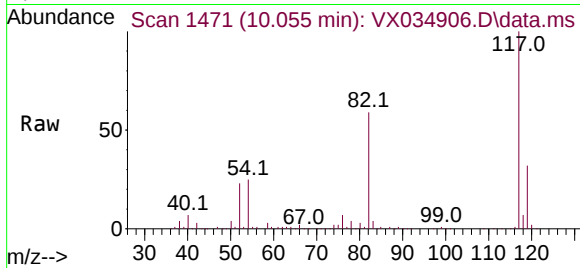

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX034906.D
Acq: 01 Apr 2023 06:33

Tgt Ion:152 Resp: 180822
Ion Ratio Lower Upper
152 100
115 64.4 45.0 135.0
150 158.4 0.0 352.4

