

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX033123\
 Data File : VX034880.D
 Acq On : 31 Mar 2023 15:58
 Operator : JC/MD
 Sample : 02048-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-8

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032923W.M

Title : SW846 8260

Signal : TIC: VX034880.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	6	9	16	rBV	52361	54760	4.42%	0.719%
2	1.270	24	30	40	rBV	682196	827584	66.81%	10.859%
3	1.368	44	46	50	rVB2	9177	13428	1.08%	0.176%
4	3.111	323	332	344	rBV	93276	210633	17.00%	2.764%
5	5.385	694	705	722	rBV2	137966	401459	32.41%	5.268%
6	5.550	722	732	748	rVV	234851	670824	54.15%	8.802%
7	5.958	788	799	821	rBV	169164	449846	36.31%	5.903%
8	6.763	921	931	946	rBV	376739	905684	73.11%	11.884%
9	8.647	1233	1240	1250	rBV	805075	1238775	100.00%	16.254%
10	10.055	1465	1471	1483	rBV	779735	1067192	86.15%	14.003%
11	10.195	1490	1494	1501	rVB2	8782	12511	1.01%	0.164%
12	10.659	1563	1570	1576	rBV3	6241	12903	1.04%	0.169%
13	11.079	1634	1639	1652	rBV	637669	799493	64.54%	10.490%
14	12.018	1788	1793	1803	rBV	731557	956051	77.18%	12.545%




Sum of corrected areas: 7621143

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX033123\
Data File : VX034880.D
Acq On : 31 Mar 2023 15:58
Operator : JC/MD
Sample : 02048-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032923W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

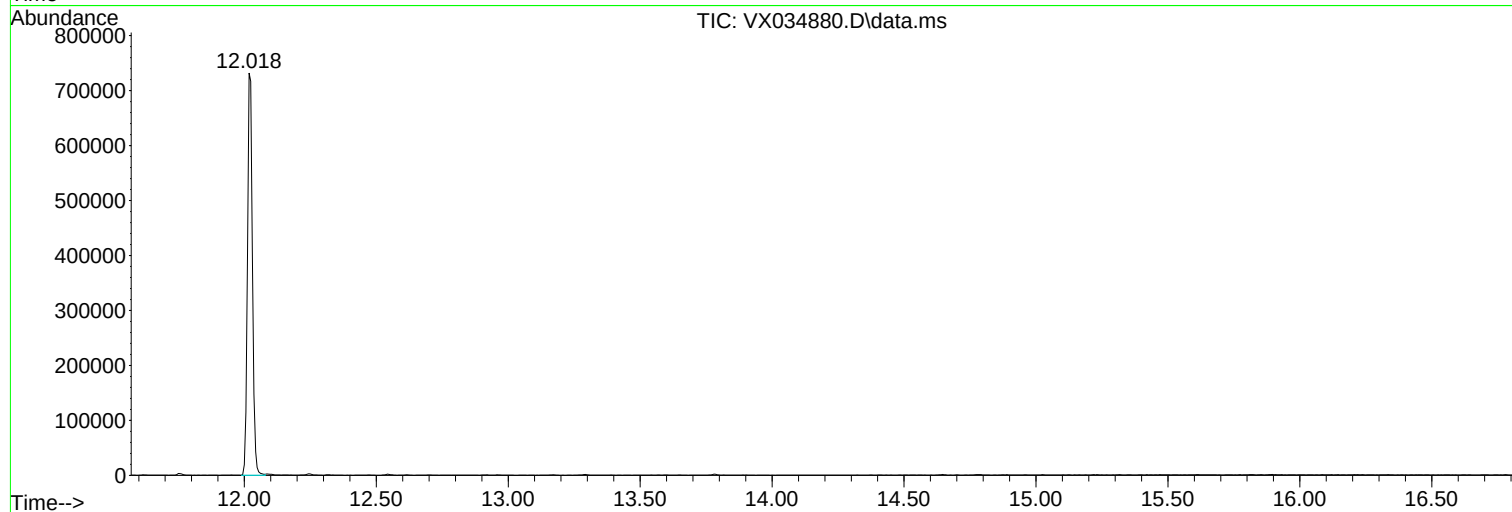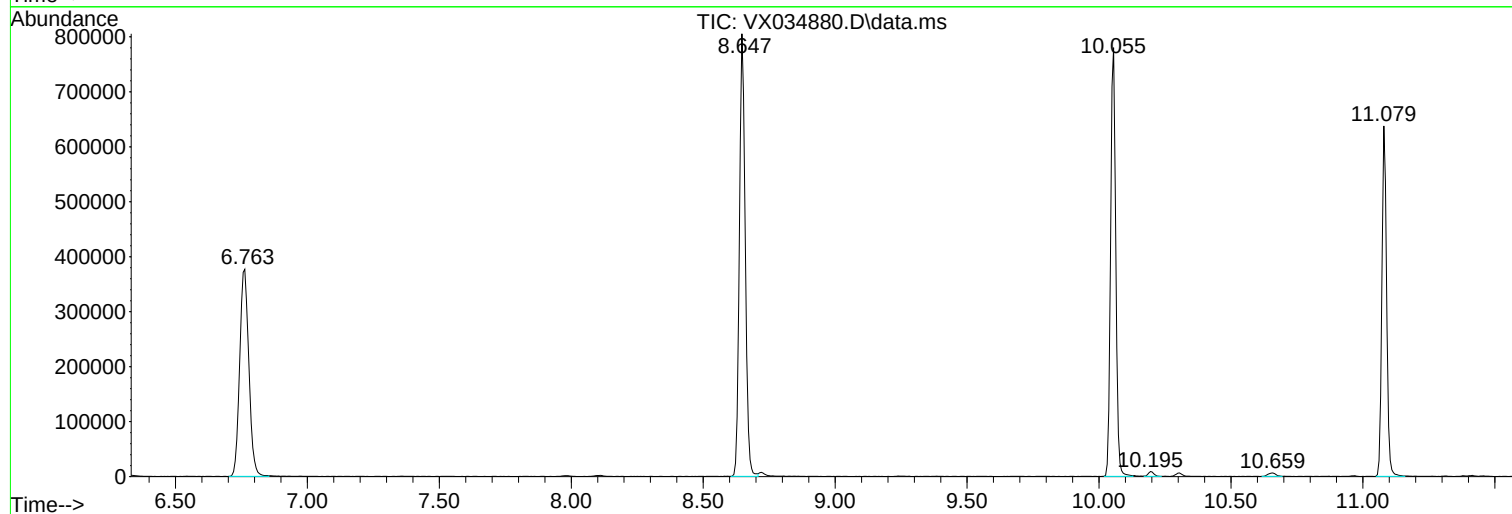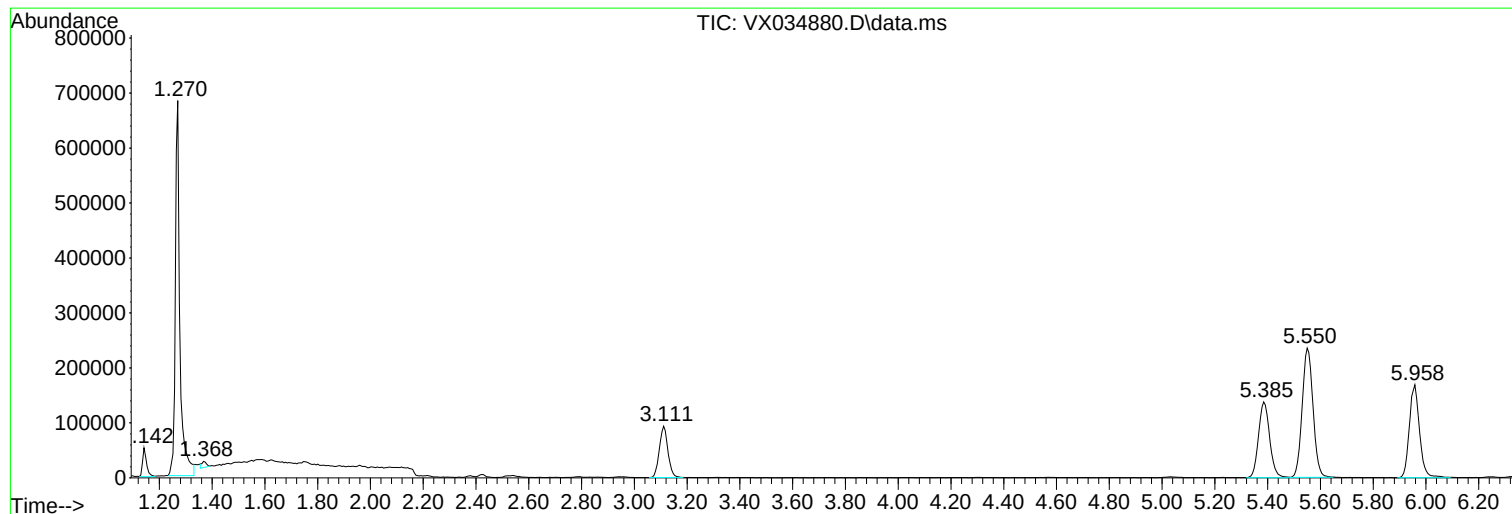

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX033123\
Data File : VX034880.D
Acq On : 31 Mar 2023 15:58
Operator : JC/MD
Sample : 02048-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-8










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032923W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Ethane, 1-chloro-1,1-difluoro- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.270	61.68 ug/l	827584	Pentafluorobenzene	5.550

Hit#	of 4	Tentative ID	MW	MolForm	CAS#	Qual
1		Ethane, 1-chloro-1,1-difluoro-	100	C2H3ClF2	000075-68-3	83
2		Propane, 2,2-difluoro-	80	C3H6F2	000420-45-1	9
3		2,2-Difluoropropionic acid	110	C3H4F2O2	000373-96-6	2
4		Propanoyl chloride	92	C3H5ClO	000079-03-8	1

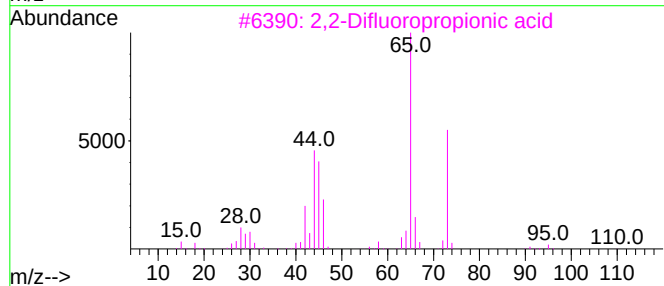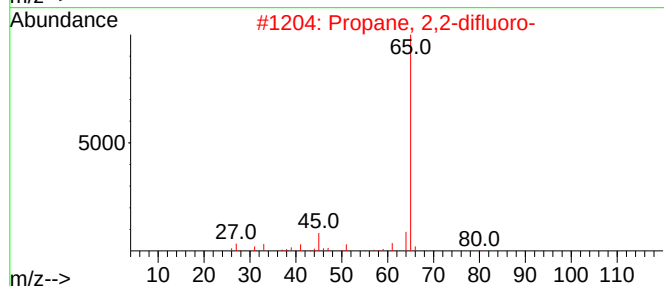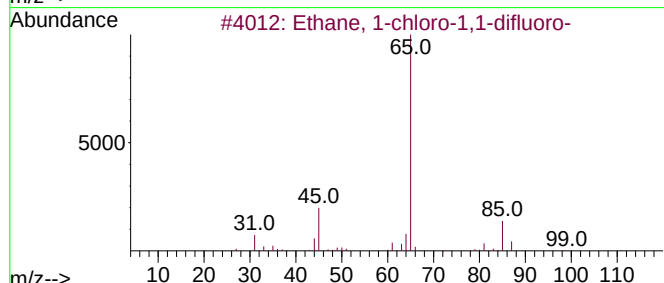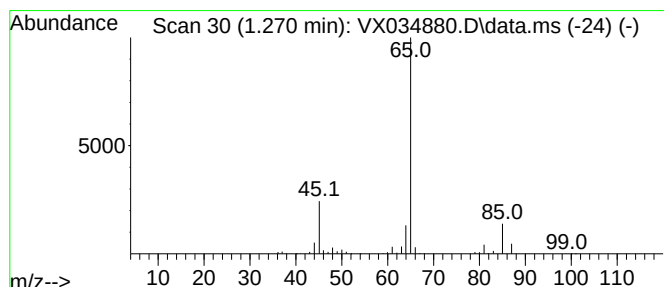

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX033123\
Data File : VX034880.D
Acq On : 31 Mar 2023 15:58
Operator : JC/MD
Sample : 02048-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032923W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Ethane, 1-chlor...	1.270	61.7	ug/l	827584	1	5.550	670824	50.0