

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX033123\  
Data File : VX034899.D  
Acq On : 01 Apr 2023 03:51  
Operator : JC/MD  
Sample : 02140-09  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 41 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
TRIP-BLANK-1

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X032923W.M

Title : SW846 8260

Signal : TIC: VX034899.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.385       | 693           | 705         | 721          | rBV      | 138665         | 400190        | 31.90%          | 5.862%        |
| 2         | 5.550       | 721           | 732         | 749          | rVV      | 236141         | 674775        | 53.79%          | 9.885%        |
| 3         | 5.958       | 787           | 799         | 816          | rBV      | 170228         | 450982        | 35.95%          | 6.606%        |
| 4         | 6.763       | 920           | 931         | 946          | rBV      | 382836         | 918861        | 73.25%          | 13.460%       |
| 5         | 8.647       | 1233          | 1240        | 1259         | rBV      | 806347         | 1254481       | 100.00%         | 18.377%       |
| 6         | 10.055      | 1465          | 1471        | 1483         | rBV      | 837561         | 1161514       | 92.59%          | 17.015%       |
| 7         | 11.079      | 1634          | 1639        | 1652         | rBV      | 673640         | 874285        | 69.69%          | 12.807%       |
| 8         | 12.024      | 1788          | 1794        | 1803         | rBV      | 851917         | 1091350       | 87.00%          | 15.987%       |




Sum of corrected areas: 6826438

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX033123\  
Data File : VX034899.D  
Acq On : 01 Apr 2023 03:51  
Operator : JC/MD  
Sample : 02140-09  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 41 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
TRIP-BLANK-1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X032923W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

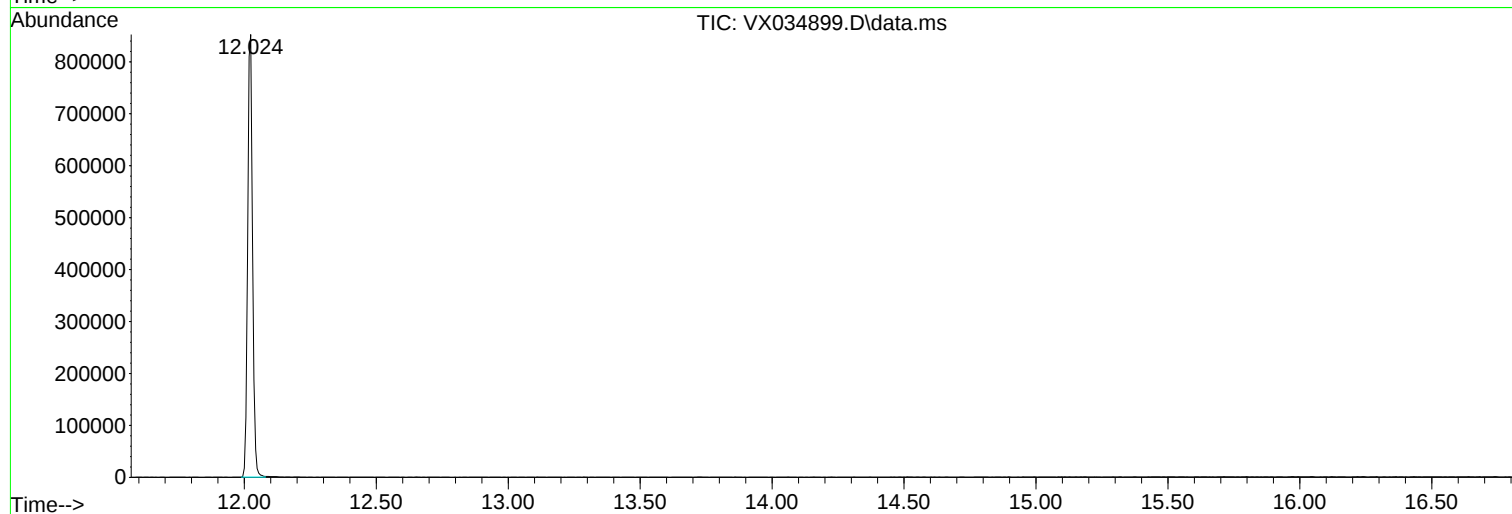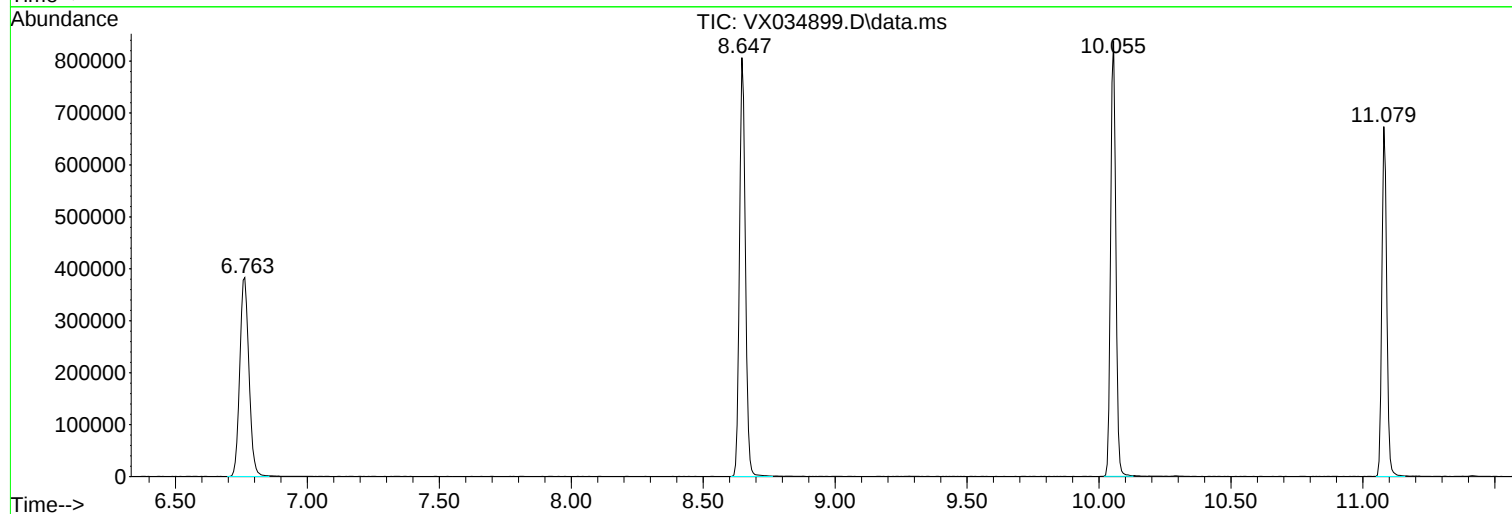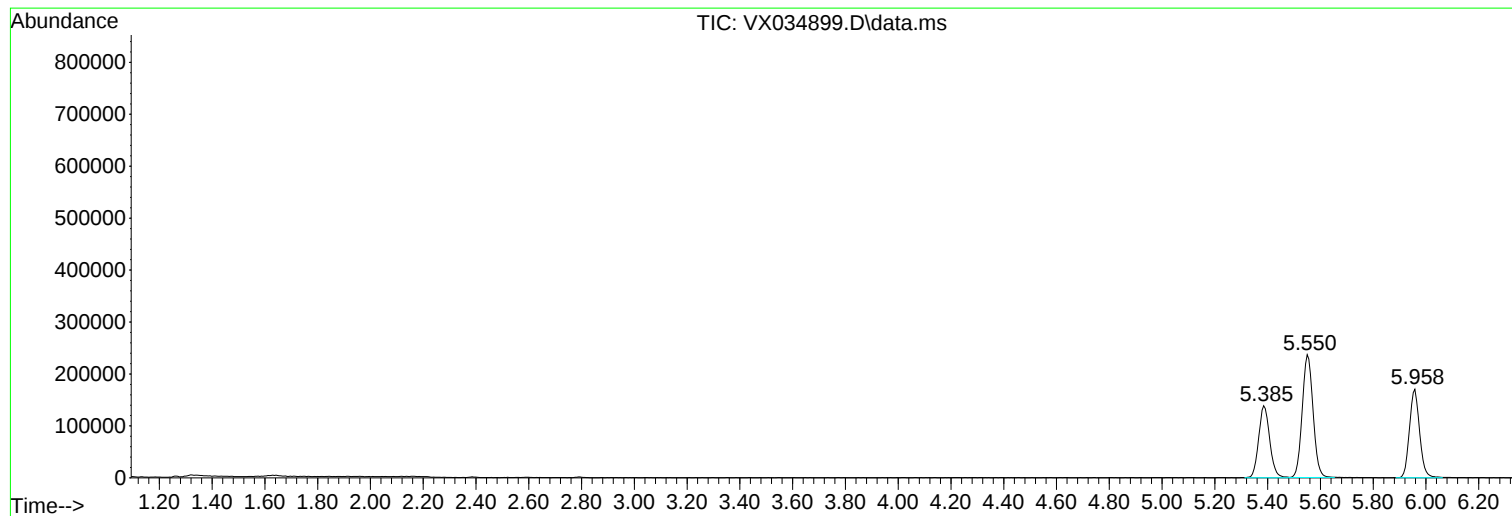

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX033123\  
Data File : VX034899.D  
Acq On : 01 Apr 2023 03:51  
Operator : JC/MD  
Sample : 02140-09  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 41 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
TRIP-BLANK-1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X032923W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX033123\  
Data File : VX034899.D  
Acq On : 01 Apr 2023 03:51  
Operator : JC/MD  
Sample : 02140-09  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 41 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
TRIP-BLANK-1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X032923W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|