
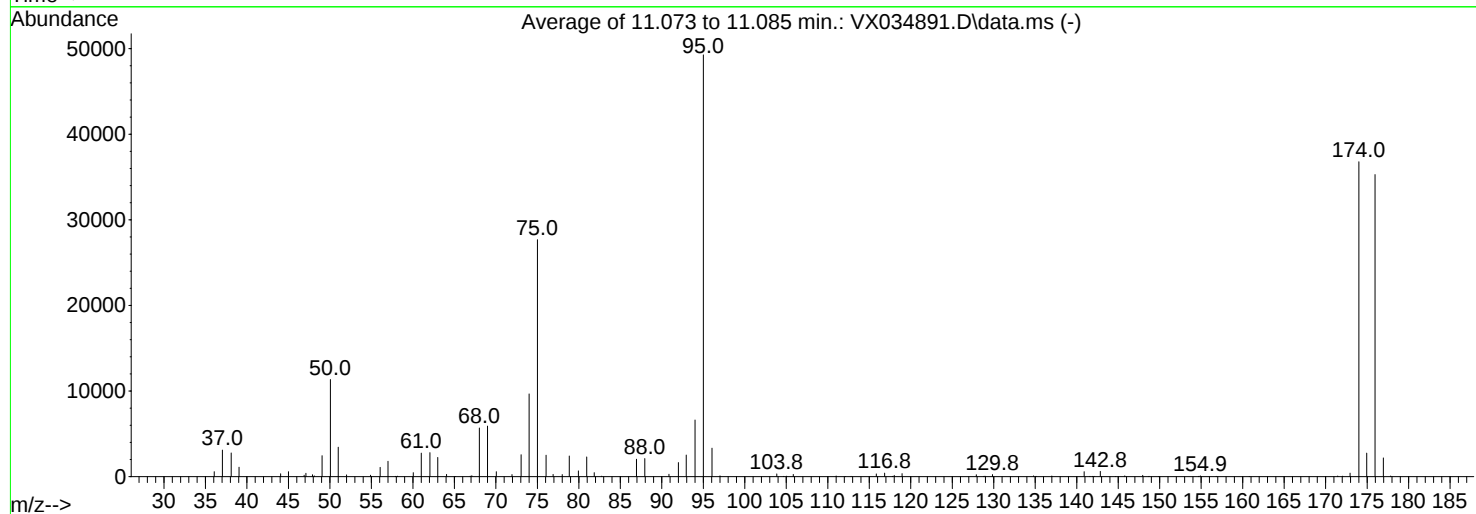


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX033123\
Data File : VX034891.D
Acq On : 31 Mar 2023 23:23
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X032823W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Tue Mar 28 09:11:00 2023

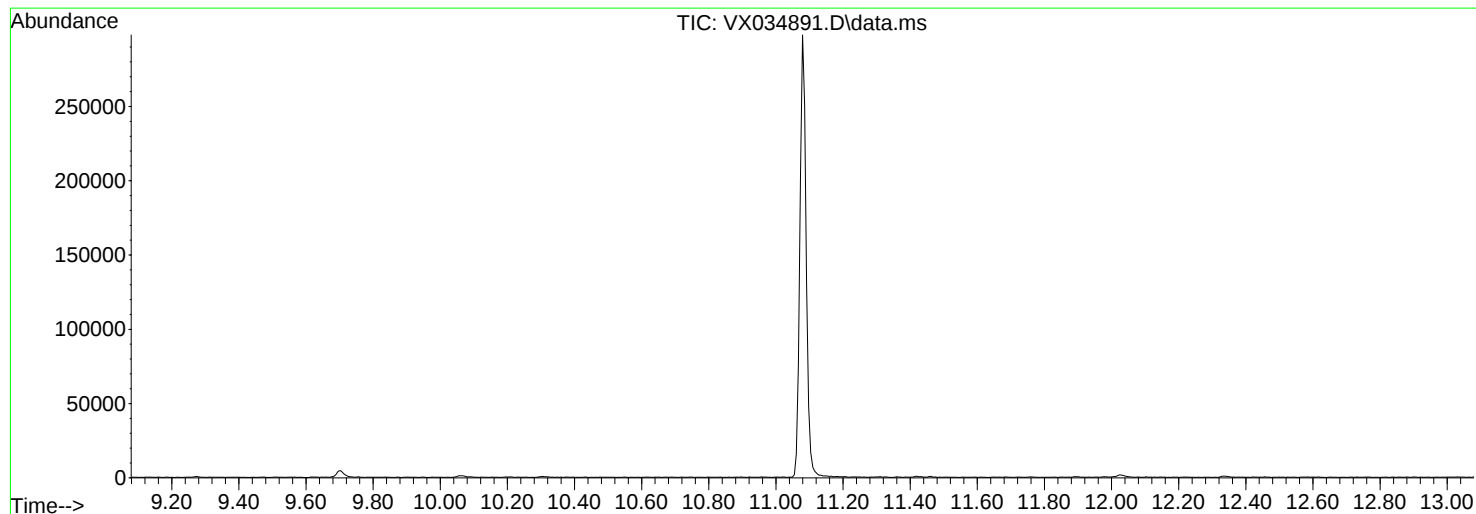

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.0	11350	PASS
75	95	30	60	56.2	27688	PASS
95	95	100	100	100.0	49269	PASS
96	95	5	9	6.7	3321	PASS
173	174	0.00	2	1.1	410	PASS
174	95	50	100	74.6	36773	PASS
175	174	5	9	7.5	2746	PASS
176	174	95	101	95.9	35280	PASS
177	176	5	9	6.2	2182	PASS