
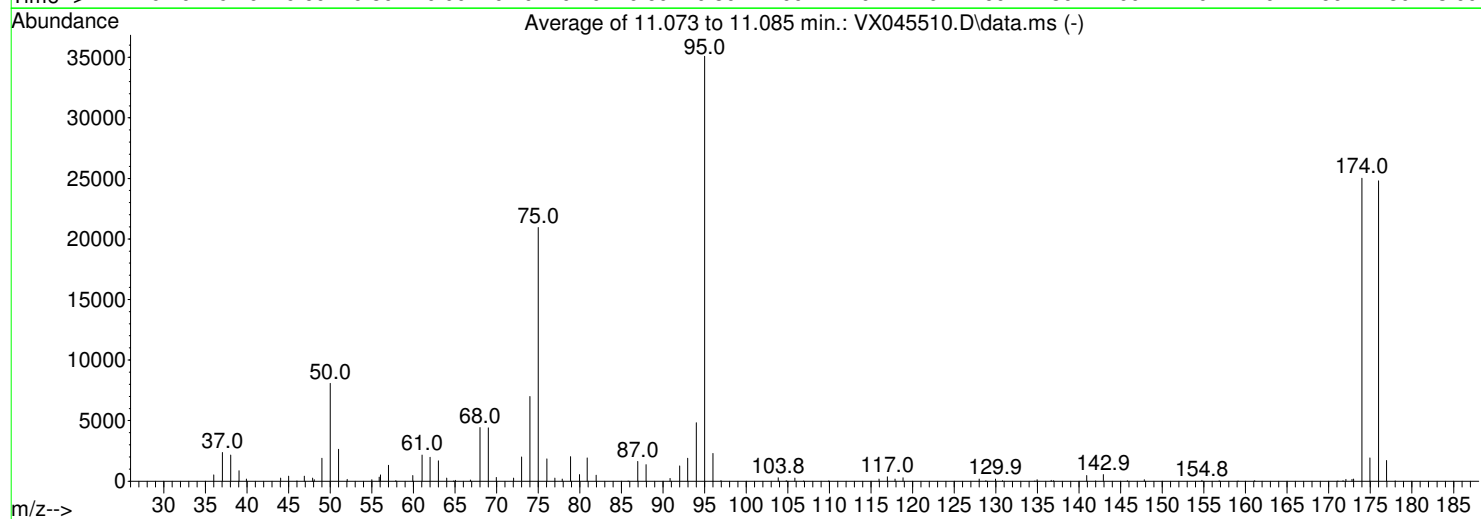


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX033125\
Data File : VX045510.D
Acq On : 31 Mar 2025 09:43
Operator : JC/MD
Sample : BFB718
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB718

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM032825WMA.M
Title : VOC Analysis
Last Update : Mon Apr 07 12:12:10 2025

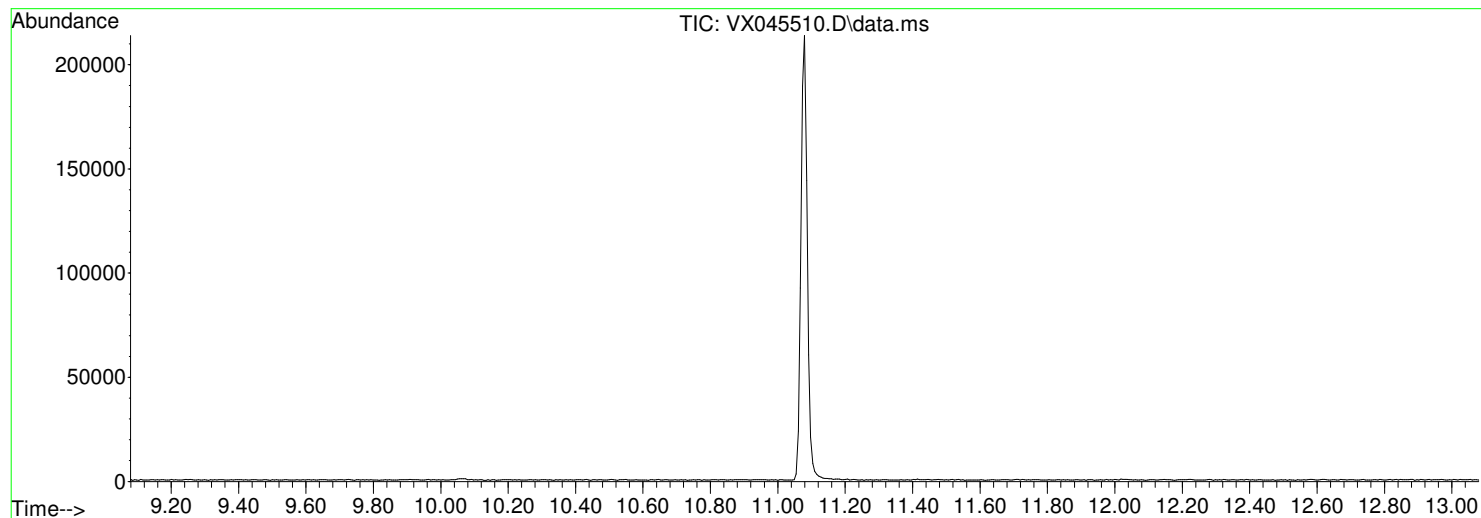

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	23.0	8071	PASS
75	95	30	80	59.7	20942	PASS
95	95	100	100	100.0	35088	PASS
96	95	5	9	6.5	2290	PASS
173	174	0.00	2	0.7	175	PASS
174	95	50	120	71.3	25005	PASS
175	174	5	9	7.7	1923	PASS
176	174	95	101	99.2	24803	PASS
177	176	5	9	6.9	1701	PASS

m/z	Abundance
40.00	430.0
44.10	299.0

Instrument :
MSVOA_X
ClientSampleId :
BFB718

m/z	Abundance
36.00	527.0
37.00	2877.0
38.10	2601.0
39.00	1039.0
40.00	485.0
44.00	614.0
45.00	356.0
46.00	57.0
46.90	502.0
47.90	427.0
49.00	2213.0
50.00	9056.0
51.00	3046.0
52.00	146.0
54.90	148.0
55.90	977.0
57.00	1368.0
57.90	64.0
60.00	500.0
61.00	2570.0
62.00	2326.0
63.00	2147.0
64.00	398.0
65.10	74.0
66.80	110.0
68.00	4812.0
69.00	5111.0
70.00	356.0
72.00	285.0
73.00	2314.0
74.00	8177.0
75.00	23264.0
76.00	2161.0
77.00	243.0
77.90	218.0
78.90	2336.0
79.90	487.0
80.90	2031.0
81.90	453.0
85.80	50.0
86.90	1936.0
87.90	1381.0
90.90	230.0
92.00	1257.0
93.00	2042.0
94.00	5014.0
95.00	36768.0
96.00	2286.0
103.90	234.0
104.80	55.0
105.80	290.0
116.10	143.0
117.00	300.0
117.90	172.0
118.80	306.0
128.00	231.0
128.90	54.0
129.90	142.0
130.80	62.0
135.00	107.0
136.60	73.0
137.00	73.0
140.90	484.0
142.90	496.0
145.80	56.0
147.80	127.0
154.80	80.0
156.80	62.0
161.10	56.0
171.70	120.0
172.10	127.0
172.80	182.0
173.00	195.0
174.00	21720.0
174.90	1840.0
176.00	22576.0
176.90	1568.0

Instrument :
MSVOA_X
ClientSampleId :
BFB718

m/z	Abundance
36.00	646.0
37.10	2657.0
38.00	2521.0
39.10	858.0
39.90	690.0
44.00	586.0
45.00	543.0
46.90	565.0
48.10	378.0
49.00	2074.0
50.00	9483.0
51.00	3169.0
52.10	179.0
55.00	136.0
56.10	836.0
57.00	1524.0
57.90	86.0
59.90	423.0
61.00	2255.0
62.00	2219.0
63.00	1847.0
64.00	263.0
64.90	77.0
65.20	59.0
66.90	142.0
68.00	5262.0
69.00	4752.0
70.00	315.0
72.10	252.0
73.00	2315.0
74.00	8021.0
75.00	23848.0
76.10	2057.0
77.00	332.0
77.90	262.0
78.90	2307.0
80.00	701.0
80.90	2303.0
82.00	595.0
87.00	1663.0
88.00	1695.0
90.80	221.0
92.00	1570.0
93.00	2059.0
94.00	5691.0
95.00	40880.0
96.00	2872.0
97.00	53.0
103.80	354.0
105.90	305.0
109.90	52.0
115.90	229.0
117.00	366.0
117.90	242.0
118.90	311.0
128.00	199.0
129.90	175.0
130.80	80.0
134.90	152.0
136.80	81.0
140.90	465.0
142.00	70.0
142.90	590.0
145.80	89.0
147.80	112.0
154.80	70.0
156.90	55.0
161.10	62.0
171.10	58.0
172.10	176.0
173.00	331.0
174.00	30496.0
175.00	2218.0
176.00	30440.0
177.00	2004.0
178.00	78.0

Instrument :
MSVOA_X
ClientSampleId :
BFB718

m/z	Abundance
36.00	379.0
37.00	1550.0
38.00	1349.0
39.00	672.0
39.90	652.0
44.10	451.0
45.00	325.0
46.90	142.0
47.90	300.0
49.00	1382.0
50.00	5673.0
51.00	1682.0
52.00	89.0
55.10	71.0
56.00	712.0
57.00	1034.0
59.90	449.0
61.10	1624.0
62.00	1394.0
63.00	1083.0
63.90	124.0
64.80	58.0
68.00	3177.0
69.00	3342.0
69.90	232.0
72.00	227.0
73.00	1326.0
74.00	4793.0
75.00	15715.0
76.10	1325.0
76.90	160.0
77.80	73.0
78.90	1392.0
80.00	427.0
80.90	1396.0
81.90	435.0
87.00	1271.0
87.90	1008.0
90.80	193.0
92.00	936.0
92.90	1606.0
94.00	3799.0
95.00	27616.0
96.00	1711.0
96.90	55.0
103.80	237.0
104.80	72.0
105.90	173.0
106.90	60.0
115.80	132.0
116.80	205.0
117.00	206.0
118.00	122.0
118.80	222.0
128.00	93.0
128.70	68.0
130.00	212.0
134.70	72.0
135.00	73.0
136.70	94.0
140.90	442.0
142.90	552.0
147.90	104.0
154.70	64.0
159.10	57.0
171.90	129.0
172.80	230.0
174.00	22800.0
174.90	1710.0
176.00	21392.0
177.00	1531.0

Instrument :
MSVOA_X
ClientSampleId :
BFB718