

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX040119\
 Data File : VX008564.D
 Acq On : 01 Apr 2019 13:27
 Operator : JC/SP
 Sample : K2189-03
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BP-VPB201R-EB-20190329

Quant Time: Apr 02 01:40:26 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X032519W.M
 Quant Title : SW846 8260
 QLast Update : Tue Mar 26 07:57:20 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.66	168	224600	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.86	114	376358	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.11	117	316724	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.08	152	124587	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.06	65	156074	45.84	ug/l	0.00
Spiked Amount 50.000			Recovery	=	91.68%	
35) Dibromofluoromethane	5.50	113	115098	46.90	ug/l	0.00
Spiked Amount 50.000			Recovery	=	93.80%	
50) Toluene-d8	8.71	98	467798	47.67	ug/l	0.00
Spiked Amount 50.000			Recovery	=	95.34%	
62) 4-Bromofluorobenzene	11.13	95	152496	41.94	ug/l	0.00
Spiked Amount 50.000			Recovery	=	83.88%	
Target Compounds						
16) Acetone	2.44	43	10722	6.025	ug/l	Qvalue 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX040119\
Data File : VX008564.D
Acq On : 01 Apr 2019 13:27
Operator : JC/SP
Sample : K2189-03
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BP-VPB201R-EB-20190329

Quant Time: Apr 02 01:40:26 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X032519W.M
Quant Title : SW846 8260
QLast Update : Tue Mar 26 07:57:20 2019
Response via : Initial Calibration




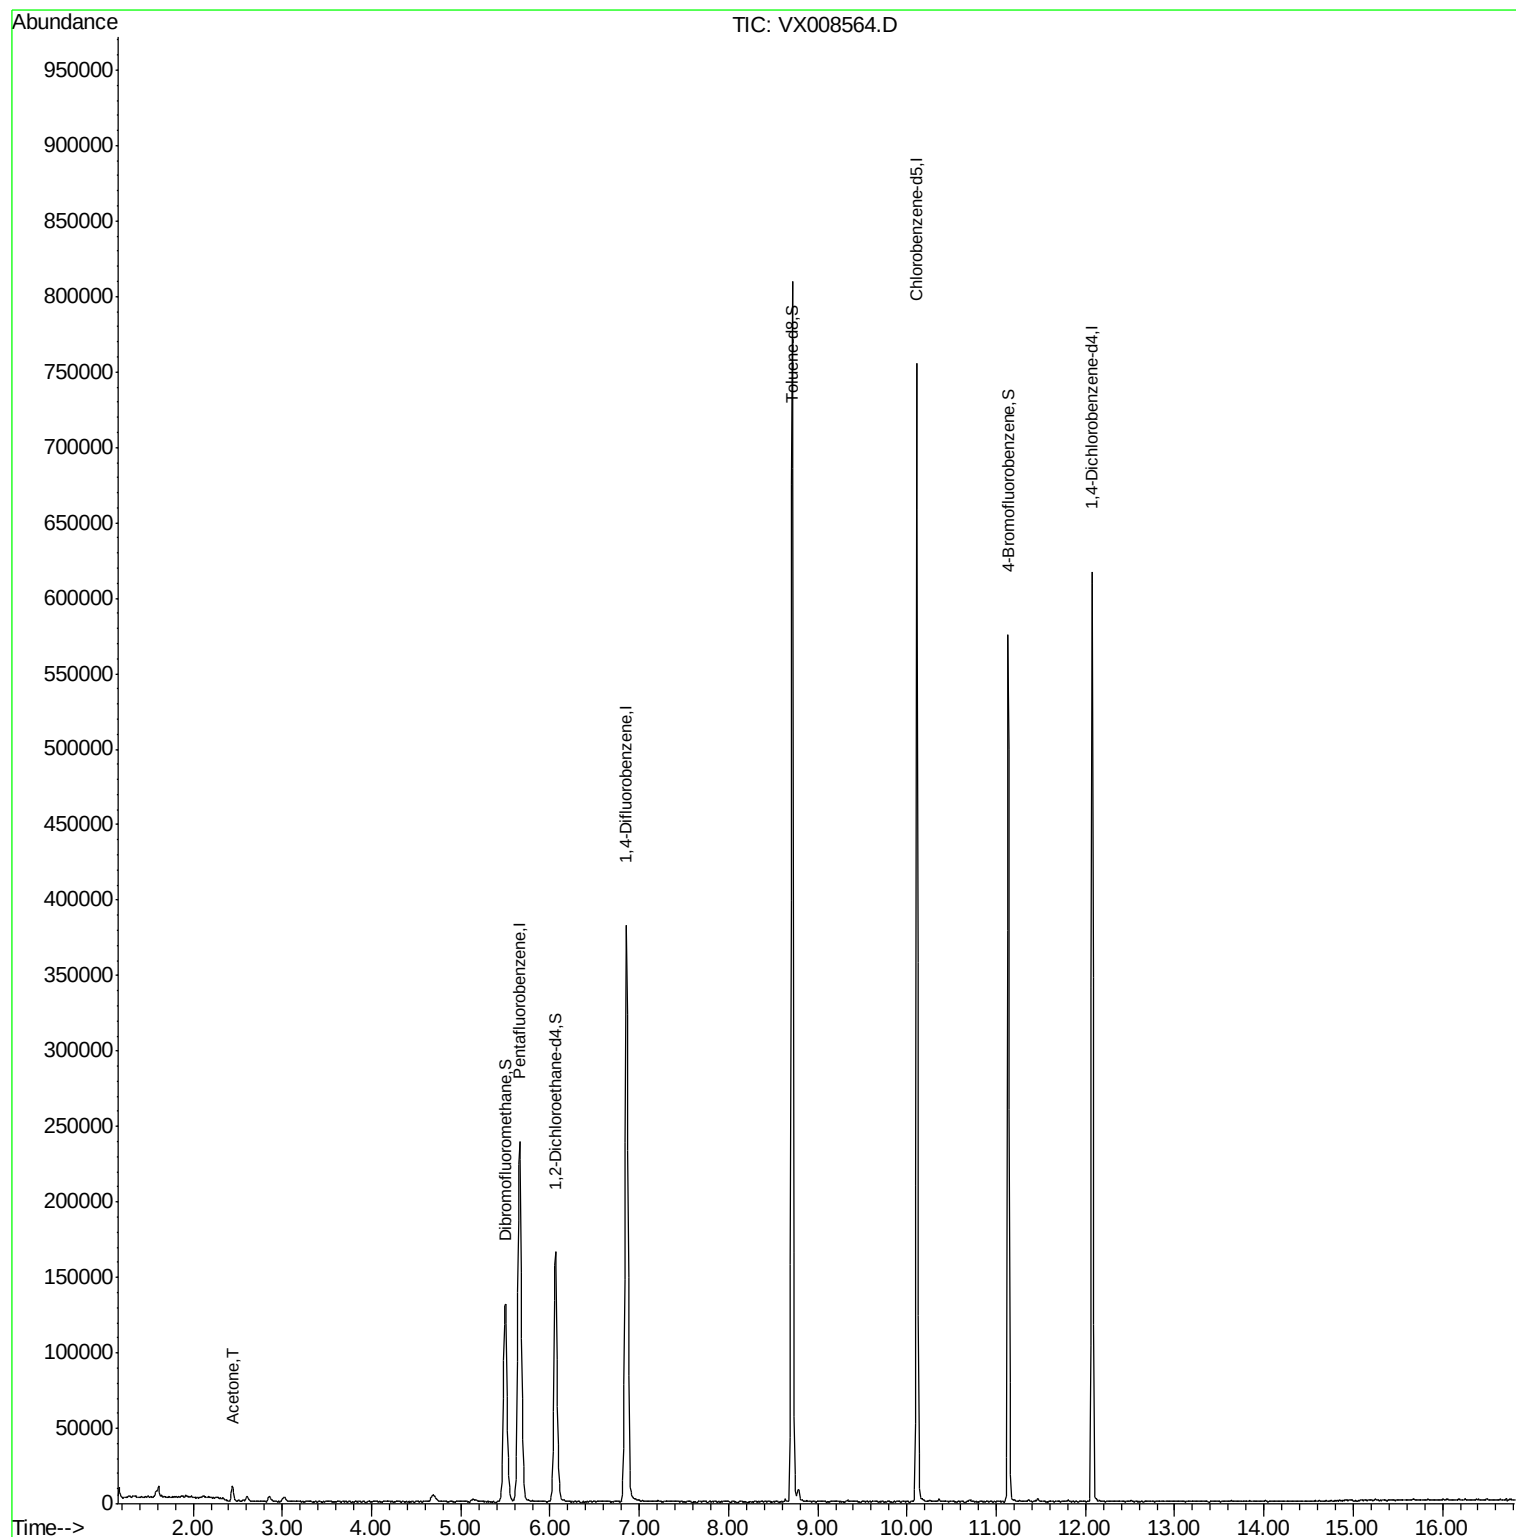


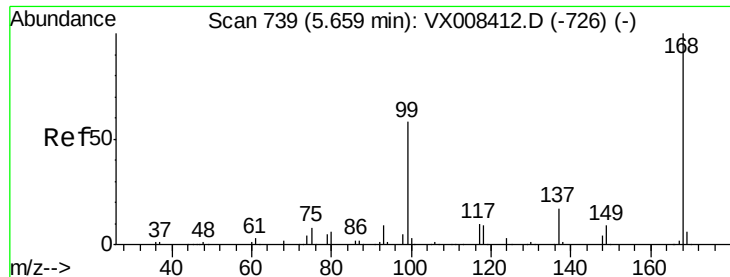

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.66 min Scan# 739
Delta R.T. 0.00 min
Lab File: VX008564.D
Acq: 01 Apr 2019 13:27




Instrument :
MSVOA_X
ClientSampleId :
BP-VPB201R-EB-20190329


Tot Ion:168 Resp: 224600
Ion Ratio Lower Upper
168 100
99 60.4 46.0 69.0

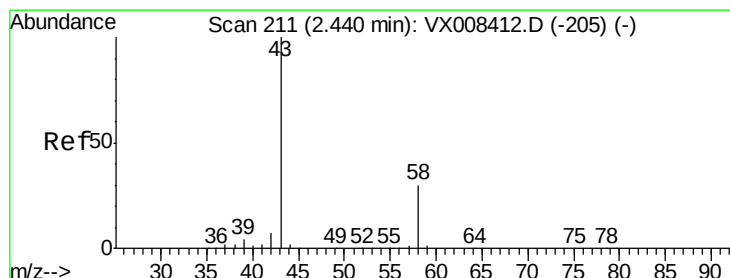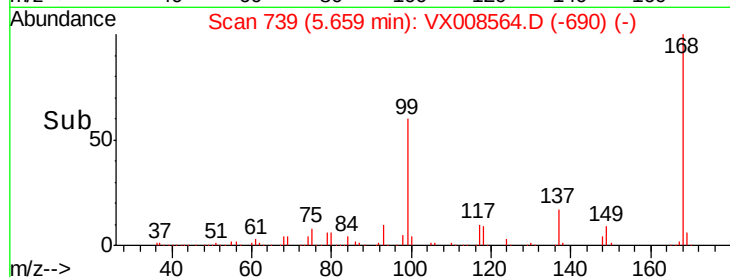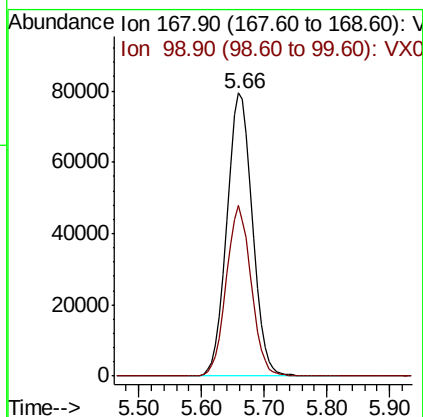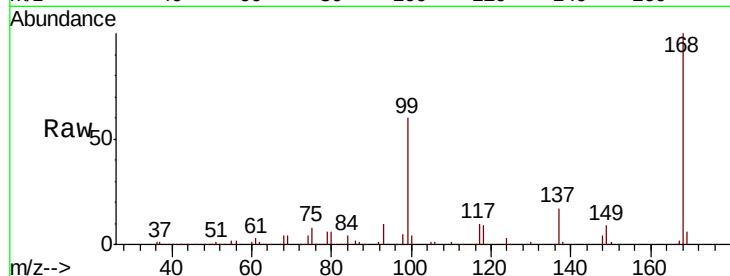

#16
Acetone
Concen: 6.025 ug/l
RT: 2.44 min Scan# 211
Delta R.T. 0.00 min
Lab File: VX008564.D
Acq: 01 Apr 2019 13:27

Tgt Ion: 43 Resp: 10722
Ion Ratio Lower Upper
43 100
58 30.2 24.2 36.2


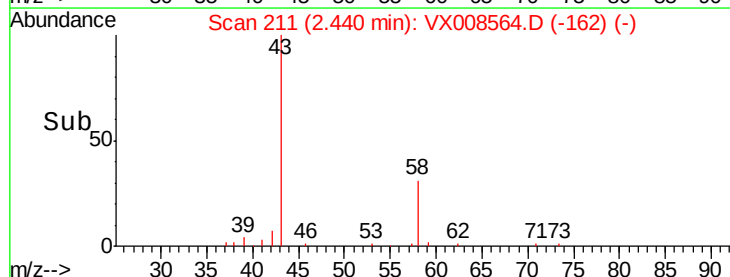
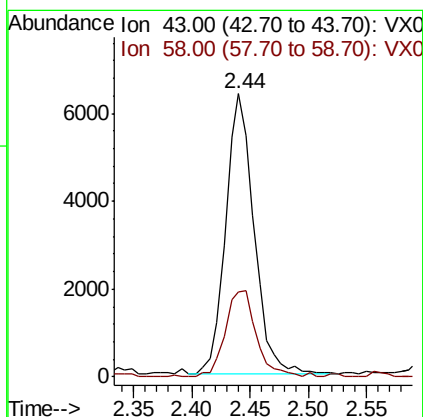
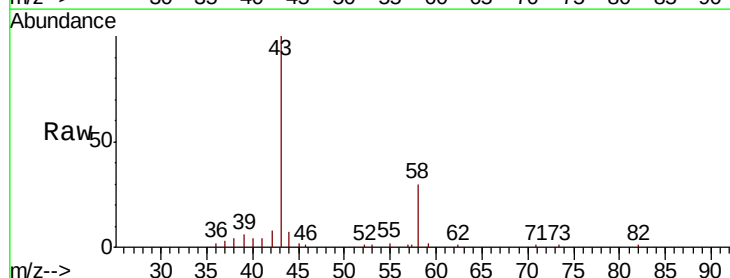


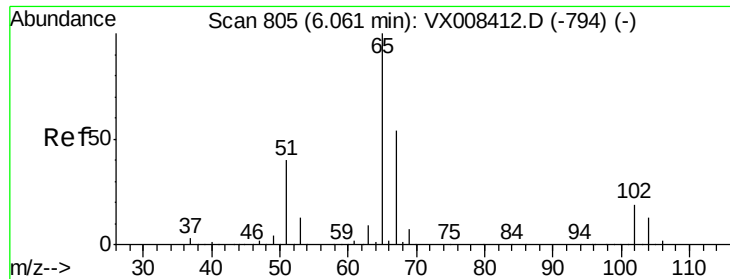

#33
 1,2-Dichloroethane-d4
 Concen: 45.837 ug/l
 RT: 6.06 min Scan# 805
 Delta R.T. 0.00 min
 Lab File: VX008564.D
 Acq: 01 Apr 2019 13:27




Instrument :
 MSVOA_X
 ClientSampleId :
 BP-VPB201R-EB-20190329


Tot Ion: 65 Resp: 156074
 Ion Ratio Lower Upper
 65 100
 67 53.8 0.0 109.4

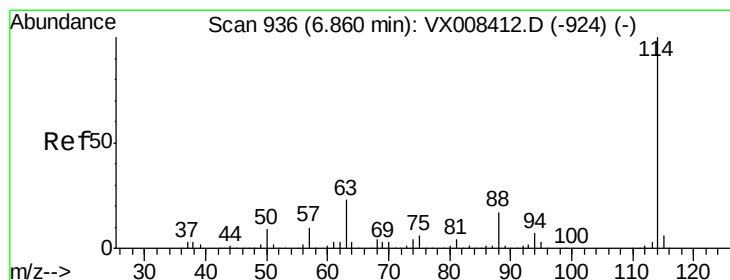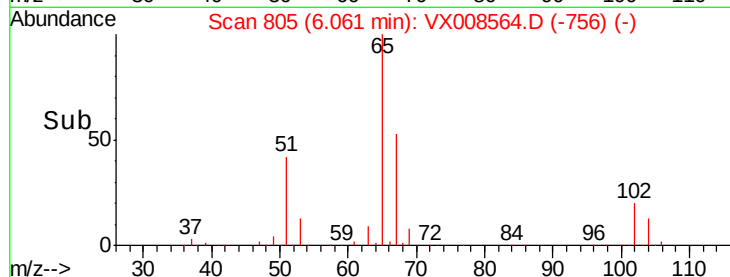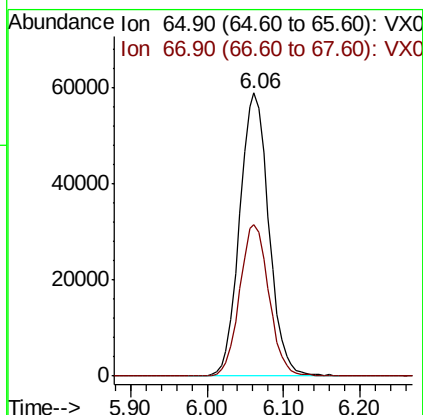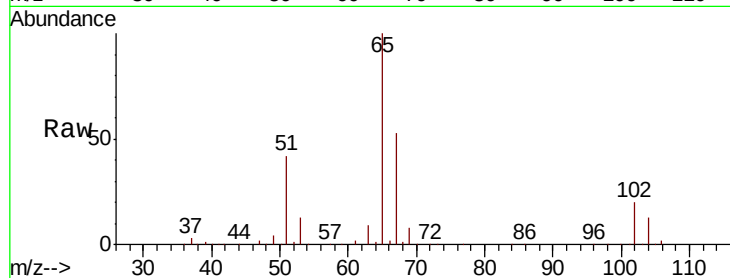

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 6.86 min Scan# 936
 Delta R.T. 0.00 min
 Lab File: VX008564.D
 Acq: 01 Apr 2019 13:27

Tgt Ion: 114 Resp: 376358
 Ion Ratio Lower Upper
 114 100
 63 22.8 0.0 46.4
 88 16.4 0.0 33.2


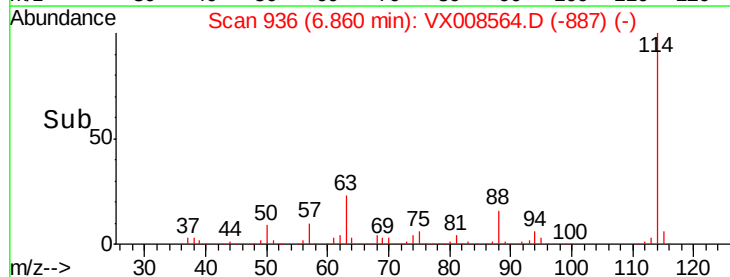
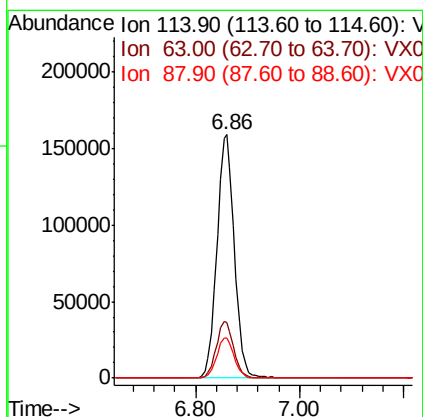
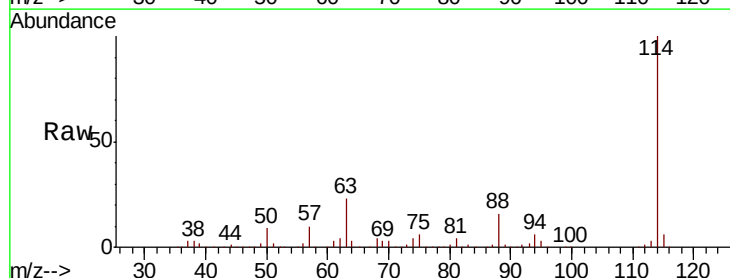


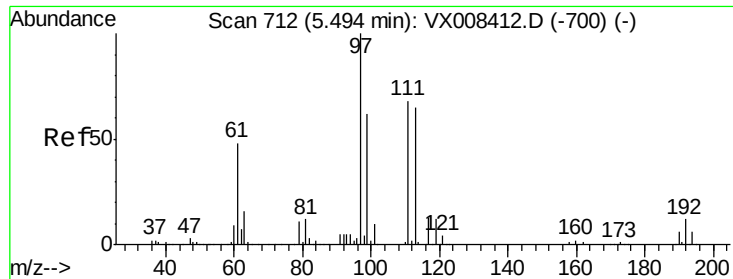

#35
 Dibromofluoromethane
 Concen: 46.902 ug/l
 RT: 5.50 min Scan# 713
 Delta R.T. 0.01 min
 Lab File: VX008564.D
 Acq: 01 Apr 2019 13:27




Instrument :
 MSVOA_X
 ClientSampleId :
 BP-VPB201R-EB-20190329


Tot Ion:113 Resp: 115098
 Ion Ratio Lower Upper
 113 100
 111 102.5 83.0 124.4
 192 19.7 15.6 23.4

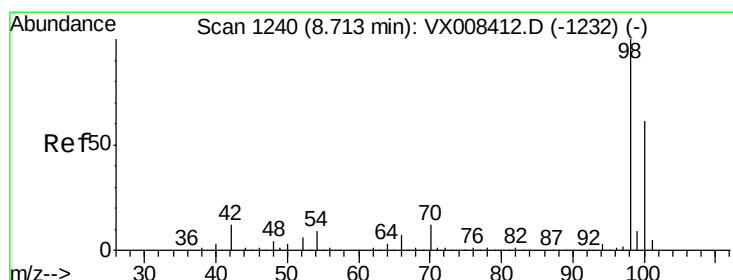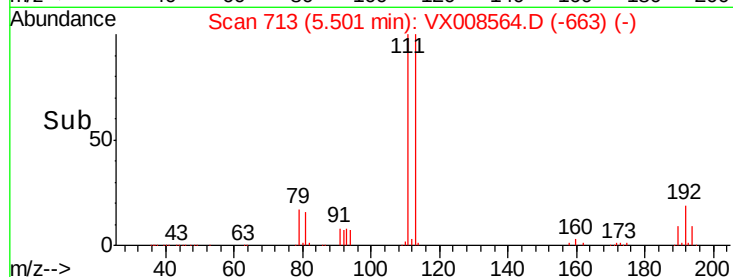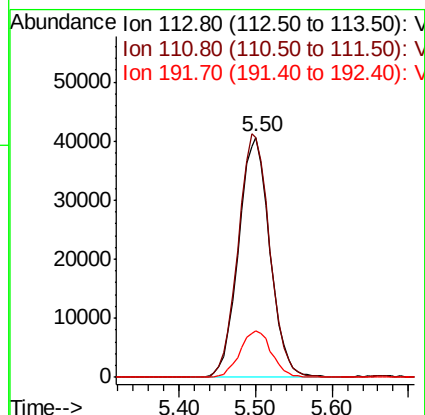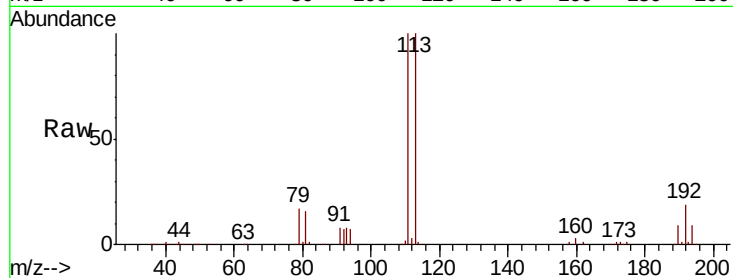

#50
 Toluene-d8
 Concen: 47.673 ug/l
 RT: 8.71 min Scan# 1240
 Delta R.T. 0.00 min
 Lab File: VX008564.D
 Acq: 01 Apr 2019 13:27

Tgt Ion: 98 Resp: 467798
 Ion Ratio Lower Upper
 98 100
 100 64.0 51.1 76.7


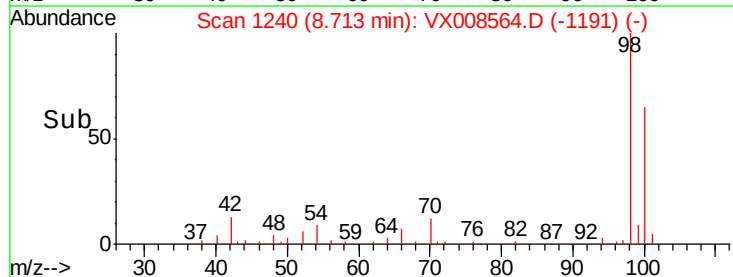
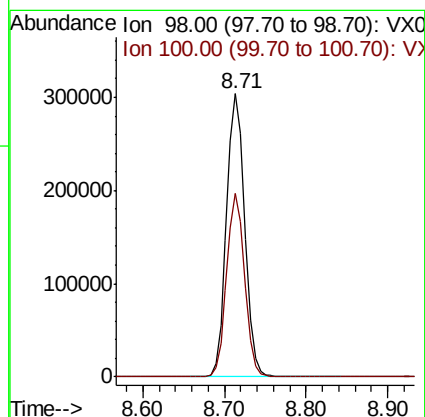
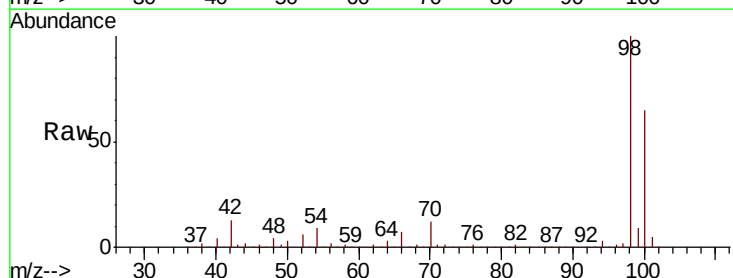


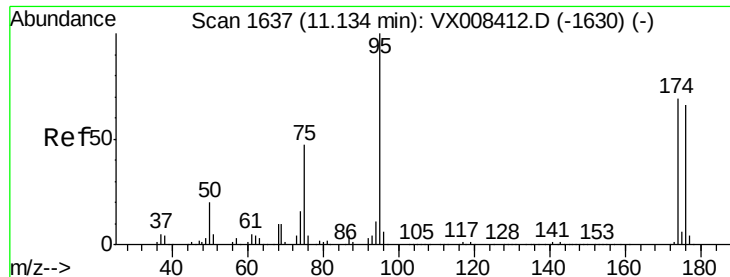

#62
 4-Bromofluorobenzene
 Concen: 41.938 ug/l
 RT: 11.13 min Scan# 1637
 Delta R.T. 0.00 min
 Lab File: VX008564.D
 Acq: 01 Apr 2019 13:27




Instrument :
 MSVOA_X
 ClientSampleId :
 BP-VPB201R-EB-20190329


Tot Ion: 95 Resp: 152496
 Ion Ratio Lower Upper
 95 100
 174 74.6 0.0 147.2
 176 73.2 0.0 142.4

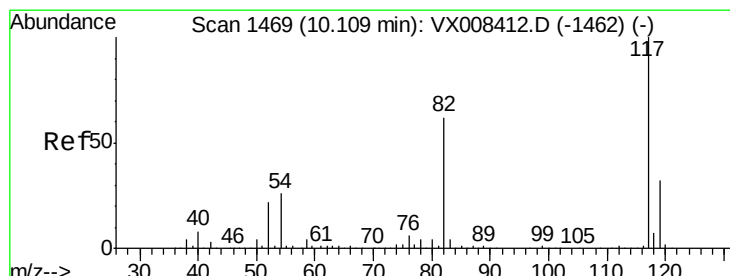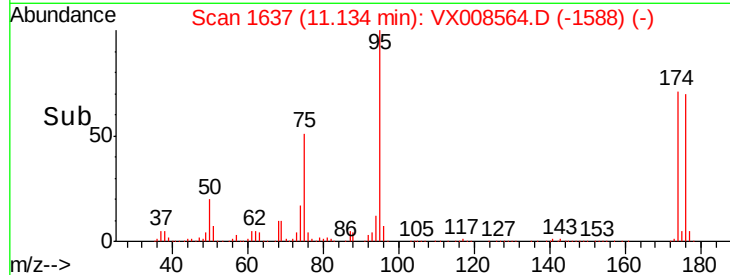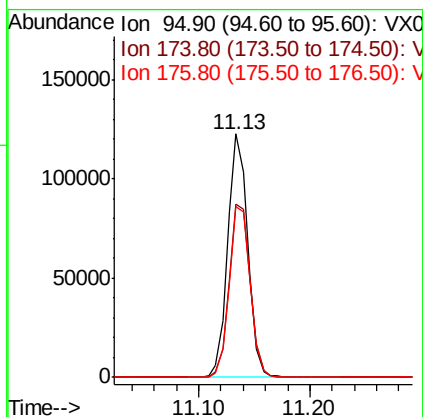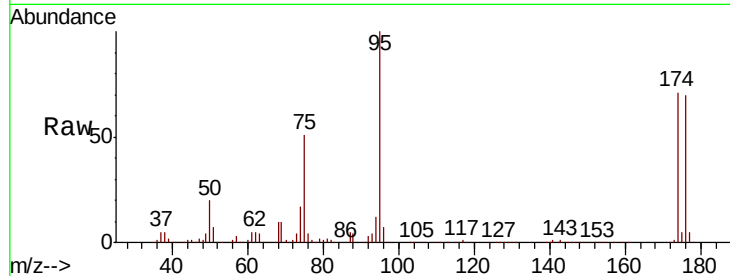

#63
 Chlorobenzene-d5
 Concen: 50.000 ug/l
 RT: 10.11 min Scan# 1469
 Delta R.T. 0.00 min
 Lab File: VX008564.D
 Acq: 01 Apr 2019 13:27

Tgt Ion: 117 Resp: 316724
 Ion Ratio Lower Upper
 117 100
 82 61.5 49.4 74.2
 119 31.8 25.4 38.0

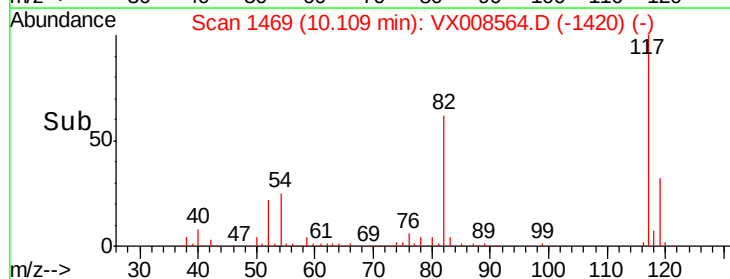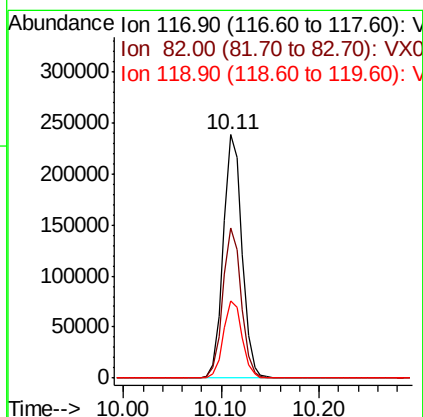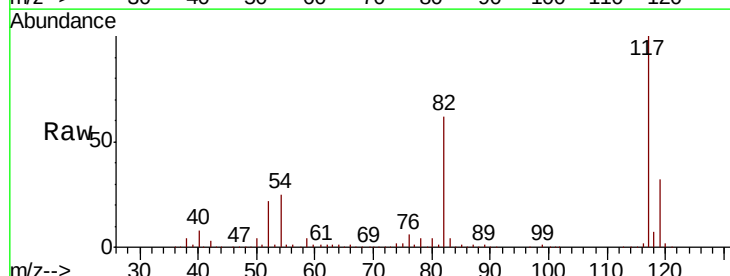

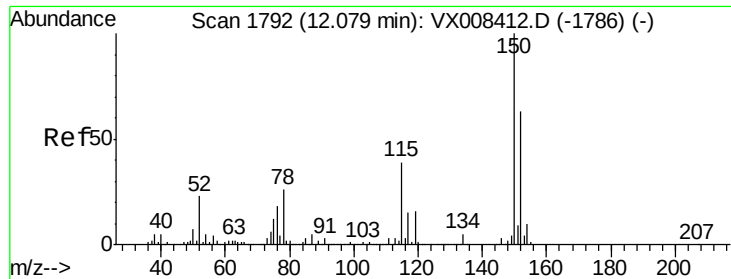

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.08 min Scan# 1792

Delta R.T. 0.00 min

Lab File: VX008564.D

Acq: 01 Apr 2019 13:27

Instrument :

MSVOA_X

ClientSampleId :

BP-VPB201R-EB-20190329

Tot Ion:152 Resp: 124587

Ion Ratio Lower Upper

152 100

115 61.0 43.5 130.5

150 158.1 0.0 348.8

