

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX040119\
 Data File : VX008579.D
 Acq On : 01 Apr 2019 19:16
 Operator : JC/SP
 Sample : K2210-04
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 WE-6

Quant Time: Apr 02 02:34:49 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X032519W.M
 Quant Title : SW846 8260
 QLast Update : Tue Mar 26 07:57:20 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.67	168	224101	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.86	114	377805	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.11	117	326778	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.08	152	137011	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.06	65	158227	46.57	ug/l	0.00
Spiked Amount	50.000		Recovery	=	93.14%	
35) Dibromofluoromethane	5.50	113	115930	47.06	ug/l	0.00
Spiked Amount	50.000		Recovery	=	94.12%	
50) Toluene-d8	8.71	98	473023	48.02	ug/l	0.00
Spiked Amount	50.000		Recovery	=	96.04%	
62) 4-Bromofluorobenzene	11.13	95	162080	44.40	ug/l	0.00
Spiked Amount	50.000		Recovery	=	88.80%	
Target Compounds						
16) Acetone	2.44	43	6339	3.570	ug/l	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX040119\
Data File : VX008579.D
Acq On : 01 Apr 2019 19:16
Operator : JC/SP
Sample : K2210-04
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
WE-6

Quant Time: Apr 02 02:34:49 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X032519W.M
Quant Title : SW846 8260
QLast Update : Tue Mar 26 07:57:20 2019
Response via : Initial Calibration

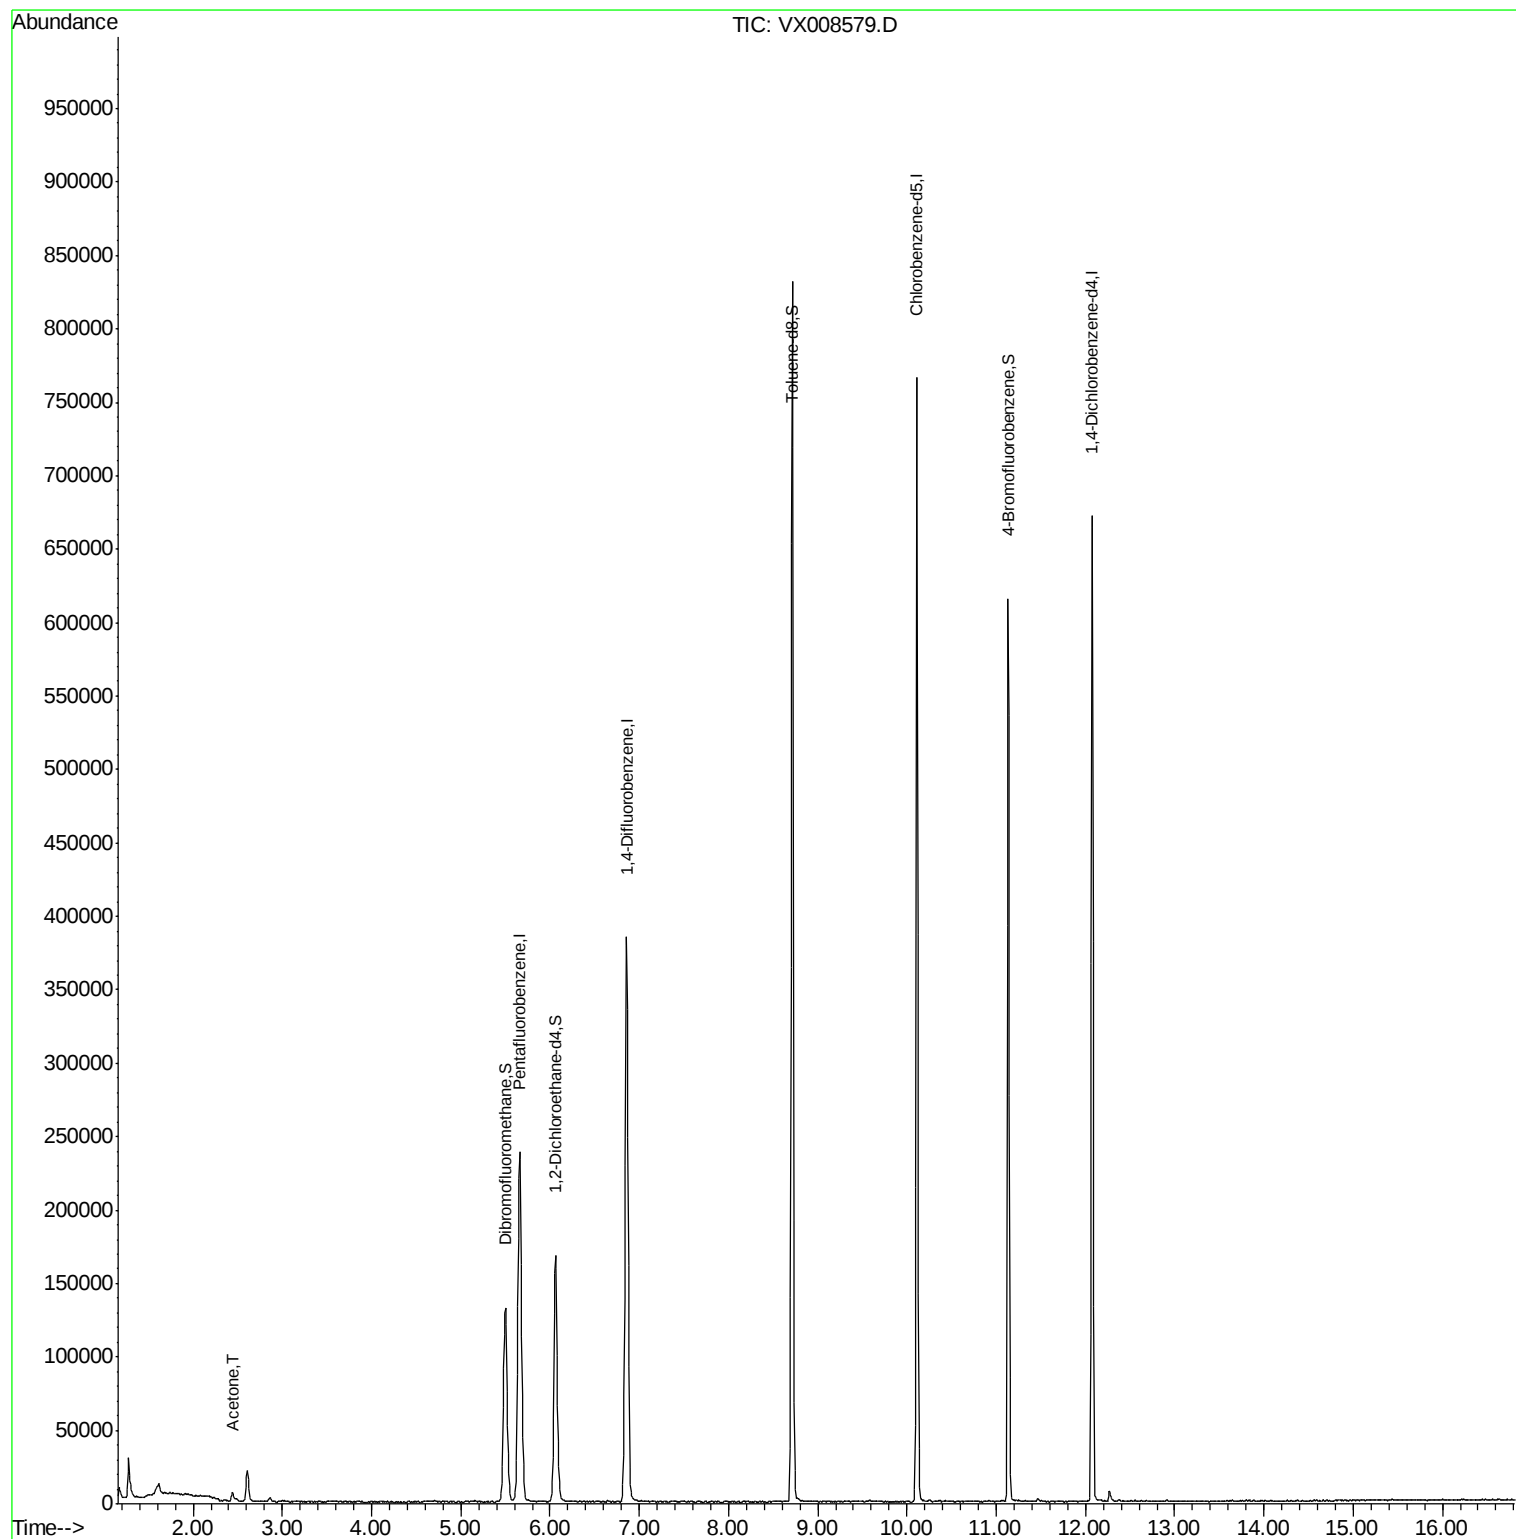

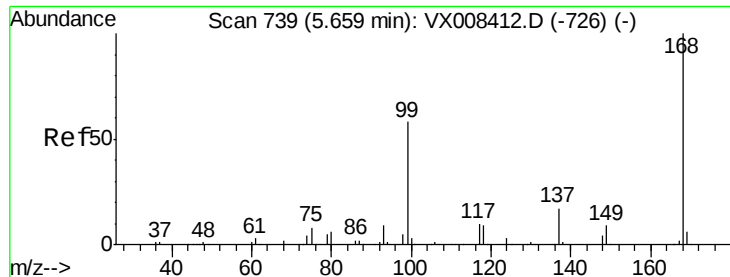

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.67 min Scan# 740

Delta R.T. 0.01 min

Lab File: VX008579.D

Acq: 01 Apr 2019 19:16

Instrument :

MSVOA_X

ClientSampled :


WE-6

Tot Ion:168 Resp: 224101

Ion Ratio Lower Upper




168 100

99 57.6 46.0 69.0

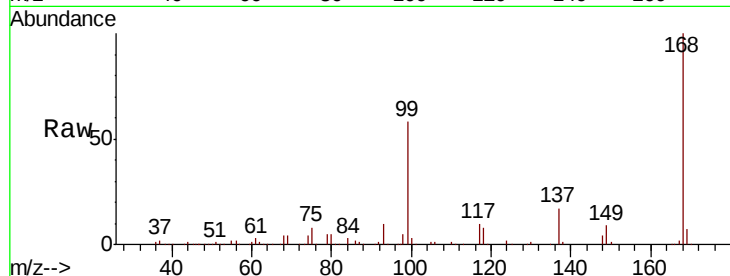

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

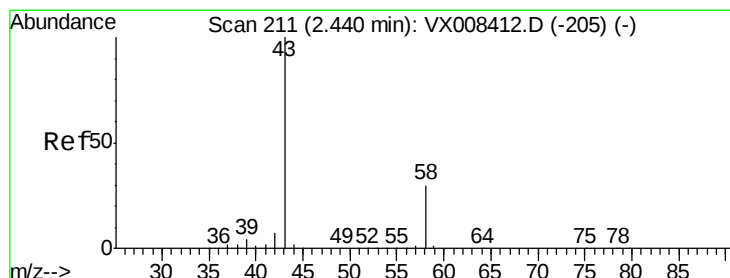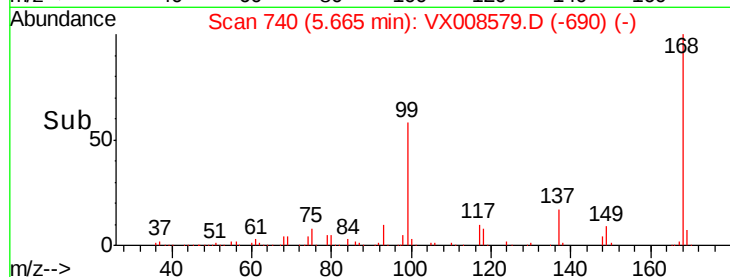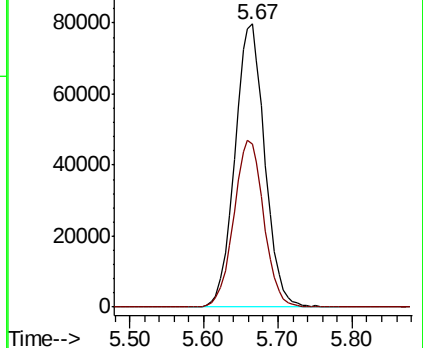

#16

Acetone

Concen: 3.570 ug/l

RT: 2.44 min Scan# 211

Delta R.T. -0.00 min

Lab File: VX008579.D


Acq: 01 Apr 2019 19:16

Tgt Ion: 43 Resp: 6339

Ion Ratio Lower Upper



43 100


58 29.9 24.2 36.2

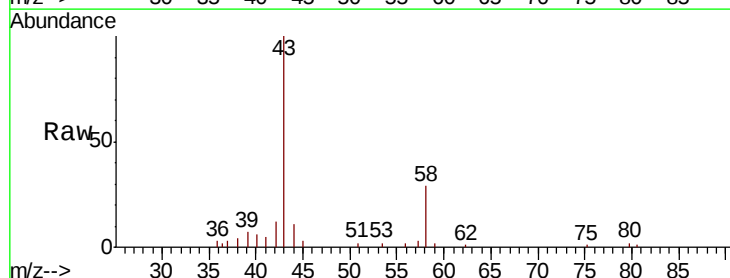

Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0

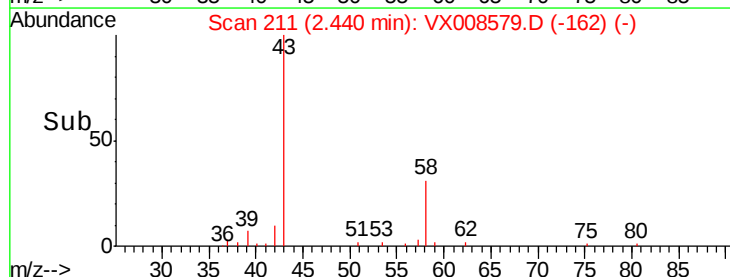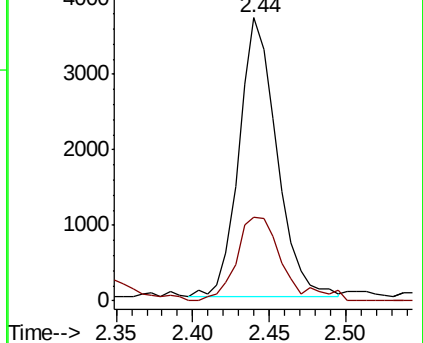

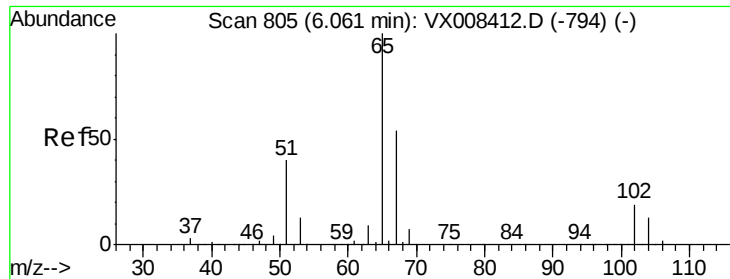

#33

1,2-Dichloroethane-d4

Concen: 46.573 ug/l

RT: 6.06 min Scan# 805

Delta R.T. -0.00 min

Lab File: VX008579.D

Acq: 01 Apr 2019 19:16

Instrument :

MSVOA_X

ClientSampleId :


WE-6

Tot Ion: 65 Resp: 158227

Ion Ratio Lower Upper




65 100

67 53.8 0.0 109.4

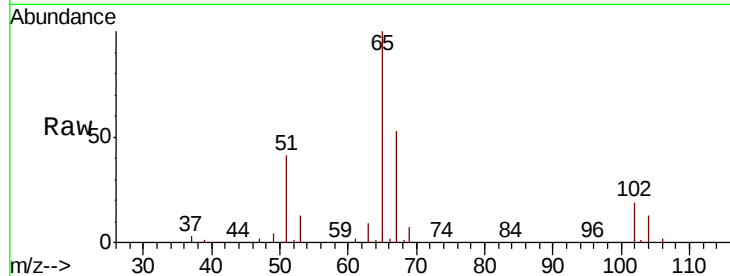

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

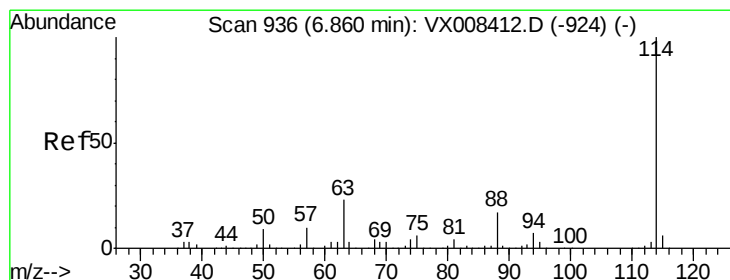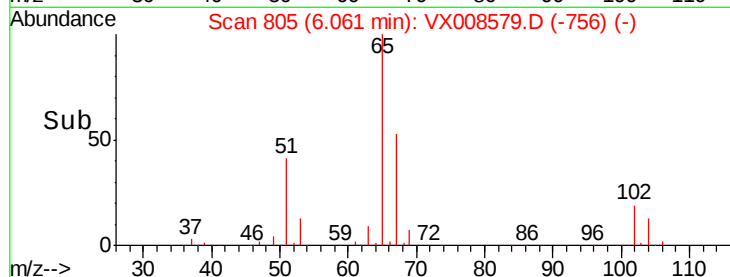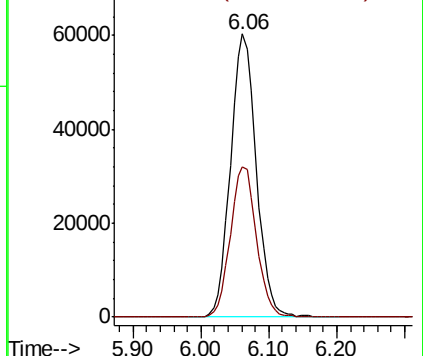

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.86 min Scan# 936

Delta R.T. -0.00 min

Lab File: VX008579.D

Acq: 01 Apr 2019 19:16


Tgt Ion: 114 Resp: 377805

Ion Ratio Lower Upper

114 100

63 23.3 0.0 46.4



88 16.7 0.0 33.2

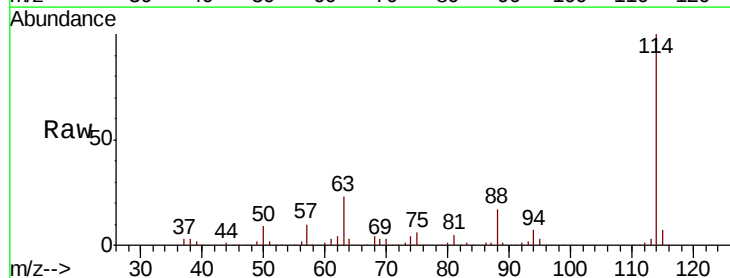


Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0



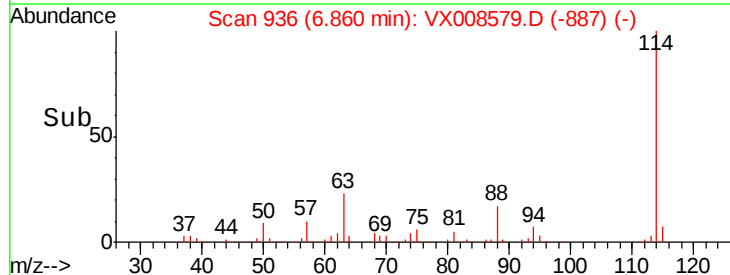
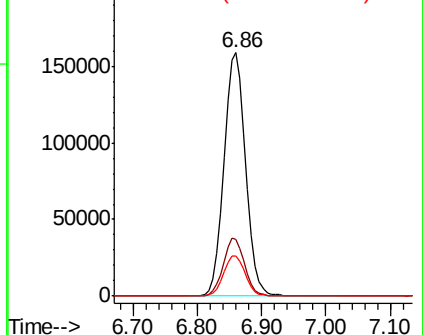


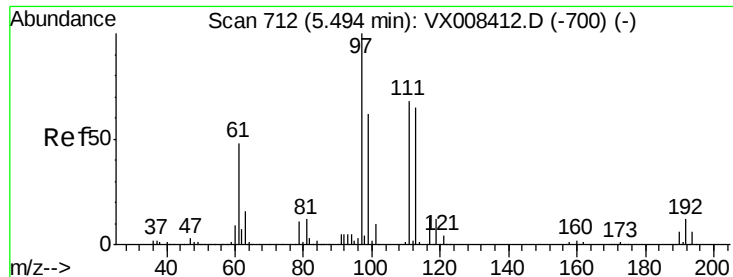

#35
 Dibromofluoromethane
 Concen: 47.060 ug/l
 RT: 5.50 min Scan# 713
 Delta R.T. 0.01 min
 Lab File: VX008579.D
 Acq: 01 Apr 2019 19:16




Instrument :
 MSVOA_X
 ClientSampleId :
 WE-6


Tot Ion:113 Resp: 115930
 Ion Ratio Lower Upper
 113 100
 111 102.6 83.0 124.4
 192 19.7 15.6 23.4

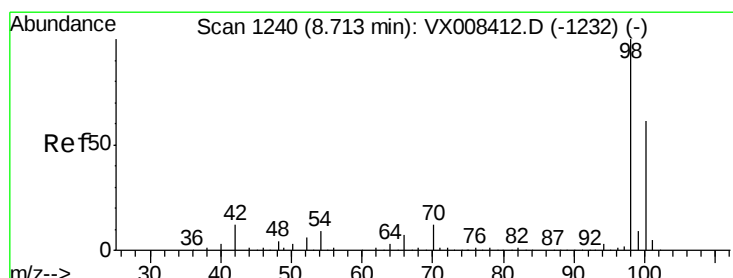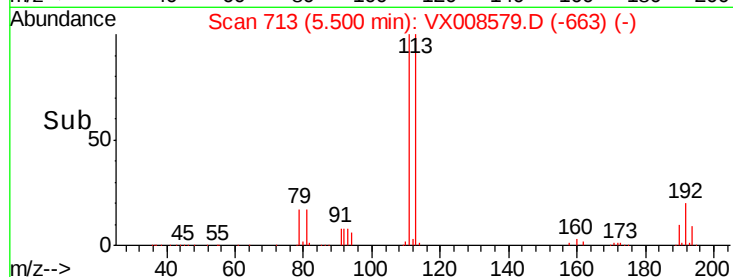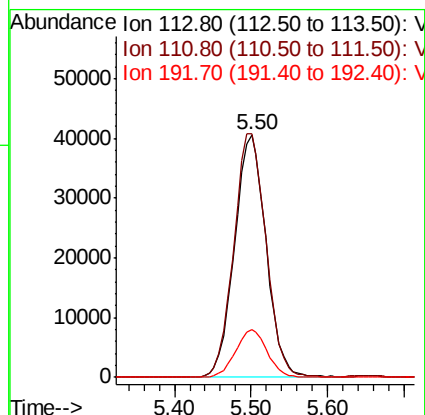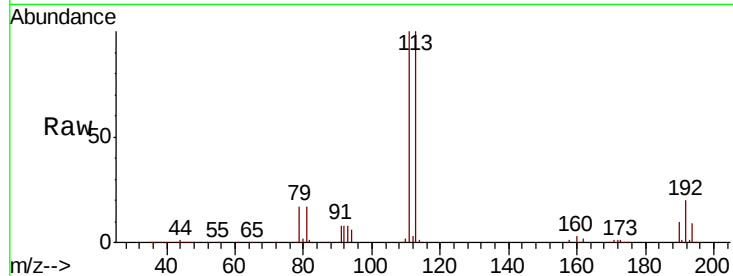

#50
 Toluene-d8
 Concen: 48.021 ug/l
 RT: 8.71 min Scan# 1240
 Delta R.T. -0.00 min
 Lab File: VX008579.D
 Acq: 01 Apr 2019 19:16

Tgt Ion: 98 Resp: 473023
 Ion Ratio Lower Upper
 98 100
 100 64.3 51.1 76.7

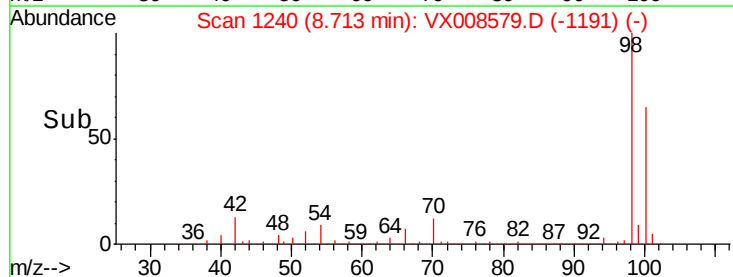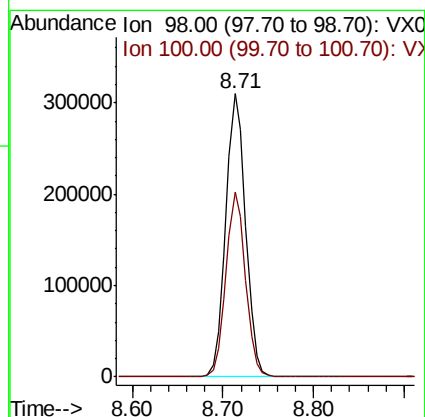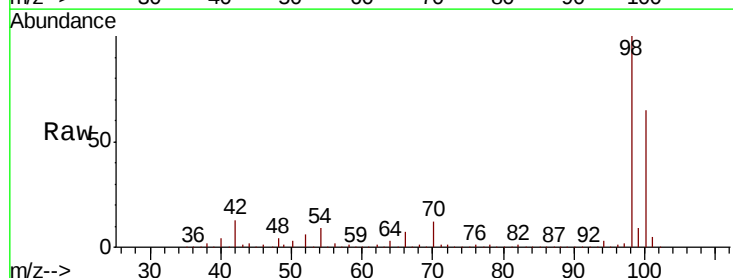

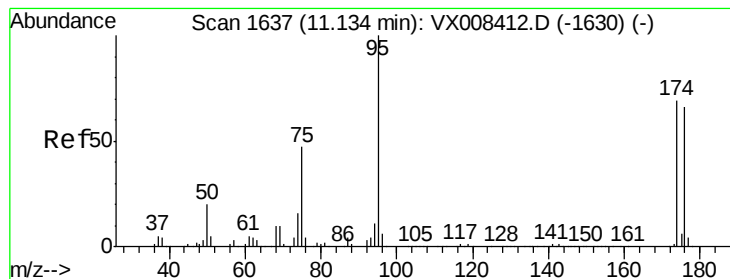

#62

4-Bromofluorobenzene

Concen: 44.403 ug/l

RT: 11.13 min Scan# 1637

Delta R.T. -0.00 min

Lab File: VX008579.D

Acq: 01 Apr 2019 19:16

Instrument :

MSVOA_X

ClientSampleId :

WE-6


Tot Ion: 95 Resp: 162080

Ion Ratio Lower Upper

95 100

174 74.8 0.0 147.2




176 71.8 0.0 142.4

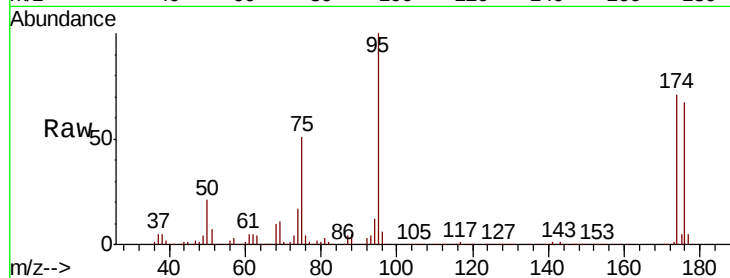

Abundance Ion 94.90 (94.60 to 95.60): VX008412.D (-1630) (-)

Ion 173.80 (173.50 to 174.50): VX008412.D (-1630) (-)

Ion 175.80 (175.50 to 176.50): VX008412.D (-1630) (-)

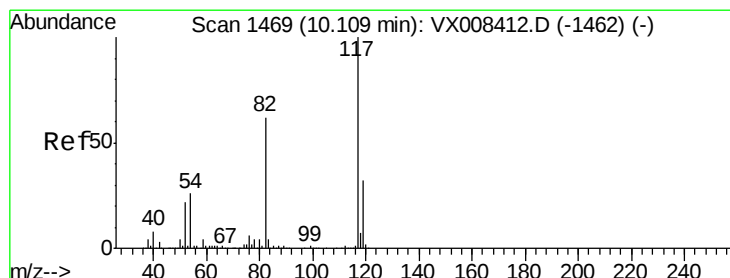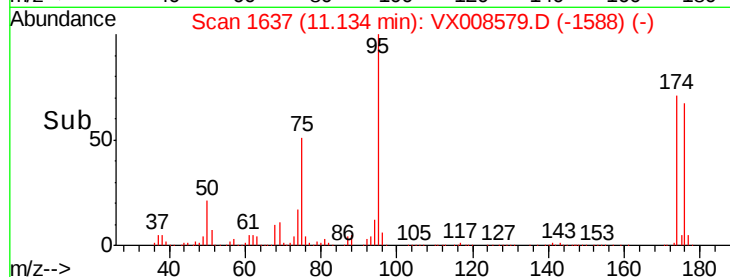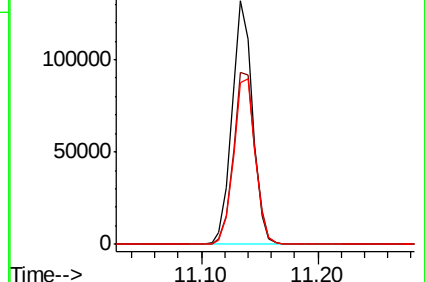

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.11 min Scan# 1469

Delta R.T. -0.00 min

Lab File: VX008579.D

Acq: 01 Apr 2019 19:16


Tgt Ion: 117 Resp: 326778

Ion Ratio Lower Upper

117 100

82 61.4 49.4 74.2



119 31.2 25.4 38.0

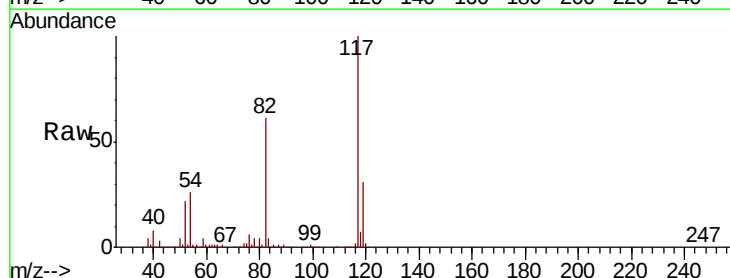


Abundance Ion 116.90 (116.60 to 117.60): VX008412.D (-1462) (-)

Ion 82.00 (81.70 to 82.70): VX008412.D (-1462) (-)

Ion 118.90 (118.60 to 119.60): VX008412.D (-1462) (-)

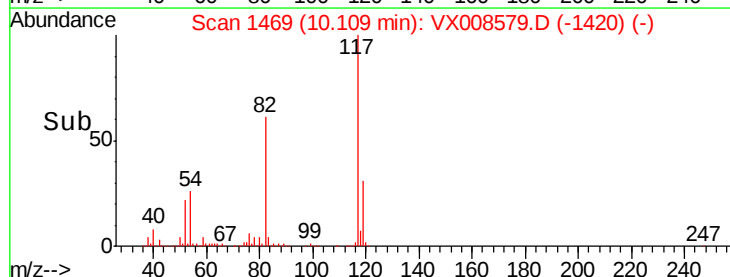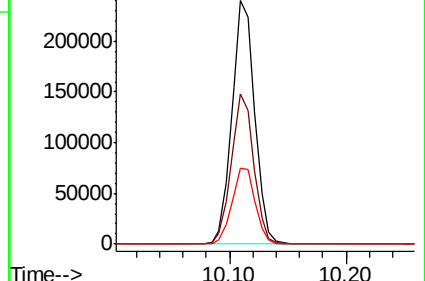

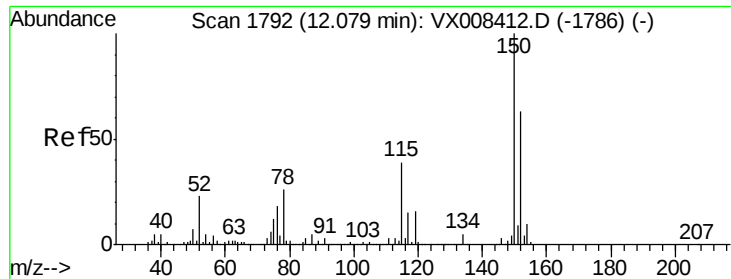

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.08 min Scan# 1792

Delta R.T. -0.00 min

Lab File: VX008579.D

Acq: 01 Apr 2019 19:16

Instrument :

MSVOA_X

ClientSampleId :

WE-6

Tot Ion:152 Resp: 137011

Ion Ratio Lower Upper

152 100

115 61.0 43.5 130.5

150 155.4 0.0 348.8

