

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX040121\
 Data File : VX021705.D
 Acq On : 01 Apr 2021 14:14
 Operator : JC/MD
 Sample : M1890-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 GWBR3-175-185-033121

Quant Time: Apr 02 03:27:09 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M
 Quant Title : SW846 8260
 QLast Update : Wed Mar 24 12:25:26 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.629	168	58786	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.829	114	110057	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.094	117	113734	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.059	152	53643	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.029	65	51548	52.70	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	105.40%
35) Dibromofluoromethane	5.470	113	40274	51.52	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	103.04%
50) Toluene-d8	8.694	98	139374	50.03	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	100.06%
62) 4-Bromofluorobenzene	11.118	95	57989	53.54	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	107.08%

Target Compounds				Qvalue		
3) Chloromethane	1.317	50	962	1.34	ug/l	93
4) Vinyl Chloride	1.399	62	171	0.26	ug/l #	69
5) Bromomethane	1.628	94	108	0.41	ug/l	94
10) Methyl Iodide	2.493	142	37	6.71	ug/l #	42
11) Tert butyl alcohol	3.011	59	153	0.95	ug/l #	73
12) 1,1-Dichloroethene	2.358	96	13053	22.03	ug/l	88
13) Acrolein	2.228	56	23	4.57	ug/l #	1
14) Allyl chloride	2.693	41	262	0.22	ug/l #	25
16) Acetone	2.423	43	4423	11.96	ug/l #	85
18) Methyl Acetate	2.746	43	468	0.44	ug/l #	47
20) Methylene Chloride	2.834	84	724	1.00	ug/l #	79
21) trans-1,2-Dichloroethene	3.146	96	615	0.95	ug/l	92
24) 1,1-Dichloroethane	3.670	63	3057	2.43	ug/l #	92
25) 2-Butanone	4.646	43	1671	2.98	ug/l	100
27) cis-1,2-Dichloroethene	4.570	96	9806	12.98	ug/l	96
28) Bromochloromethane	5.182	49	833	1.32	ug/l #	9
30) Chloroform	5.176	83	8031	6.04	ug/l	90
31) Cyclohexane	5.629	56	1622	1.51	ug/l #	44
36) 1,1-Dichloropropene	5.635	75	5273	4.89	ug/l #	48
38) Carbon Tetrachloride	5.629	117	6440	5.56	ug/l #	17
39) Methylcyclohexane	7.194	83	459	0.38	ug/l #	1
40) Benzene	6.111	78	879	0.29	ug/l #	52
42) 1,2-Dichloroethane	6.164	62	2395	1.80	ug/l	89
44) Trichloroethene	7.188	130	36561	45.24	ug/l	97
48) Methyl methacrylate	7.753	41	537	0.50	ug/l #	72
49) 1,4-Dioxane	7.723	88	311	16.08	ug/l #	79
51) 4-Methyl-2-Pentanone	8.623	43	810	0.65	ug/l #	85
52) Toluene	8.765	92	206327	109.09	ug/l	97
53) t-1,3-Dichloropropene	8.770	75	2787	2.24	ug/l #	1
59) 2-Hexanone	9.465	43	415	0.44	ug/l	76
67) Ethyl Benzene	10.235	91	1138	0.27	ug/l	100
68) m/p-Xylenes	10.341	106	1236	0.83	ug/l	88
69) o-Xylene	10.682	106	599	0.42	ug/l	98
74) N-amyl acetate	10.894	43	437	0.24	ug/l #	26
76) 1,2,3-Trichloropropane	11.118	75	32183	25.77	ug/l #	39
81) trans-1,4-Dichloro-2-b...	11.118	75	32183	78.50	ug/l #	12

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX040121\
Data File : VX021705.D
Acq On : 01 Apr 2021 14:14
Operator : JC/MD
Sample : M1890-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
GWBR3-175-185-033121

Quant Time: Apr 02 03:27:09 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M
Quant Title : SW846 8260
QLast Update : Wed Mar 24 12:25:26 2021
Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
84) 1,2,4-Trimethylbenzene	11.789	105	887	0.27	ug/l	83
95) Naphthalene	13.818	128	1122	0.32	ug/l #	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX040121\
Data File : VX021705.D
Acq On : 01 Apr 2021 14:14
Operator : JC/MD
Sample : M1890-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
GWBR3-175-185-033121


Quant Time: Apr 02 03:27:09 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M
Quant Title : SW846 8260
QLast Update : Wed Mar 24 12:25:26 2021
Response via : Initial Calibration

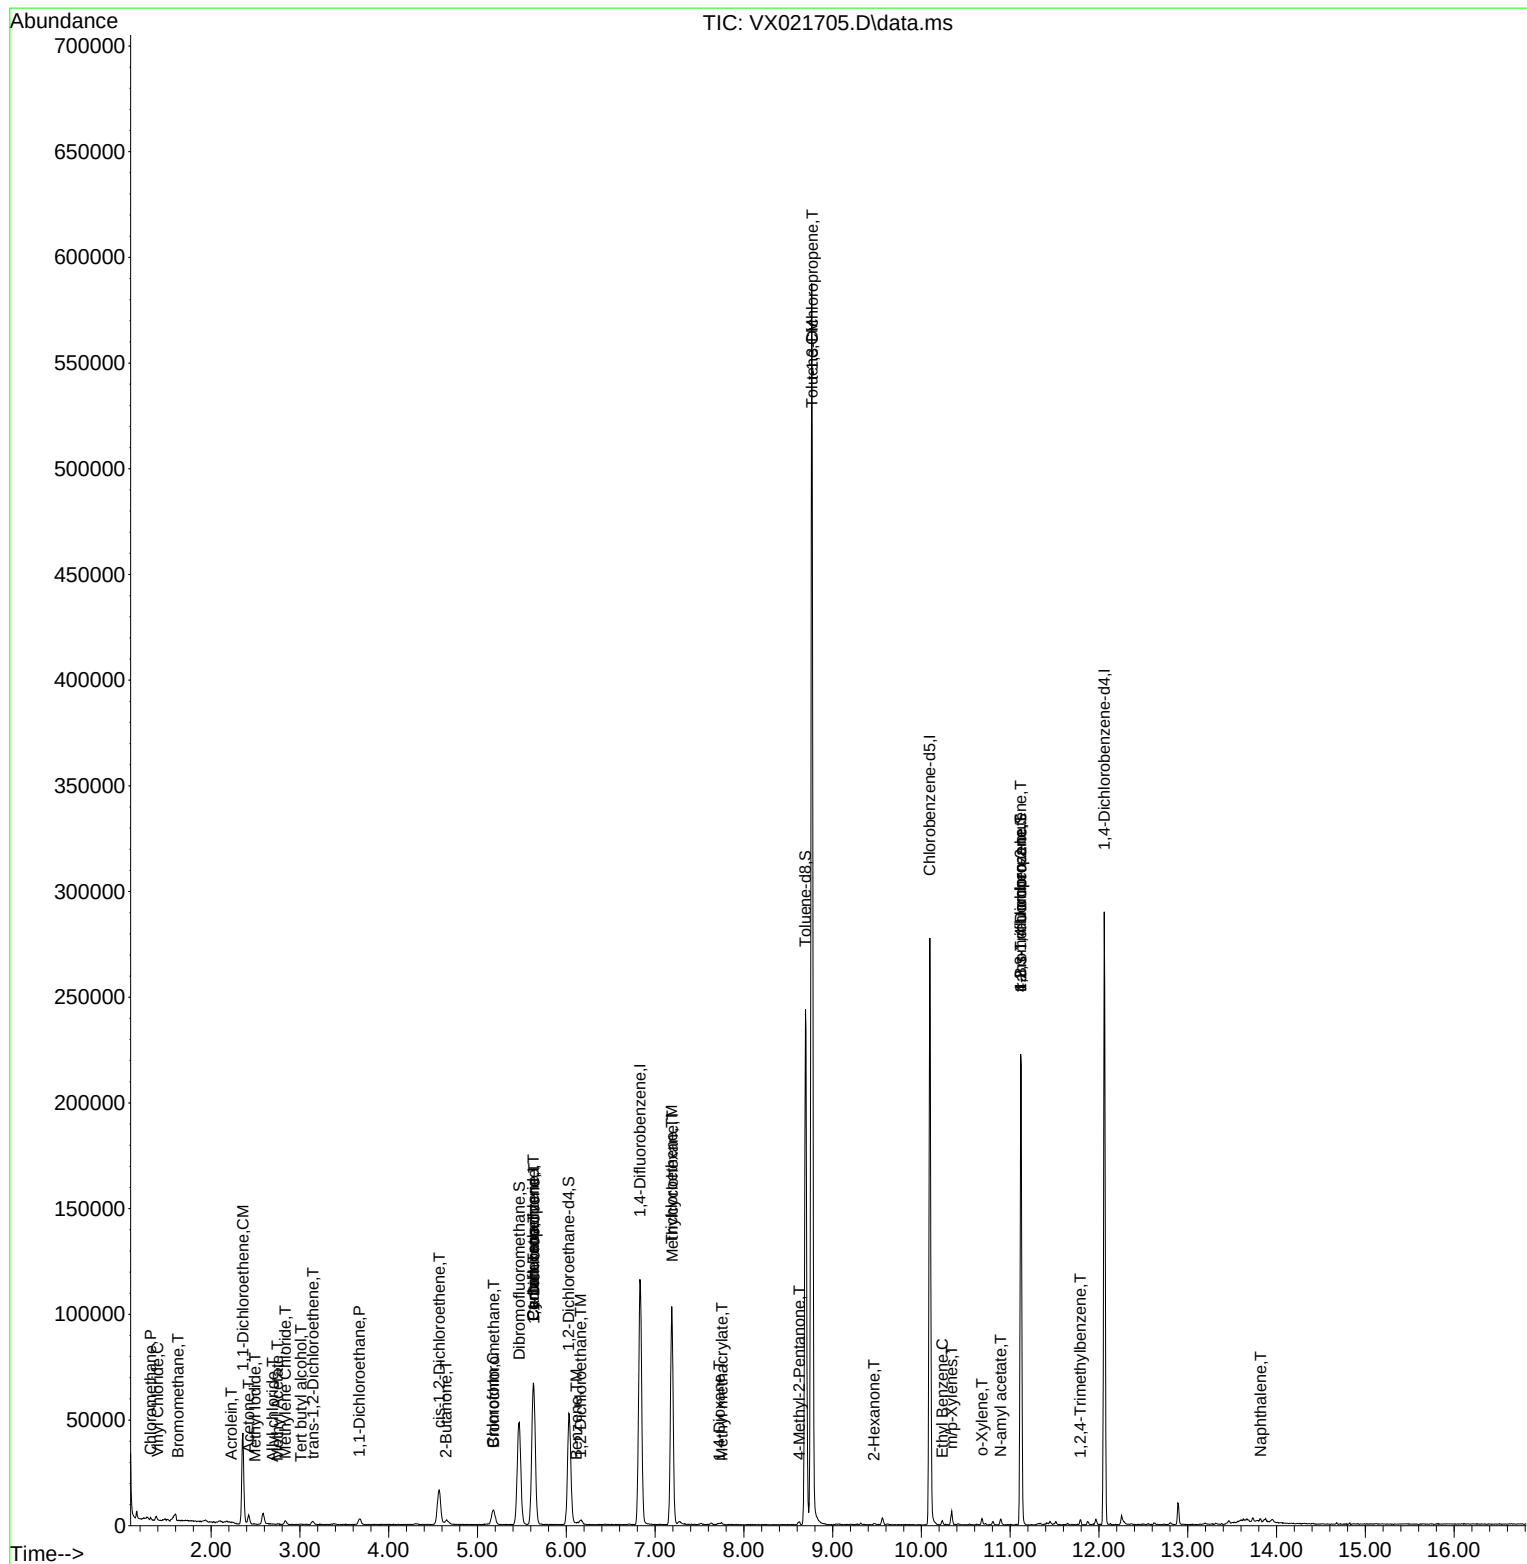



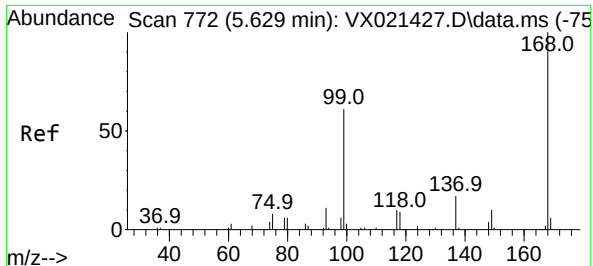


#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 5.629 min Scan# 772
Delta R.T. -0.000 min
Lab File: VX021705.D
Acq: 01 Apr 2021 14:14

Instrument :
MSVOA_X
ClientSampleId :
GWBR3-175-185-033121







Tgt Ion:168 Resp: 58786
Ion Ratio Lower Upper
168 100
99 62.5 45.8 68.6

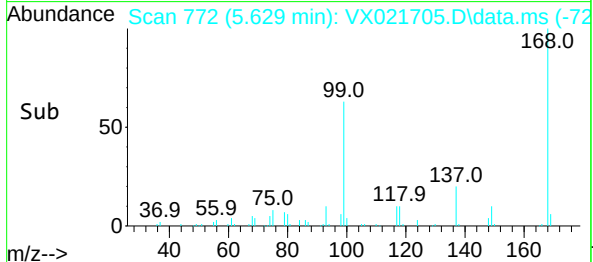

#3
Chloromethane
Concen: 1.34 ug/l
RT: 1.317 min Scan# 39
Delta R.T. 0.006 min
Lab File: VX021705.D
Acq: 01 Apr 2021 14:14

Tgt Ion: 50 Resp: 962
Ion Ratio Lower Upper
50 100
52 36.9 26.4 39.6


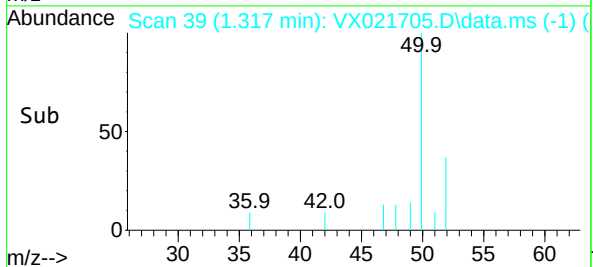

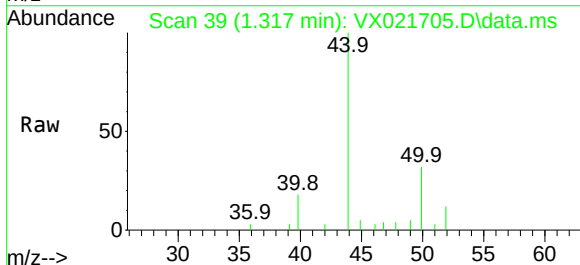


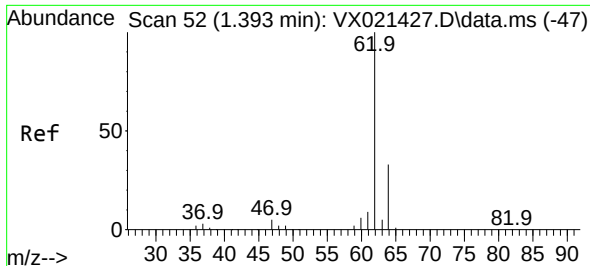

#4
 Vinyl Chloride
 Concen: 0.26 ug/l
 RT: 1.399 min Scan# 53
 Delta R.T. 0.006 min
 Lab File: VX021705.D
 Acq: 01 Apr 2021 14:14




Instrument :
 MSVOA_X
 ClientSampleId :
 GWBR3-175-185-033121


Tgt Ion: 62 Resp: 171
 Ion Ratio Lower Upper
 62 100
 64 49.6 25.7 38.5#

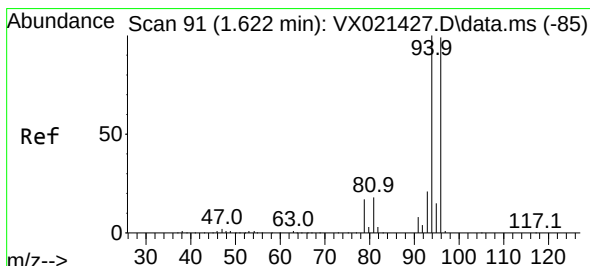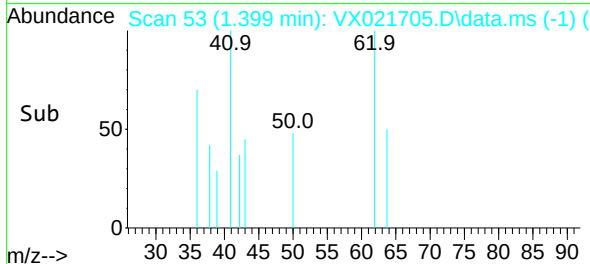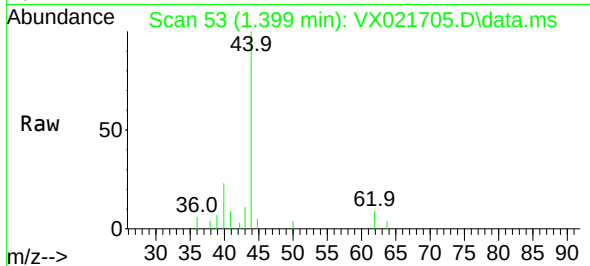

#5
 Bromomethane
 Concen: 0.41 ug/l
 RT: 1.628 min Scan# 92
 Delta R.T. 0.006 min
 Lab File: VX021705.D
 Acq: 01 Apr 2021 14:14

Tgt Ion: 94 Resp: 108
 Ion Ratio Lower Upper
 94 100
 96 101.1 76.4 114.6


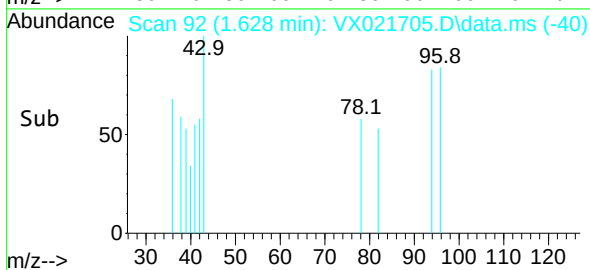

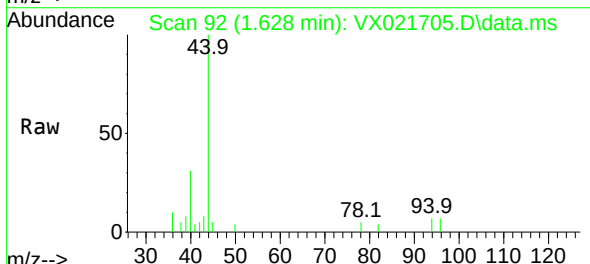


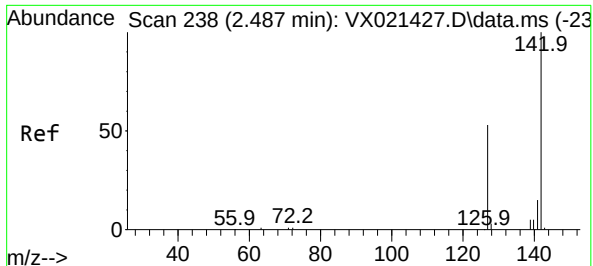

#10
Methyl Iodide
Concen: 6.71 ug/l
RT: 2.493 min Scan# 239
Delta R.T. 0.006 min
Lab File: VX021705.D
Acq: 01 Apr 2021 14:14




Instrument :
MSVOA_X
ClientSampleId :
GWBR3-175-185-033121


Tgt Ion:142 Resp: 37
Ion Ratio Lower Upper
142 100
127 0.0 33.3 49.9#
141 0.0 11.4 17.0#

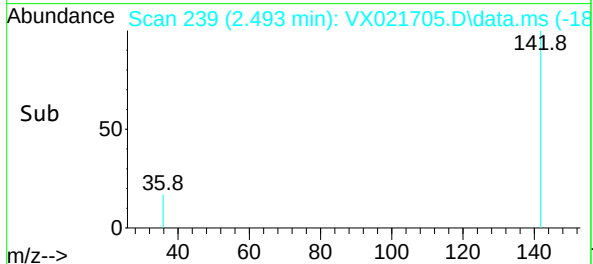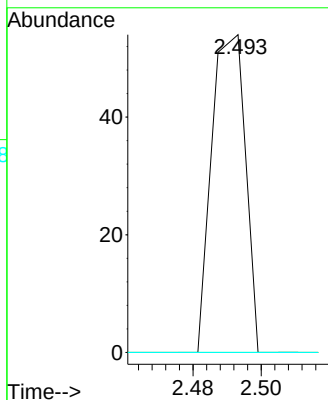

#11
Tert butyl alcohol
Concen: 0.95 ug/l
RT: 3.011 min Scan# 327
Delta R.T. -0.012 min
Lab File: VX021705.D
Acq: 01 Apr 2021 14:14


Tgt Ion: 59 Resp: 153
Ion Ratio Lower Upper
59 100
57 0.0 7.8 11.8#

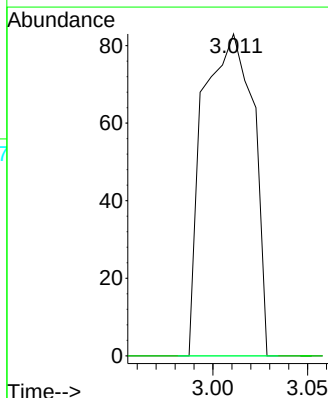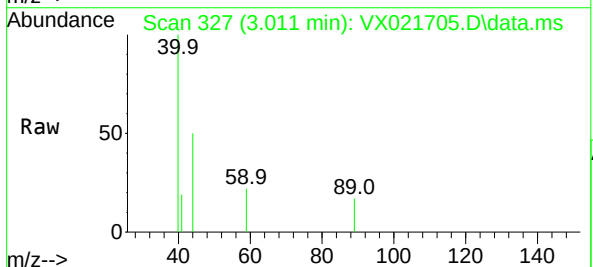






#12
1,1-Dichloroethene
Concen: 22.03 ug/l
RT: 2.358 min Scan# 216
Delta R.T. 0.006 min
Lab File: VX021705.D
Acq: 01 Apr 2021 14:14

Instrument :
MSVOA_X
ClientSampleId :
GWBR3-175-185-033121







Tgt Ion: 96 Resp: 13053
Ion Ratio Lower Upper
96 100
61 177.1 124.6 187.0
98 64.7 50.6 76.0

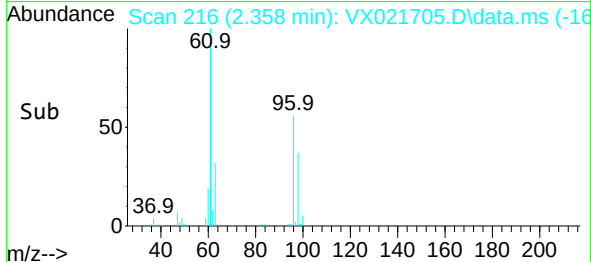

#13
Acrolein
Concen: 4.57 ug/l
RT: 2.228 min Scan# 194
Delta R.T. -0.048 min
Lab File: VX021705.D
Acq: 01 Apr 2021 14:14

Tgt Ion: 56 Resp: 23
Ion Ratio Lower Upper
56 100
55 369.6 56.4 84.6#


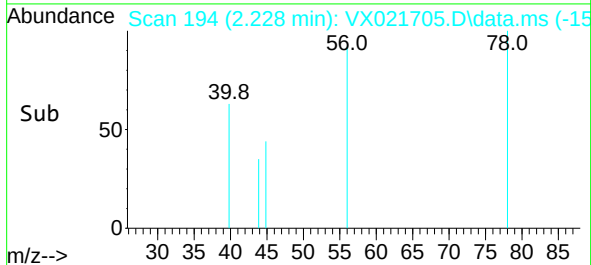

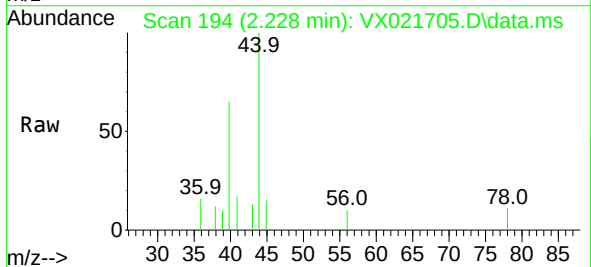




#14
Allyl chloride
Concen: 0.22 ug/l
RT: 2.693 min Scan# 273
Delta R.T. -0.012 min
Lab File: VX021705.D
Acq: 01 Apr 2021 14:14




Instrument :
MSVOA_X
ClientSampleId :
GWBR3-175-185-033121


Tgt Ion:	41	Resp:	262
Ion Ratio	Lower	Upper	
41	100		
39	0.0	51.6	77.4#
76	0.0	30.5	45.7#



#16
Acetone
Concen: 11.96 ug/l
RT: 2.423 min Scan# 227
Delta R.T. -0.000 min
Lab File: VX021705.D
Acq: 01 Apr 2021 14:14


Tgt Ion:	43	Resp:	4423
Ion Ratio	Lower	Upper	
43	100		
58	26.2	27.8	41.8#

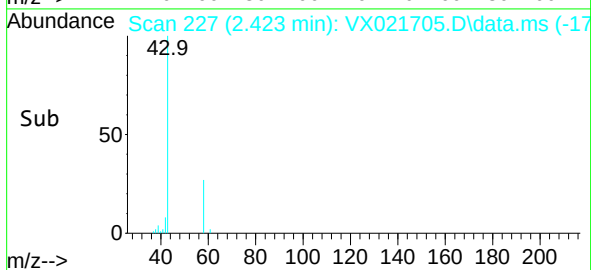



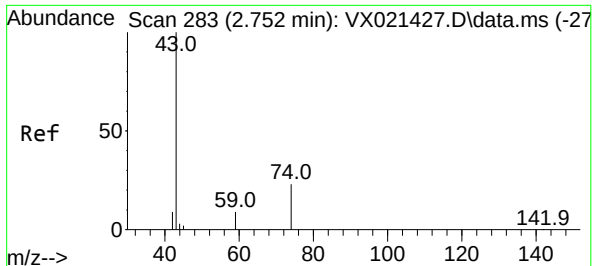


#18
Methyl Acetate
Concen: 0.44 ug/l
RT: 2.746 min Scan# 282
Delta R.T. -0.006 min
Lab File: VX021705.D
Acq: 01 Apr 2021 14:14

Instrument :
MSVOA_X
ClientSampleId :
GWBR3-175-185-033121







Tgt Ion: 43 Resp: 468
Ion Ratio Lower Upper
43 100
74 0.0 21.9 32.9#

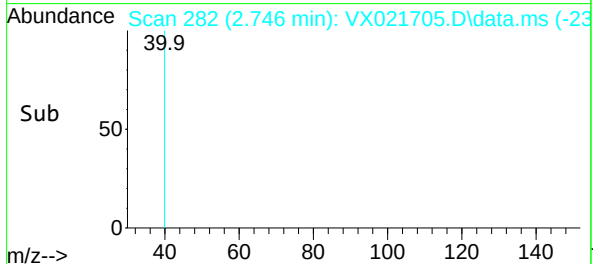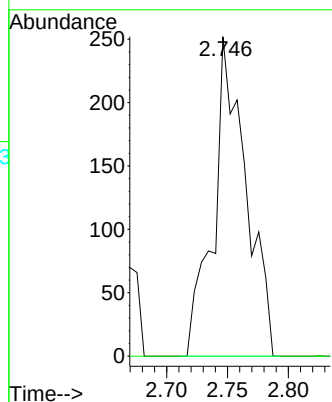

#20
Methylene Chloride
Concen: 1.00 ug/l
RT: 2.834 min Scan# 297
Delta R.T. 0.000 min
Lab File: VX021705.D
Acq: 01 Apr 2021 14:14


Tgt Ion: 84 Resp: 724
Ion Ratio Lower Upper
84 100
49 141.5 88.6 132.8#
51 45.4 27.0 40.6#
86 56.2 50.3 75.5

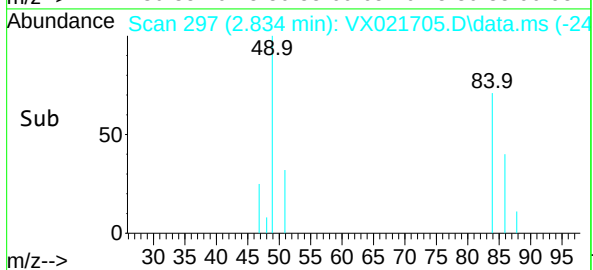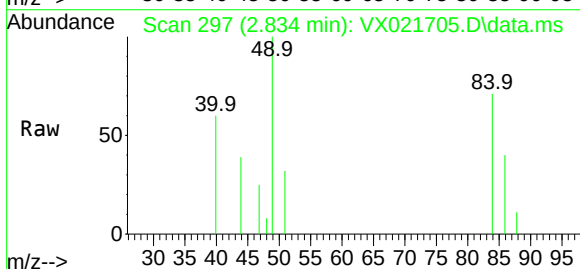






#21
trans-1,2-Dichloroethene
Concen: 0.95 ug/l
RT: 3.146 min Scan# 350
Delta R.T. 0.006 min
Lab File: VX021705.D
Acq: 01 Apr 2021 14:14

Instrument :
MSVOA_X
ClientSampleId :
GWBR3-175-185-033121




Tgt Ion: 96 Resp: 615

Ion	Ratio	Lower	Upper
96	100		
61	141.4	107.7	161.5
98	52.3	50.4	75.6


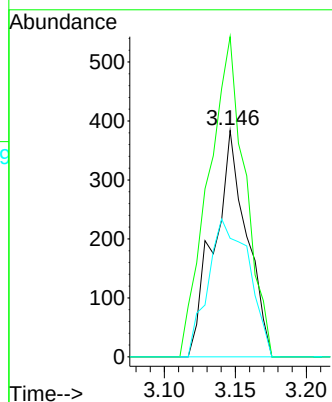



#24
1,1-Dichloroethane
Concen: 2.43 ug/l
RT: 3.670 min Scan# 439
Delta R.T. -0.000 min
Lab File: VX021705.D
Acq: 01 Apr 2021 14:14



Tgt Ion: 63 Resp: 3057

Ion	Ratio	Lower	Upper
63	100		
98	8.5	3.8	11.2
100	0.0	2.5	7.5#



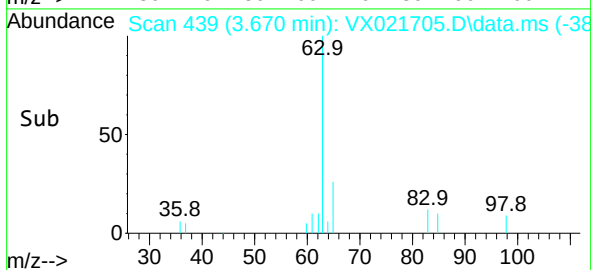
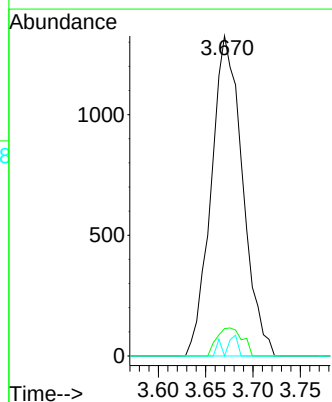




#25
2-Butanone
Concen: 2.98 ug/l
RT: 4.646 min Scan# 605
Delta R.T. 0.011 min
Lab File: VX021705.D
Acq: 01 Apr 2021 14:14




Instrument :
MSVOA_X
ClientSampleId :
GWBR3-175-185-033121


Tgt Ion: 43 Resp: 1671
Ion Ratio Lower Upper
43 100
72 29.8 23.7 35.5

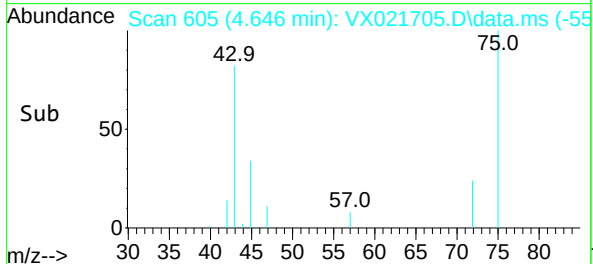

#27
cis-1,2-Dichloroethene
Concen: 12.98 ug/l
RT: 4.570 min Scan# 592
Delta R.T. 0.012 min
Lab File: VX021705.D
Acq: 01 Apr 2021 14:14

Tgt Ion: 96 Resp: 9806
Ion Ratio Lower Upper
96 100
61 136.7 0.0 285.6
98 64.3 0.0 129.6


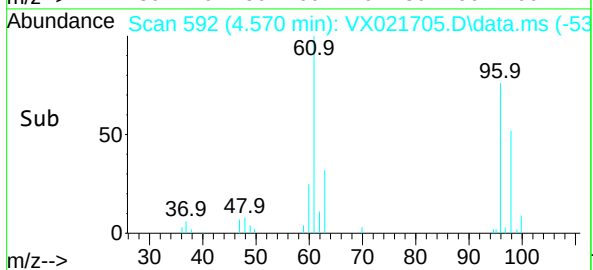

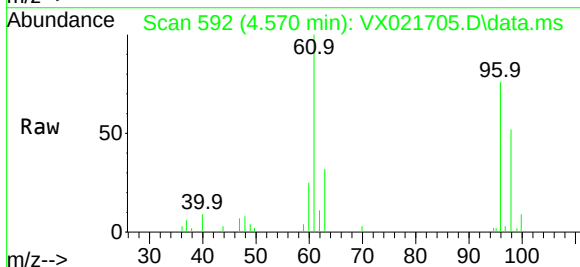




#28
Bromochloromethane
Concen: 1.32 ug/l
RT: 5.182 min Scan# 696
Delta R.T. 0.206 min
Lab File: VX021705.D
Acq: 01 Apr 2021 14:14




Instrument :
MSVOA_X
ClientSampleId :
GWBR3-175-185-033121


Tgt Ion: 49 Resp: 833
Ion Ratio Lower Upper
49 100
129 0.0 0.0 4.0
130 0.0 68.2 102.2#



#30
Chloroform
Concen: 6.04 ug/l
RT: 5.176 min Scan# 695
Delta R.T. -0.000 min
Lab File: VX021705.D
Acq: 01 Apr 2021 14:14


Tgt Ion: 83 Resp: 8031
Ion Ratio Lower Upper
83 100
85 57.2 52.0 78.0

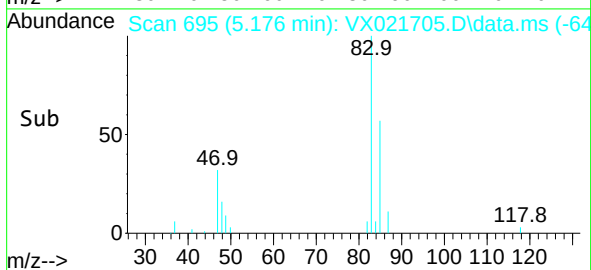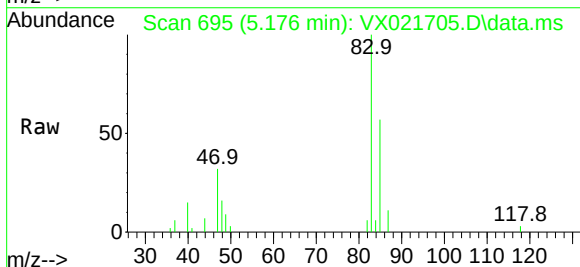






#31
Cyclohexane
Concen: 1.51 ug/l
RT: 5.629 min Scan# 772
Delta R.T. 0.082 min
Lab File: VX021705.D
Acq: 01 Apr 2021 14:14


Instrument :
MSVOA_X
ClientSampleId :
GWBR3-175-185-033121

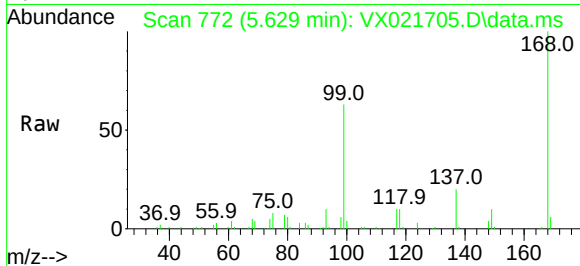



Tgt Ion: 56 Resp: 1622
Ion Ratio Lower Upper
56 100
69 145.7 25.3 37.9#
84 92.2 71.4 107.0




#33
1,2-Dichloroethane-d4
Concen: 52.70 ug/l
RT: 6.029 min Scan# 840
Delta R.T. -0.000 min
Lab File: VX021705.D
Acq: 01 Apr 2021 14:14

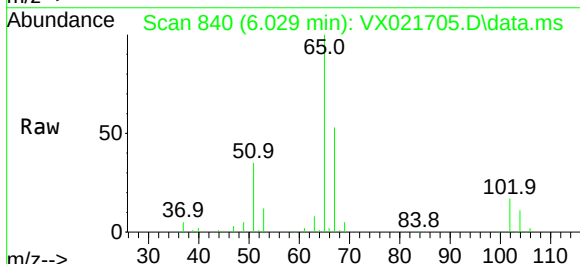


Tgt Ion: 65 Resp: 51548
Ion Ratio Lower Upper
65 100
67 51.0 0.0 105.4

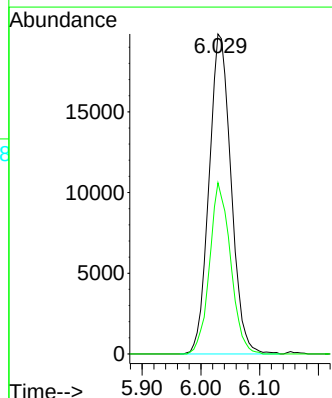



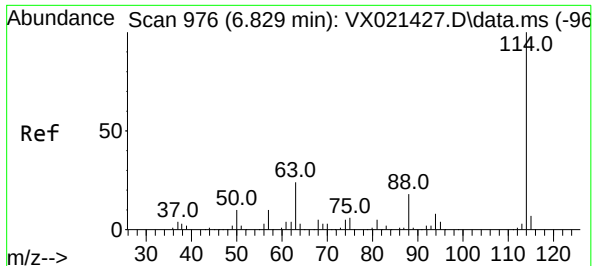


#34
1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 6.829 min Scan# 976
Delta R.T. 0.000 min
Lab File: VX021705.D
Acq: 01 Apr 2021 14:14

Instrument :
MSVOA_X
ClientSampleId :
GWBR3-175-185-033121







Tgt Ion:114 Resp: 110057
Ion Ratio Lower Upper
114 100
63 21.9 0.0 40.8
88 16.9 0.0 32.8

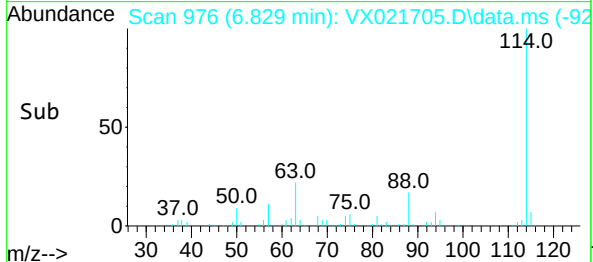

#35
Dibromofluoromethane
Concen: 51.52 ug/l
RT: 5.470 min Scan# 745
Delta R.T. 0.006 min
Lab File: VX021705.D
Acq: 01 Apr 2021 14:14

Tgt Ion:113 Resp: 40274
Ion Ratio Lower Upper
113 100
111 103.1 81.9 122.9
192 18.8 16.7 25.1

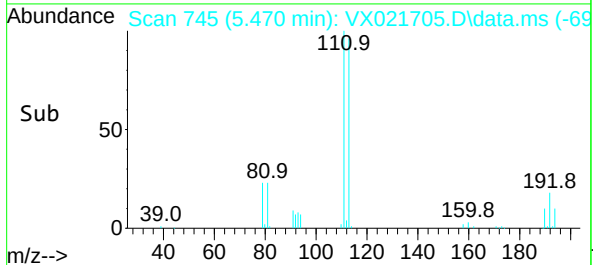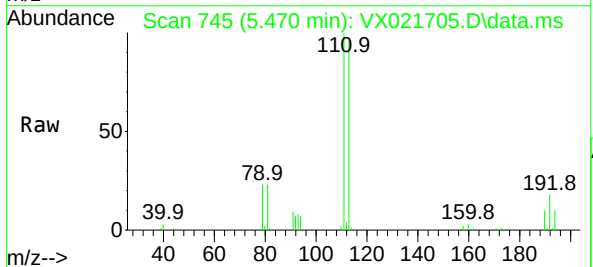

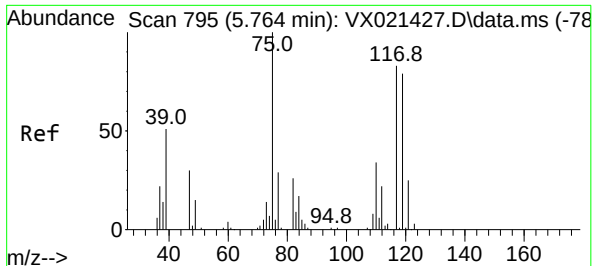

#36

1,1-Dichloropropene

Concen: 4.89 ug/l

RT: 5.635 min Scan# 773

Delta R.T. -0.129 min

Lab File: VX021705.D

Acq: 01 Apr 2021 14:14

Tgt Ion: 75 Resp: 5273

Ion Ratio Lower Upper

75 100

110 8.5 18.1 54.4#





77 0.0 25.3 37.9#

Instrument :

MSVOA_X

ClientSampleId :

GWBR3-175-185-033121

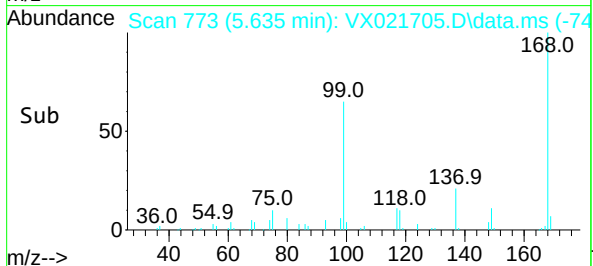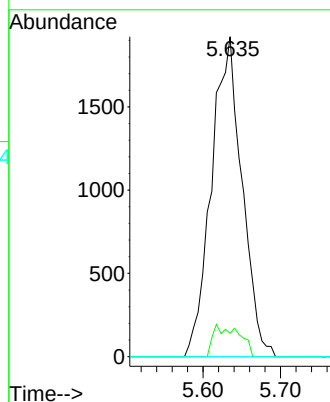

#38

Carbon Tetrachloride

Concen: 5.56 ug/l

RT: 5.629 min Scan# 772

Delta R.T. -0.123 min

Lab File: VX021705.D

Acq: 01 Apr 2021 14:14




Tgt Ion: 117 Resp: 6440


Ion Ratio Lower Upper

117 100

119 5.5 76.2 114.2#

121 0.0 24.8 37.2#

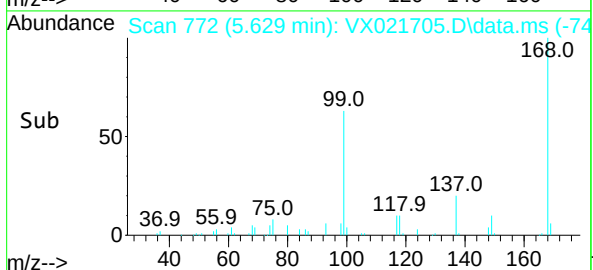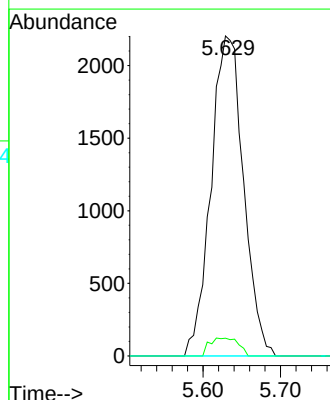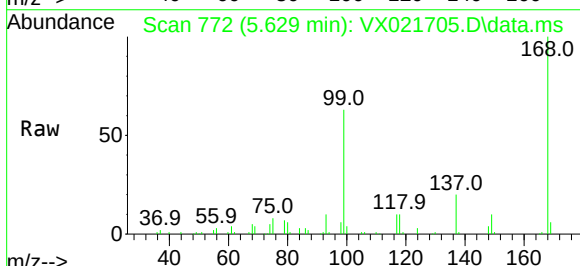



#39

Methylcyclohexane

Concen: 0.38 ug/l

RT: 7.194 min Scan# 1038

Delta R.T. -0.241 min

Lab File: VX021705.D


Acq: 01 Apr 2021 14:14

Instrument :




MSVOA_X

ClientSampleId :

GWBR3-175-185-033121



Tgt Ion:	83	Resp:	459
Ion	Ratio	Lower	Upper
83	100		
55	0.0	58.9	88.3#
98	228.1	38.1	57.1#

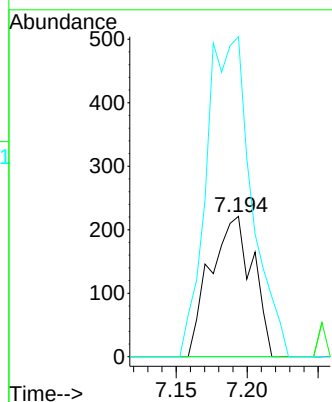

#40

Benzene

Concen: 0.29 ug/l




RT: 6.111 min Scan# 854


Delta R.T. 0.000 min

Lab File: VX021705.D

Acq: 01 Apr 2021 14:14

Tgt Ion:	78	Resp:	879
Ion	Ratio	Lower	Upper
78	100		
77	0.0	18.9	28.3#

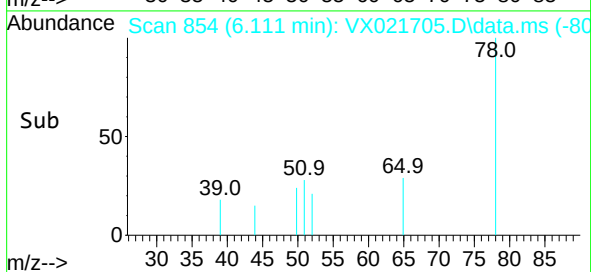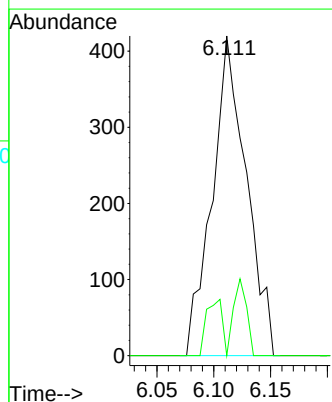



#42

1,2-Dichloroethane

Concen: 1.80 ug/l

RT: 6.164 min Scan# 863

Delta R.T. 0.006 min

Lab File: VX021705.D





Acq: 01 Apr 2021 14:14

Tgt Ion: 62 Resp: 2395

Ion Ratio Lower Upper

62 100

98 6.0 0.0 20.2



#44

Trichloroethene

Concen: 45.24 ug/l

RT: 7.188 min Scan# 1037

Delta R.T. -0.000 min

Lab File: VX021705.D




Acq: 01 Apr 2021 14:14


Tgt Ion: 130 Resp: 36561

Ion Ratio Lower Upper

130 100

95 102.1 0.0 198.0


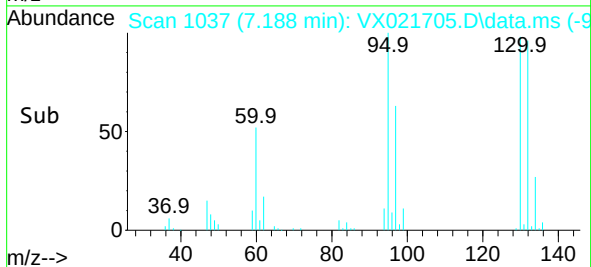

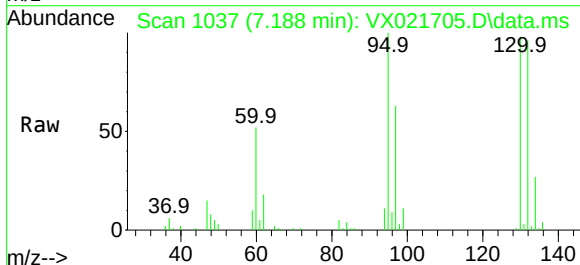




#48
Methyl methacrylate
Concen: 0.50 ug/l
RT: 7.753 min Scan# 1133
Delta R.T. 0.006 min
Lab File: VX021705.D
Acq: 01 Apr 2021 14:14




Instrument :
MSVOA_X
ClientSampleId :
GWBR3-175-185-033121


Tgt Ion: 41 Resp: 537
Ion Ratio Lower Upper
41 100
69 64.4 76.0 114.0#
39 71.5 44.6 67.0#

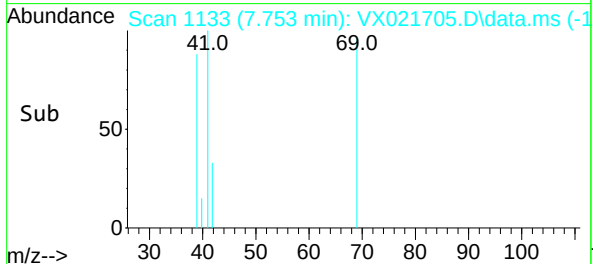

#49
1,4-Dioxane
Concen: 16.08 ug/l
RT: 7.723 min Scan# 1128
Delta R.T. 0.011 min
Lab File: VX021705.D
Acq: 01 Apr 2021 14:14

Tgt Ion: 88 Resp: 311
Ion Ratio Lower Upper
88 100
43 63.0 23.2 34.8#
58 66.6 55.0 82.4


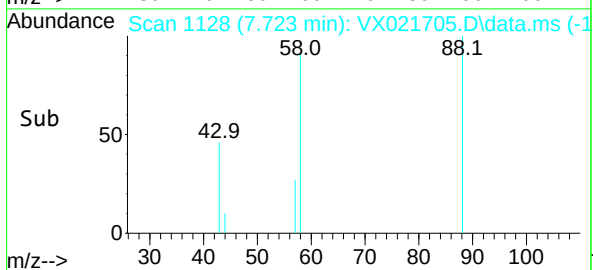

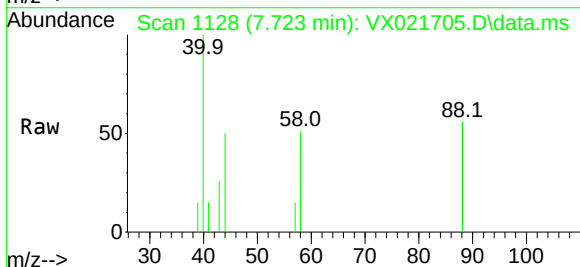




#50
Toluene-d8
Concen: 50.03 ug/l
RT: 8.694 min Scan# 1293
Delta R.T. 0.000 min
Lab File: VX021705.D
Acq: 01 Apr 2021 14:14




Instrument :
MSVOA_X
ClientSampleId :
GWBR3-175-185-033121


Tgt Ion: 98 Resp: 139374
Ion Ratio Lower Upper
98 100
100 64.4 51.9 77.9



#51
4-Methyl-2-Pentanone
Concen: 0.65 ug/l
RT: 8.623 min Scan# 1281
Delta R.T. 0.006 min
Lab File: VX021705.D
Acq: 01 Apr 2021 14:14

Tgt Ion: 43 Resp: 810
Ion Ratio Lower Upper
43 100
58 34.2 35.4 53.0#









#52
Toluene
Concen: 109.09 ug/l
RT: 8.765 min Scan# 1305
Delta R.T. -0.000 min
Lab File: VX021705.D
Acq: 01 Apr 2021 14:14




Instrument :
MSVOA_X
ClientSampleId :
GWBR3-175-185-033121


Tgt Ion: 92 Resp: 206327
Ion Ratio Lower Upper
92 100
91 175.8 137.1 205.7



#53
t-1,3-Dichloropropene
Concen: 2.24 ug/l
RT: 8.770 min Scan# 1306
Delta R.T. -0.253 min
Lab File: VX021705.D
Acq: 01 Apr 2021 14:14

Tgt Ion: 75 Resp: 2787
Ion Ratio Lower Upper
75 100
77 144.4 24.9 37.3#


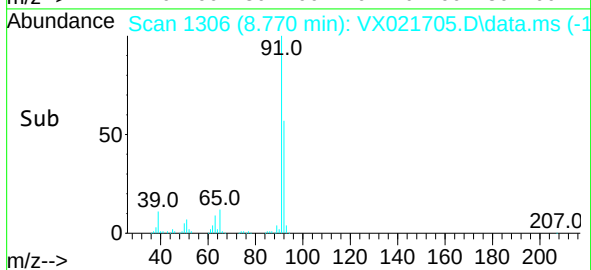




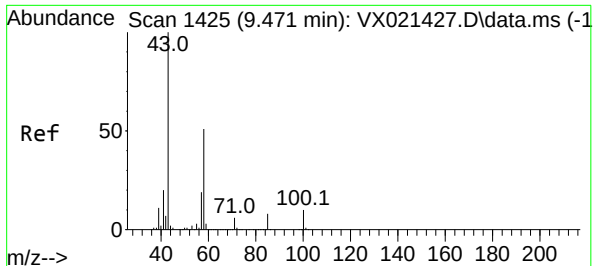

#59
2-Hexanone
Concen: 0.44 ug/l
RT: 9.465 min Scan# 1424
Delta R.T. -0.006 min
Lab File: VX021705.D
Acq: 01 Apr 2021 14:14




Instrument :
MSVOA_X
ClientSampleId :
GWBR3-175-185-033121


Tgt Ion: 43 Resp: 415
Ion Ratio Lower Upper
43 100
58 43.1 30.9 92.8

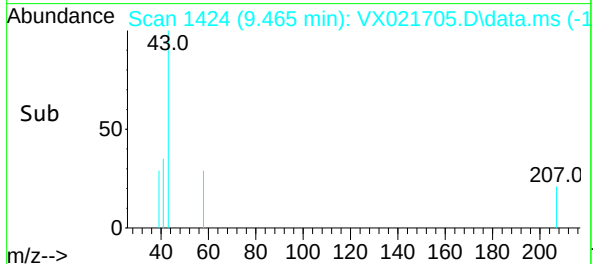

#62
4-Bromofluorobenzene
Concen: 53.54 ug/l
RT: 11.118 min Scan# 1705
Delta R.T. -0.000 min
Lab File: VX021705.D
Acq: 01 Apr 2021 14:14

Tgt Ion: 95 Resp: 57989
Ion Ratio Lower Upper
95 100
174 73.8 0.0 154.6
176 73.4 0.0 155.8


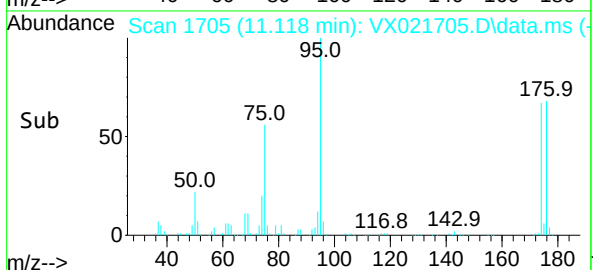

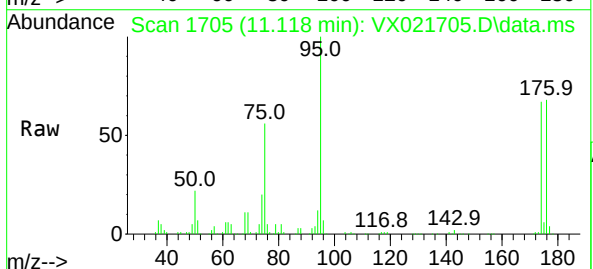


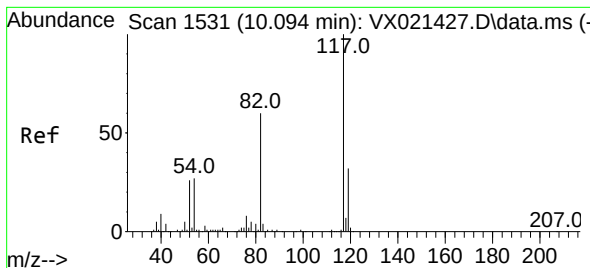

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 10.094 min Scan# 1531
Delta R.T. 0.000 min
Lab File: VX021705.D
Acq: 01 Apr 2021 14:14




Instrument :
MSVOA_X
ClientSampleId :
GWBR3-175-185-033121


Tgt Ion:117 Resp: 113734
Ion Ratio Lower Upper
117 100
82 60.7 47.4 71.2
119 32.5 26.6 39.8

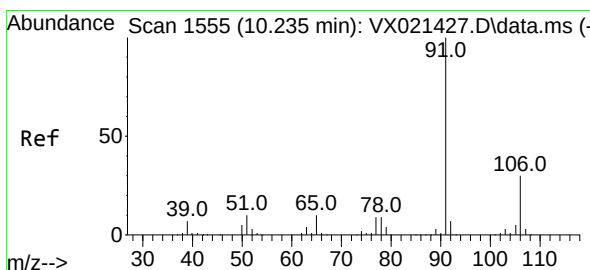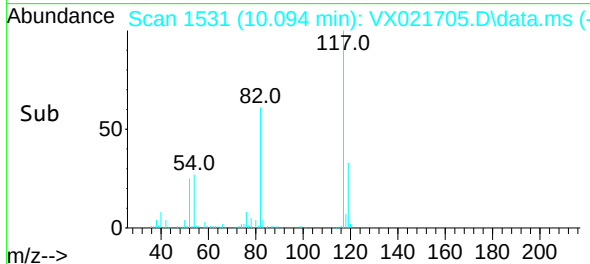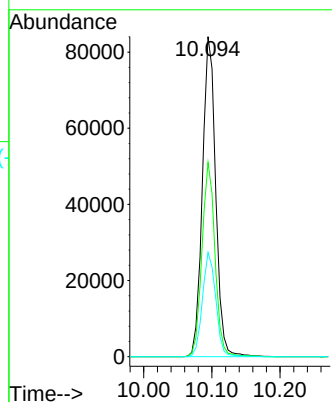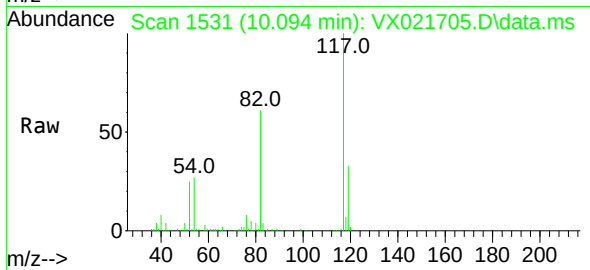

#67
Ethyl Benzene
Concen: 0.27 ug/l
RT: 10.235 min Scan# 1555
Delta R.T. 0.000 min
Lab File: VX021705.D
Acq: 01 Apr 2021 14:14

Tgt Ion: 91 Resp: 1138
Ion Ratio Lower Upper
91 100
106 30.7 24.6 37.0


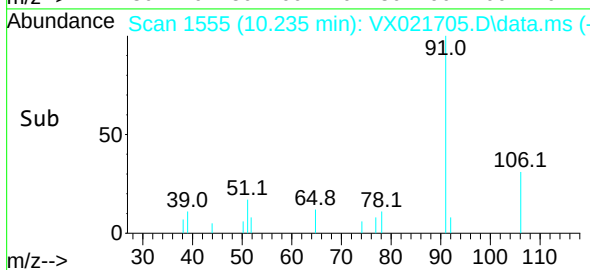
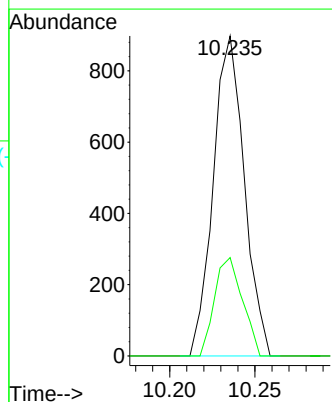
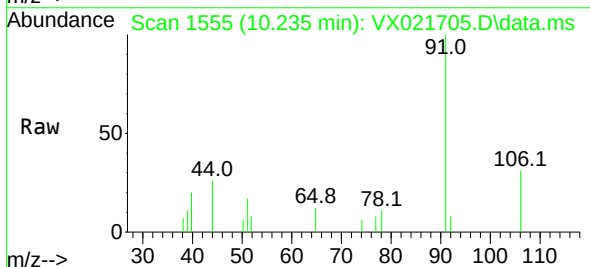




#68
m/p-Xylenes
Concen: 0.83 ug/l
RT: 10.341 min Scan# 1573
Delta R.T. 0.000 min
Lab File: VX021705.D
Acq: 01 Apr 2021 14:14




Instrument :
MSVOA_X
ClientSampleId :
GWBR3-175-185-033121


Tgt Ion:106 Resp: 1236
Ion Ratio Lower Upper
106 100
91 222.4 162.8 244.2



#69
o-Xylene
Concen: 0.42 ug/l
RT: 10.682 min Scan# 1631
Delta R.T. 0.000 min
Lab File: VX021705.D
Acq: 01 Apr 2021 14:14

Tgt Ion:106 Resp: 599
Ion Ratio Lower Upper
106 100
91 218.5 108.1 324.2


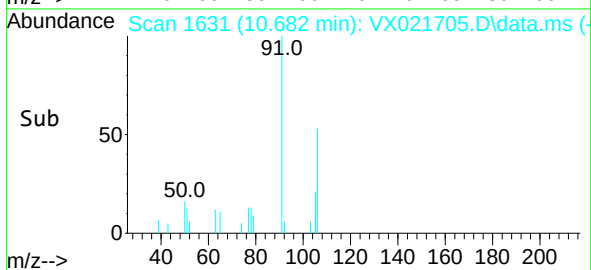

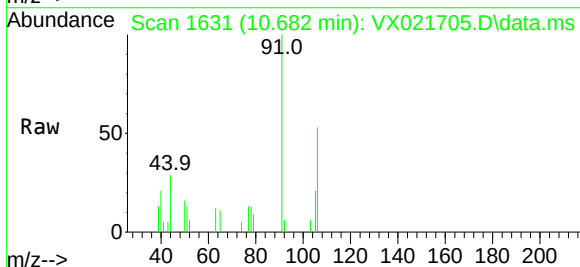




#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 12.059 min Scan# 1865
Delta R.T. 0.000 min
Lab File: VX021705.D
Acq: 01 Apr 2021 14:14




Instrument :
MSVOA_X
ClientSampleId :
GWBR3-175-185-033121


Tgt Ion:152 Resp: 53643
Ion Ratio Lower Upper
152 100
115 64.6 41.1 123.3
150 157.3 0.0 349.0



#74
N-ethyl acetate
Concen: 0.24 ug/l
RT: 10.894 min Scan# 1667
Delta R.T. 0.011 min
Lab File: VX021705.D
Acq: 01 Apr 2021 14:14

Tgt Ion: 43 Resp: 437
Ion Ratio Lower Upper
43 100
70 94.1 39.0 58.6#
55 83.1 21.5 32.3#
61 0.0 22.1 33.1#


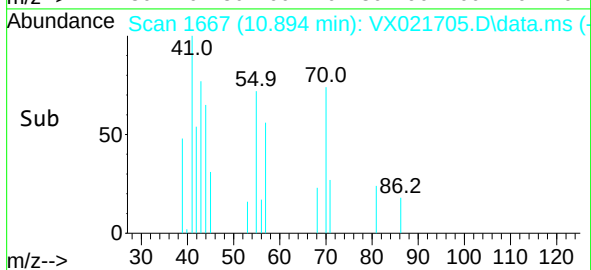

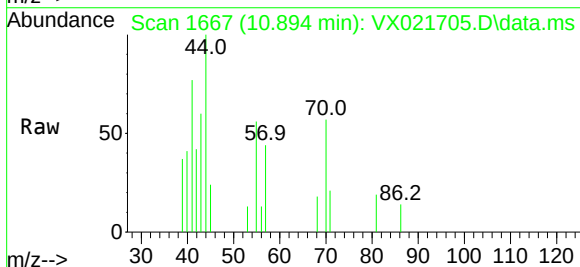




#76
1,2,3-Trichloropropane
Concen: 25.77 ug/l
RT: 11.118 min Scan# 1705
Delta R.T. -0.159 min
Lab File: VX021705.D
Acq: 01 Apr 2021 14:14




Instrument :
MSVOA_X
ClientSampleId :
GWBR3-175-185-033121


Tgt Ion: 75 Resp: 32183
Ion Ratio Lower Upper
75 100
77 1.1 19.1 57.5#

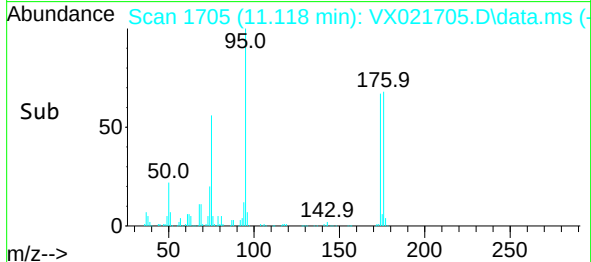

#81
trans-1,4-Dichloro-2-butene
Concen: 78.50 ug/l
RT: 11.118 min Scan# 1705
Delta R.T. 0.059 min
Lab File: VX021705.D
Acq: 01 Apr 2021 14:14

Tgt Ion: 75 Resp: 32183
Ion Ratio Lower Upper
75 100
53 0.0 74.5 111.7#
89 0.1 37.9 56.9#


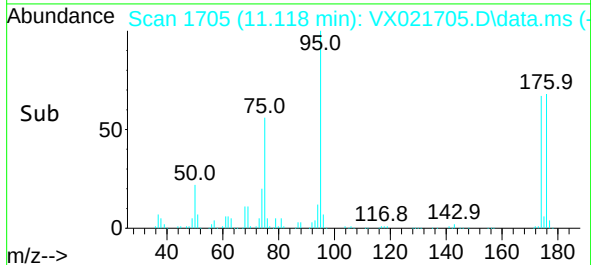

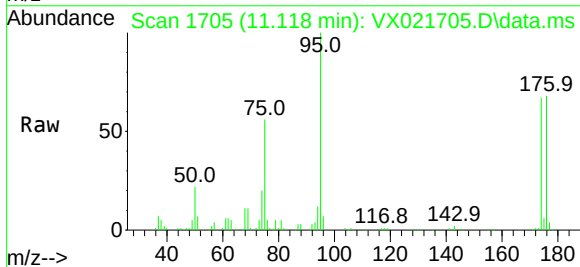




#84
1,2,4-Trimethylbenzene
Concen: 0.27 ug/l
RT: 11.789 min Scan# 1819
Delta R.T. -0.000 min
Lab File: VX021705.D
Acq: 01 Apr 2021 14:14

Instrument :
MSVOA_X
ClientSampleId :
GWBR3-175-185-033121

Tgt Ion:105 Resp: 887
Ion Ratio Lower Upper
105 100
120 34.0 22.4 67.3

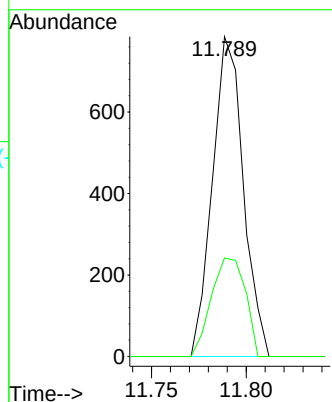

#95
Naphthalene
Concen: 0.32 ug/l
RT: 13.818 min Scan# 2164
Delta R.T. 0.000 min
Lab File: VX021705.D
Acq: 01 Apr 2021 14:14

Tgt Ion:128 Resp: 1122
Ion Ratio Lower Upper
128 100
127 11.9 10.3 15.5
129 7.8 8.8 13.2#

