

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX040121\
 Data File : VX021717.D
 Acq On : 01 Apr 2021 18:37
 Operator : JC/MD
 Sample : M1895-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-8

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M

Title : SW846 8260

Signal : TIC: VX021717.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.164	10	13	22	rVB	34027	35230	5.34%	1.224%
2	1.293	31	35	39	rBV	580717	659267	100.00%	22.897%
3	2.423	219	227	231	rBV	4606	8147	1.24%	0.283%
4	2.587	244	255	262	rBV2	4565	14296	2.17%	0.497%
5	3.164	344	353	364	rBV	46879	110323	16.73%	3.832%
6	5.464	729	744	757	rBV2	44828	131351	19.92%	4.562%
7	5.629	761	772	785	rBV	66281	180278	27.35%	6.261%
8	6.029	829	840	852	rBV	49803	131309	19.92%	4.560%
9	6.829	966	976	992	rBV	118651	305232	46.30%	10.601%
10	8.694	1286	1293	1301	rBV	238294	363945	55.20%	12.640%
11	10.094	1525	1531	1548	rVB	258707	349959	53.08%	12.154%
12	11.118	1699	1705	1716	rBV	208958	268727	40.76%	9.333%
13	12.059	1859	1865	1872	rBV	261718	321236	48.73%	11.157%




Sum of corrected areas: 2879300

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX040121\
Data File : VX021717.D
Acq On : 01 Apr 2021 18:37
Operator : JC/MD
Sample : M1895-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

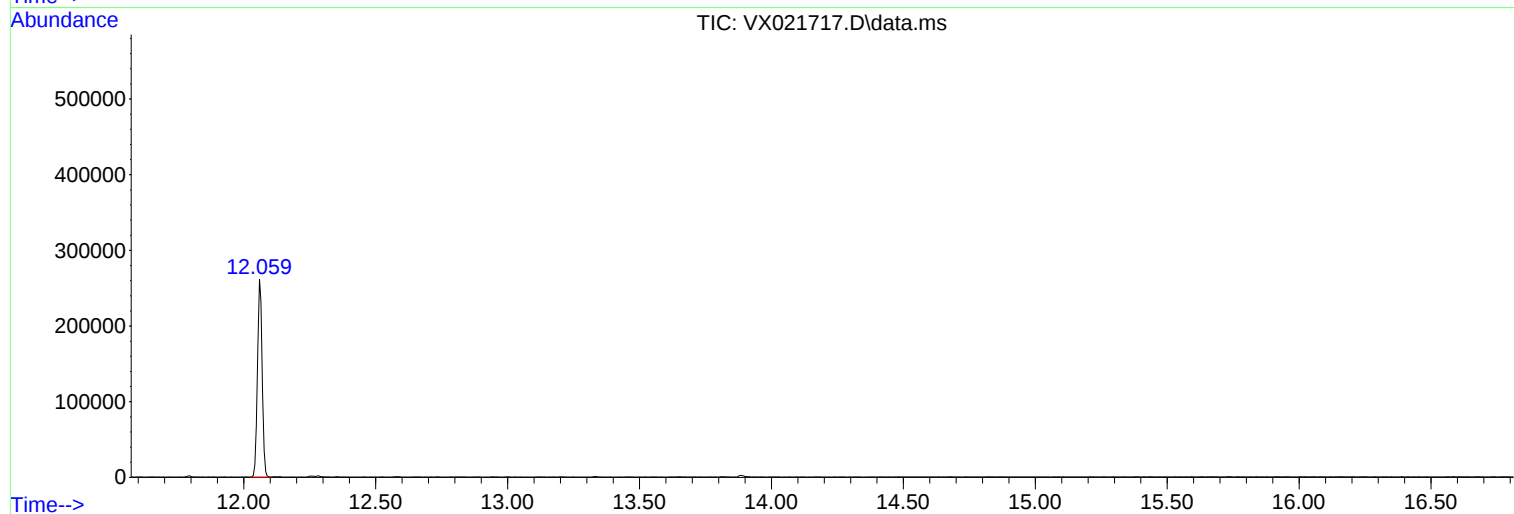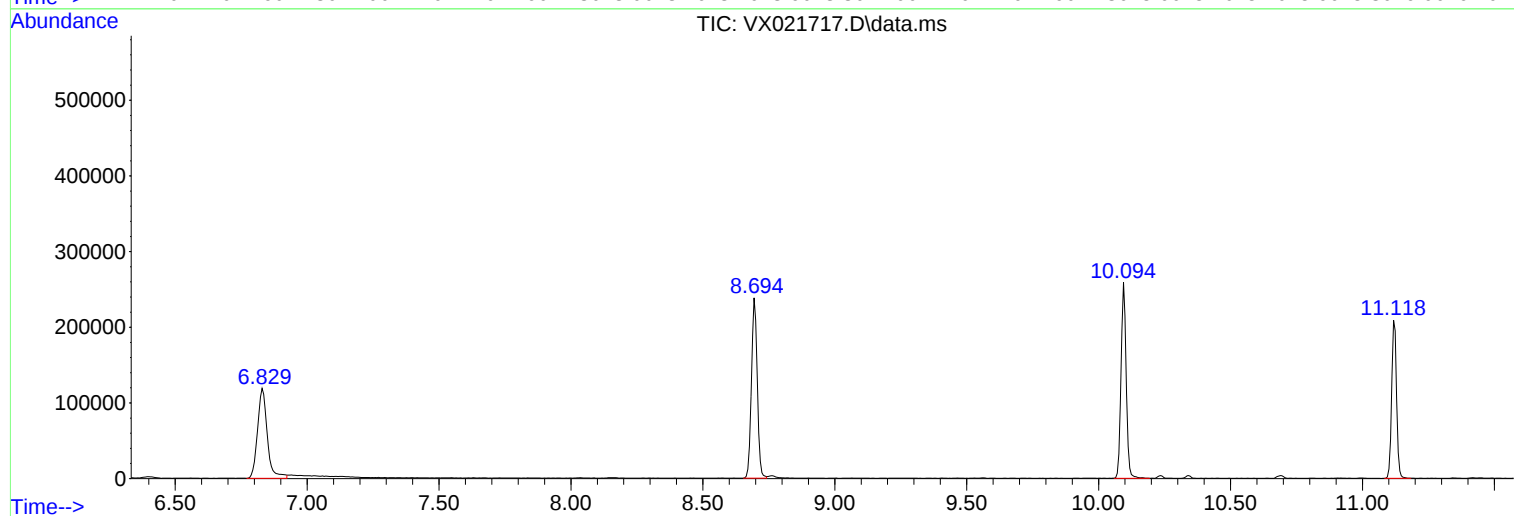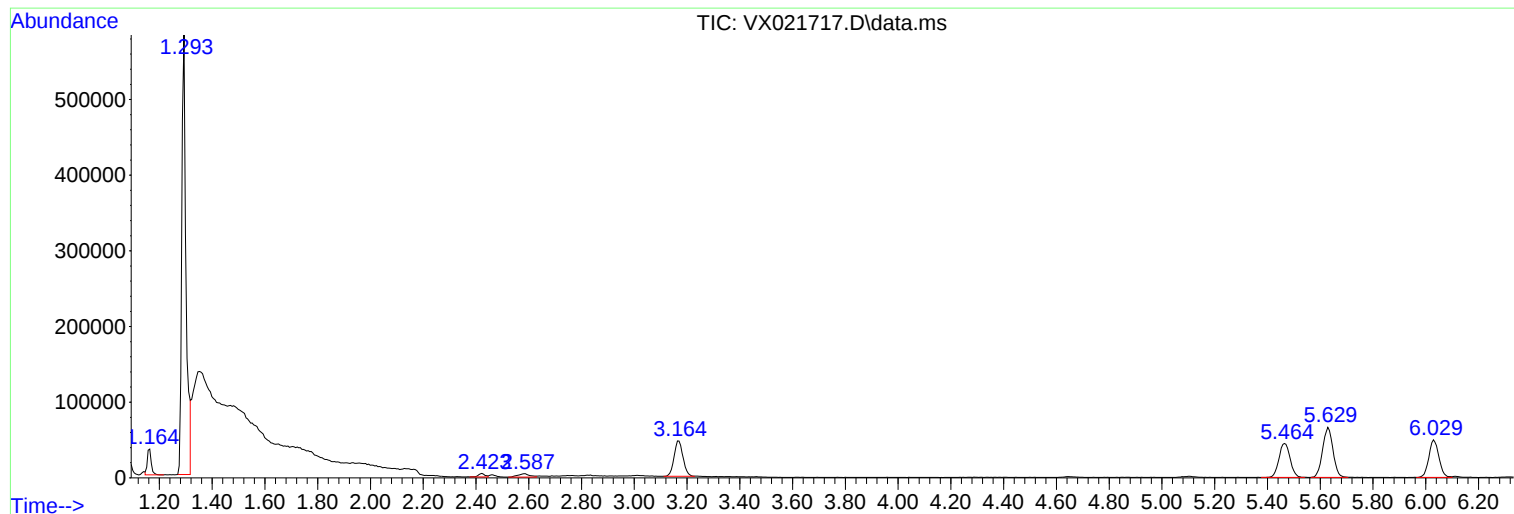

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX040121\
Data File : VX021717.D
Acq On : 01 Apr 2021 18:37
Operator : JC/MD
Sample : M1895-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-8










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Ethane, 1,1-difluoro- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.164	9.77 ug/l	35230	Pentafluorobenzene	5.629

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Ethane, 1,1-difluoro-	66	C2H4F2	000075-37-6	91
2			Propiolonitrile	51	C3HN	001070-71-9	3
3			Propane, 2,2-difluoro-	80	C3H6F2	000420-45-1	2
4			Difluoromethane	52	CH2F2	000075-10-5	1
5			2-Chloroethanol	80	C2H5ClO	000107-07-3	1

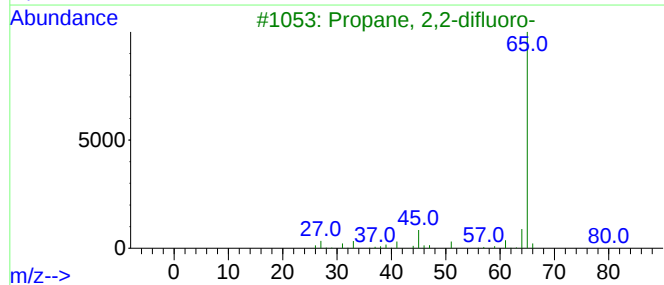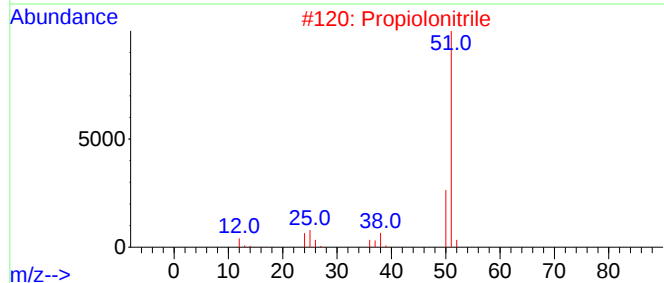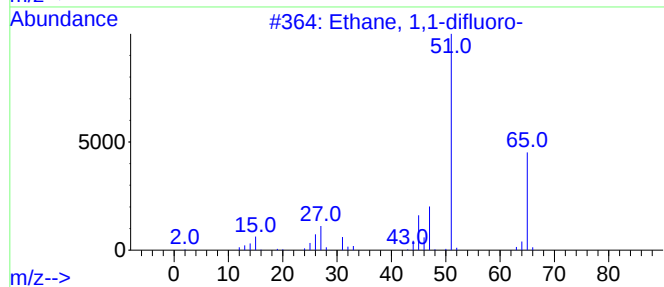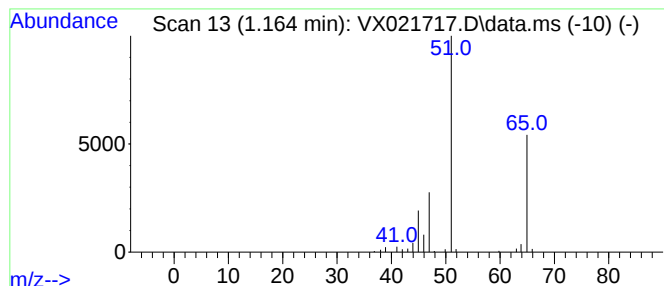

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX040121\
Data File : VX021717.D
Acq On : 01 Apr 2021 18:37
Operator : JC/MD
Sample : M1895-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-8










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Ethane, 1-chloro-1,1-difluoro- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.293	182.85 ug/l	659267	Pentafluorobenzene	5.629

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Ethane, 1-chloro-1,1-difluoro-	100	C2H3ClF2	000075-68-3	83
2			Propane, 2,2-difluoro-	80	C3H6F2	000420-45-1	9
3			Methanesulfinic acid	80	CH4O2S	017696-73-0	1
4			Benzene, 1-nitro-2-(p-methylphen...	247	C13H10FN03	028987-57-7	1
5			1-Propanol, 2-chloro-	94	C3H7ClO	000078-89-7	1

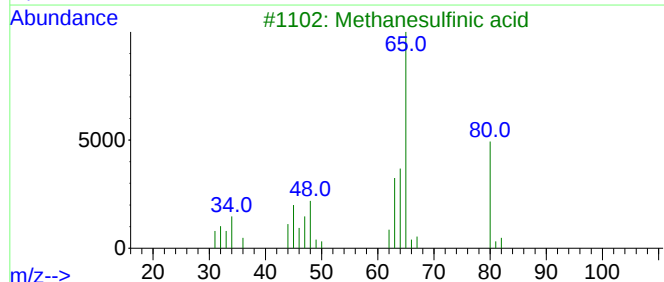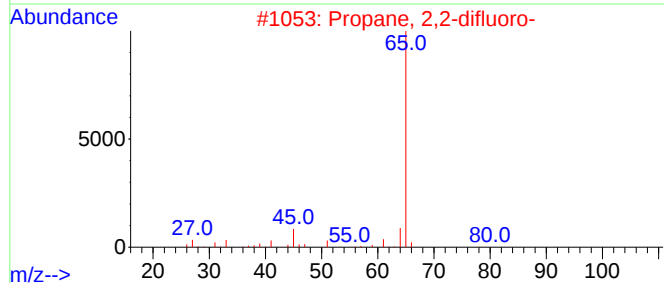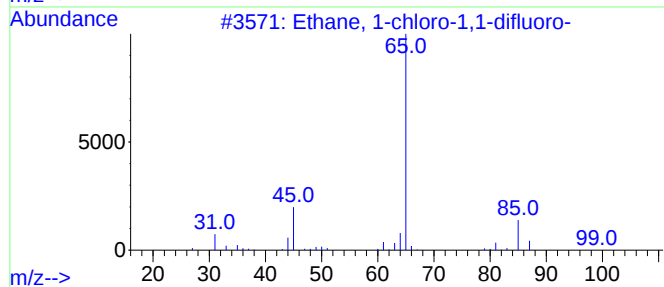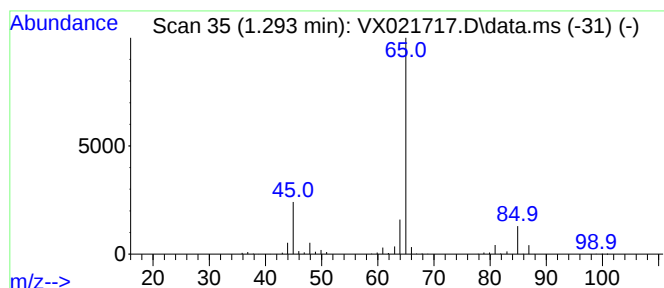

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX040121\
Data File : VX021717.D
Acq On : 01 Apr 2021 18:37
Operator : JC/MD
Sample : M1895-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Ethane, 1,1-dif...	1.164	9.8	ug/l	35230	1	5.629	180278	50.0
Ethane, 1-chlor...	1.293	182.8	ug/l	659267	1	5.629	180278	50.0