
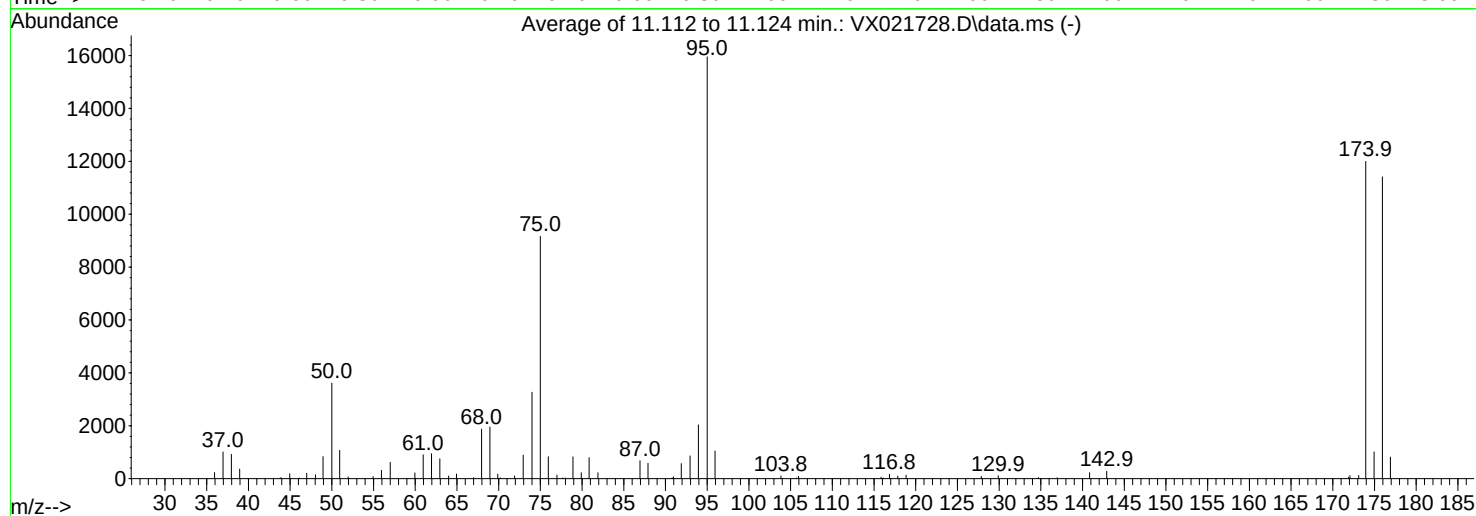


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX040121\
 Data File : VX021728.D
 Acq On : 02 Apr 2021 08:25
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M
 Title : SW846 8260
 Last Update : Wed Mar 24 12:25:26 2021

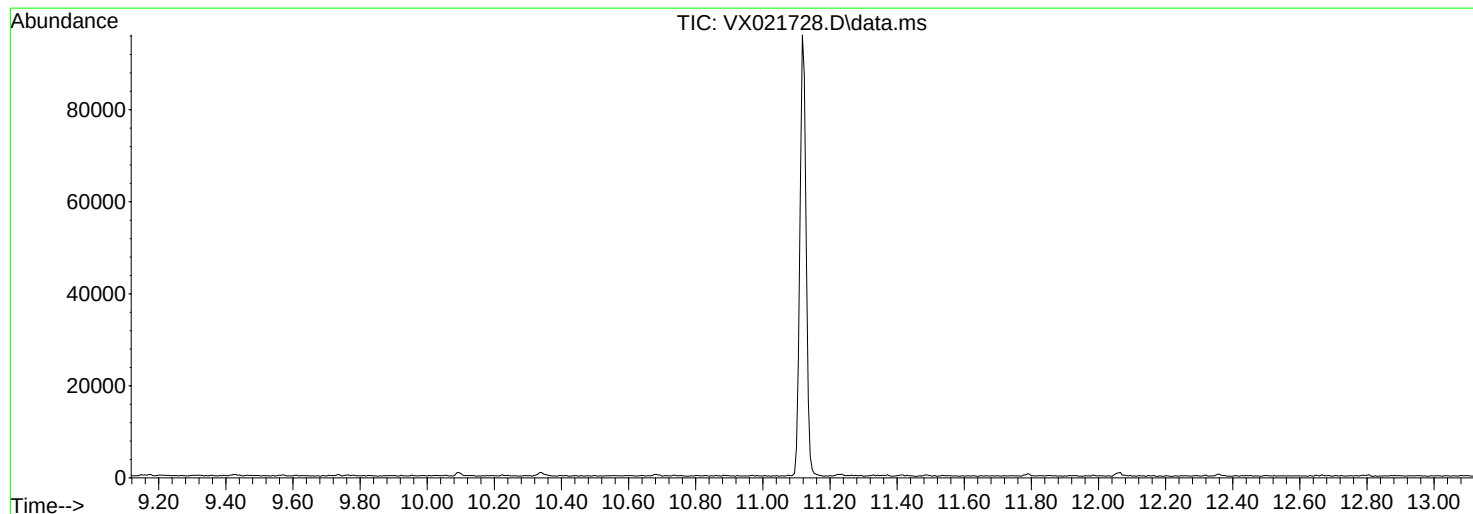

AutoFind: Scans 1704, 1705, 1706; Background Corrected with Scan 1698

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.7	3614	PASS
75	95	30	60	57.5	9165	PASS
95	95	100	100	100.0	15951	PASS
96	95	5	9	6.6	1050	PASS
173	174	0.00	2	1.0	122	PASS
174	95	50	100	75.2	12001	PASS
175	174	5	9	8.4	1011	PASS
176	174	95	101	95.1	11411	PASS
177	176	5	9	7.2	819	PASS