

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX040122\
 Data File : VX027904.D
 Acq On : 02 Apr 2022 00:53
 Operator : JC/MD
 Sample : N2172-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-3R

Quant Time: Apr 02 07:32:35 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032922W.M
 Quant Title : SW846 8260
 QLast Update : Wed Mar 30 04:39:27 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.556	168	82869	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	6.769	114	138925	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	124514	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	57967	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	56275	52.631	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	= 105.260%	
35) Dibromofluoromethane	5.385	113	47488	52.957	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	= 105.920%	
50) Toluene-d8	8.653	98	154024	48.818	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	= 97.640%	
62) 4-Bromofluorobenzene	11.079	95	60969	45.472	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	= 90.940%	
Target Compounds						
16) Acetone	2.374	43	692	1.462	ug/l	# 78


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX040122\
Data File : VX027904.D
Acq On : 02 Apr 2022 00:53
Operator : JC/MD
Sample : N2172-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-3R


Quant Time: Apr 02 07:32:35 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032922W.M
Quant Title : SW846 8260
QLast Update : Wed Mar 30 04:39:27 2022
Response via : Initial Calibration

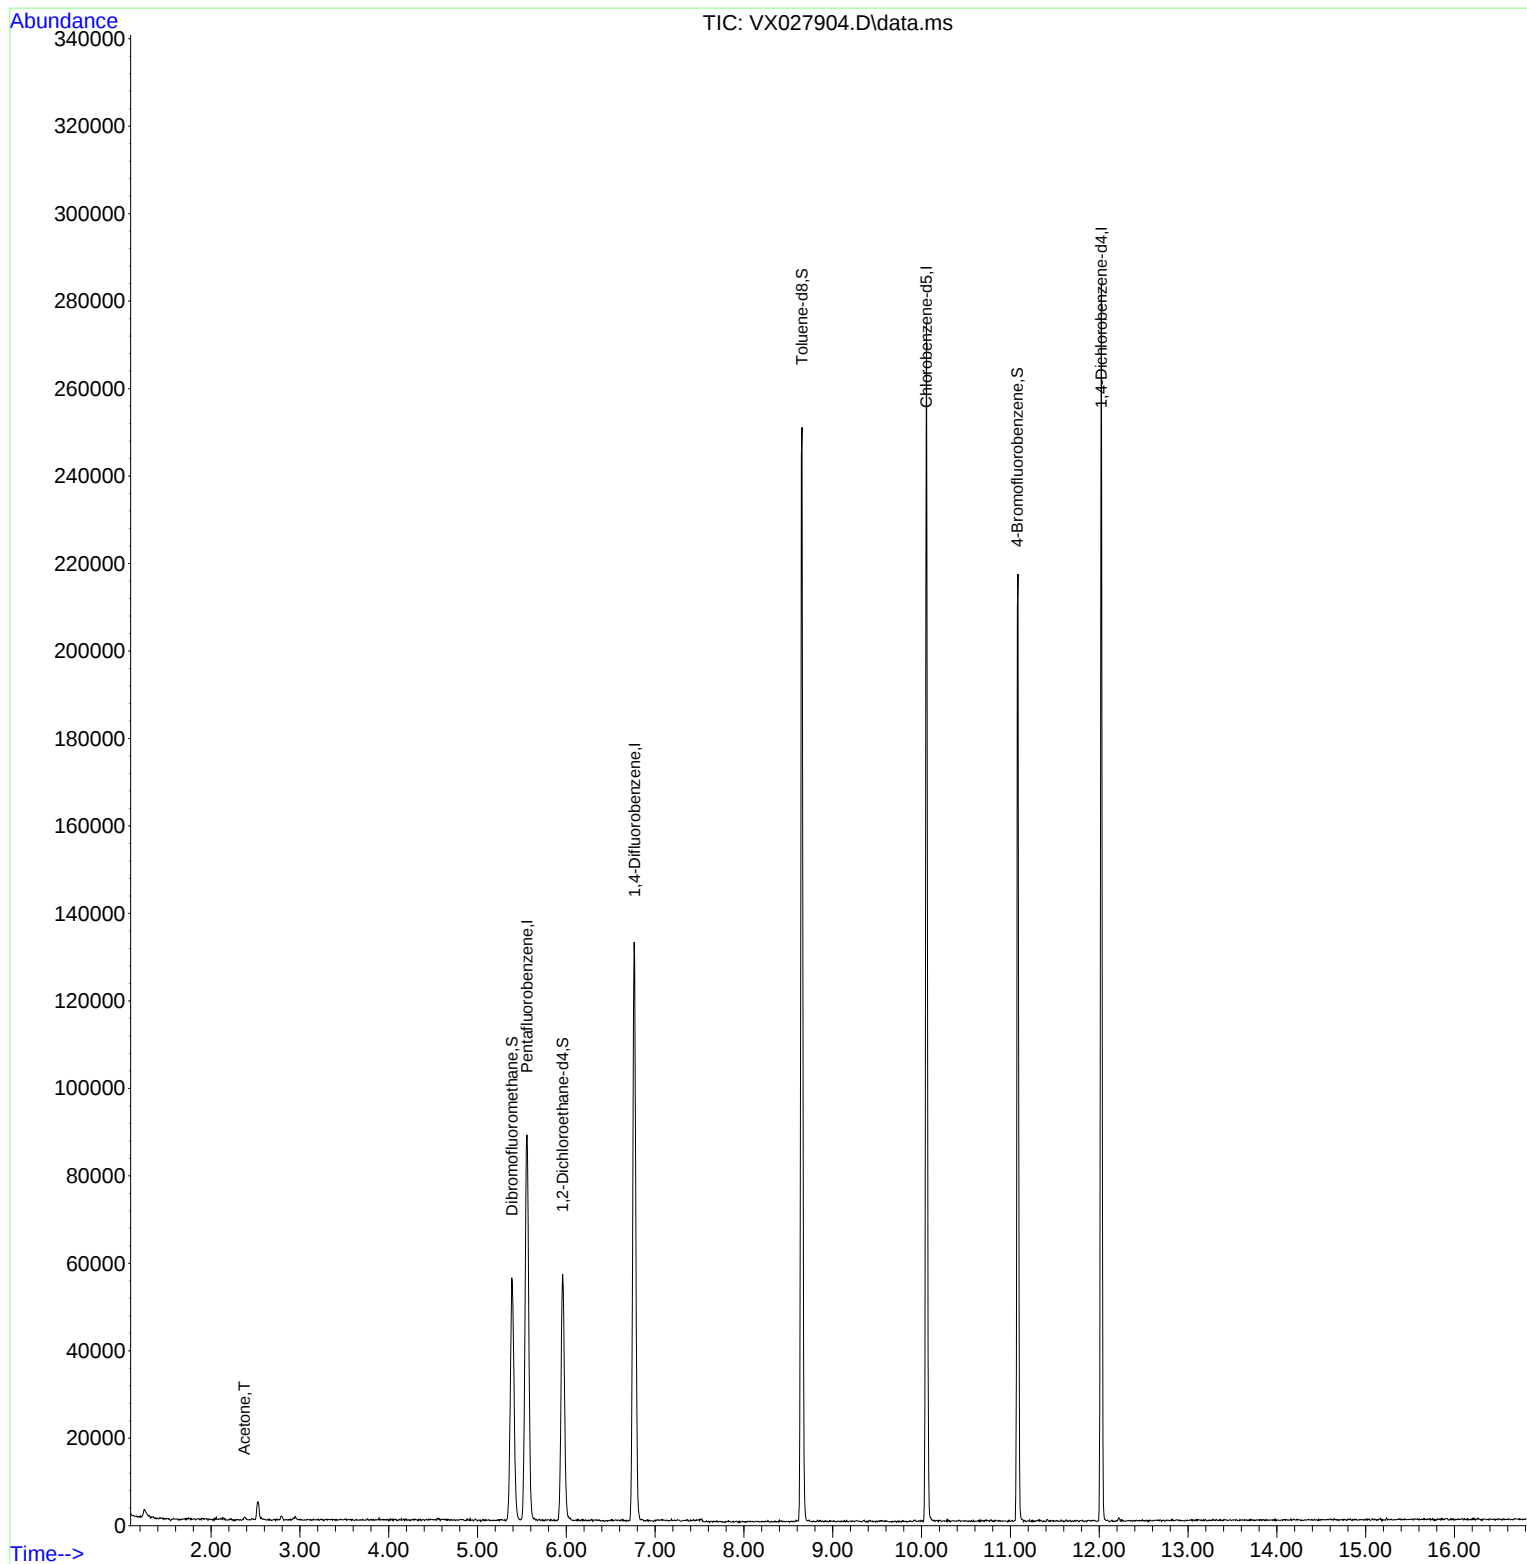



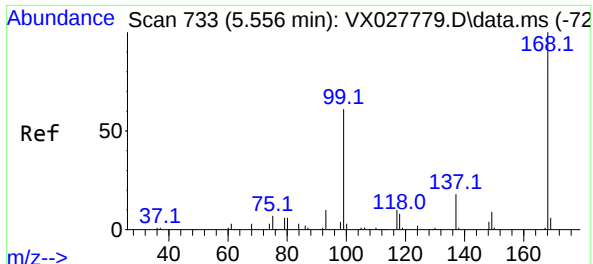


#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX027904.D
Acq: 02 Apr 2022 00:53

Instrument :
MSVOA_X
ClientSampleId :
MW-3R



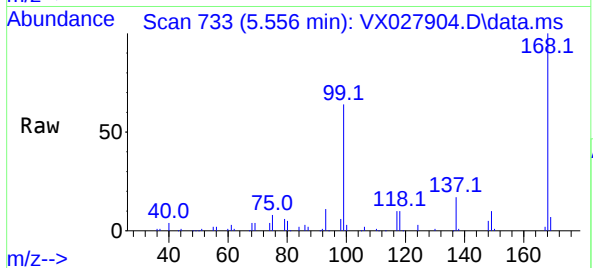



Tgt Ion:168 Resp: 82869
Ion Ratio Lower Upper
168 100
99 63.7 41.7 62.5#

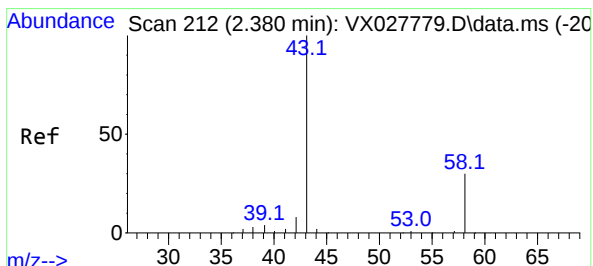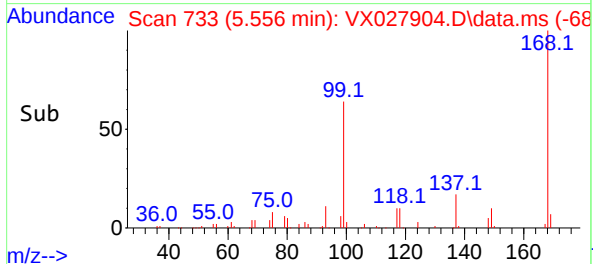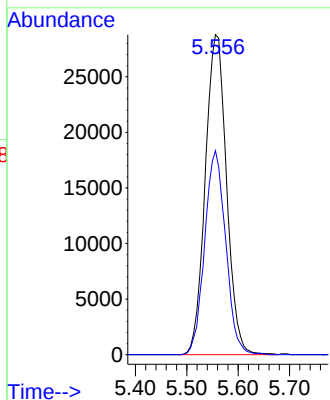

#16
Acetone
Concen: 1.462 ug/l
RT: 2.374 min Scan# 211
Delta R.T. -0.006 min
Lab File: VX027904.D
Acq: 02 Apr 2022 00:53

Tgt Ion: 43 Resp: 692
Ion Ratio Lower Upper
43 100
58 23.0 28.8 43.2#


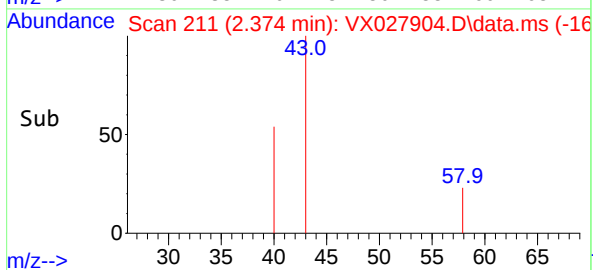
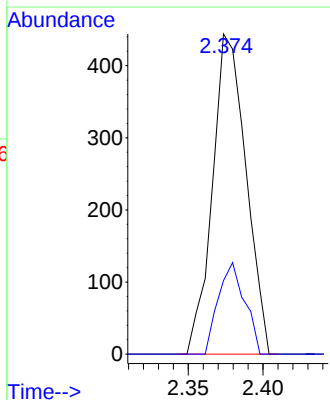
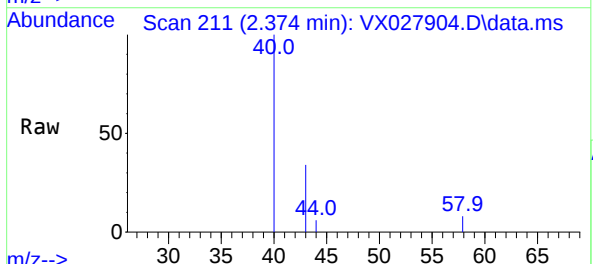


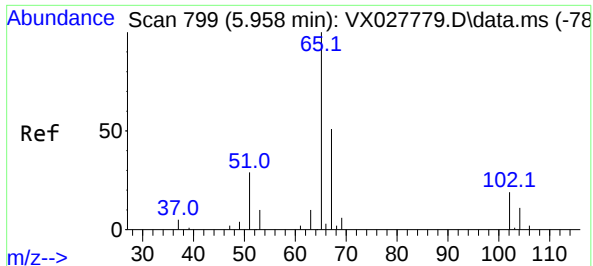

#33
1,2-Dichloroethane-d4
Concen: 52.631 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.000 min
Lab File: VX027904.D
Acq: 02 Apr 2022 00:53




Instrument :
MSVOA_X
ClientSampleId :
MW-3R


Tgt Ion: 65 Resp: 56275
Ion Ratio Lower Upper
65 100
67 52.4 0.0 107.4

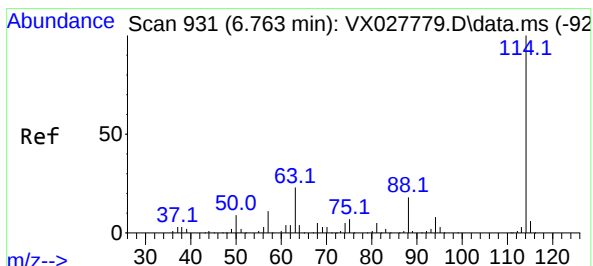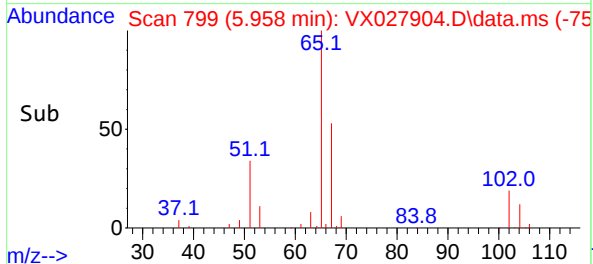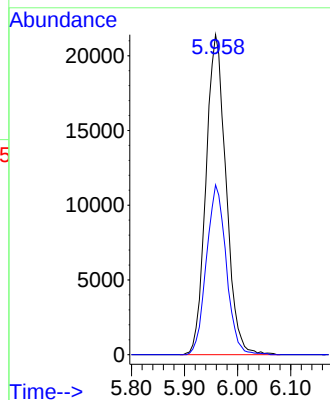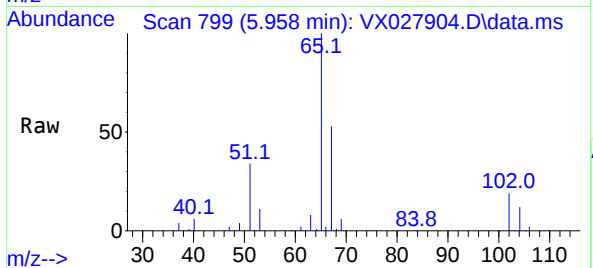

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.769 min Scan# 932
Delta R.T. 0.006 min
Lab File: VX027904.D
Acq: 02 Apr 2022 00:53


Tgt Ion: 114 Resp: 138925
Ion Ratio Lower Upper
114 100
63 18.7 0.0 36.8
88 15.7 0.0 32.4

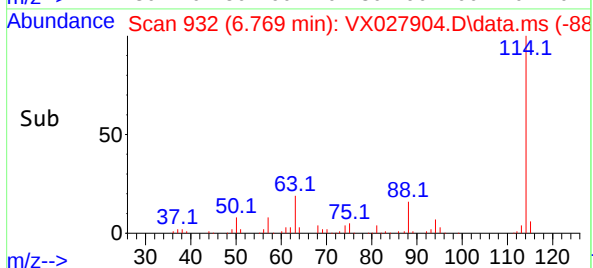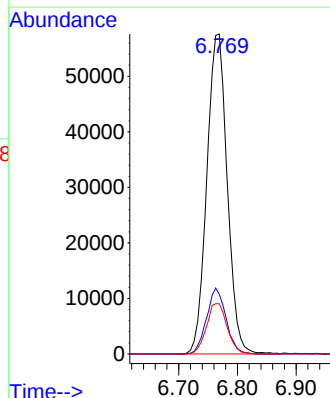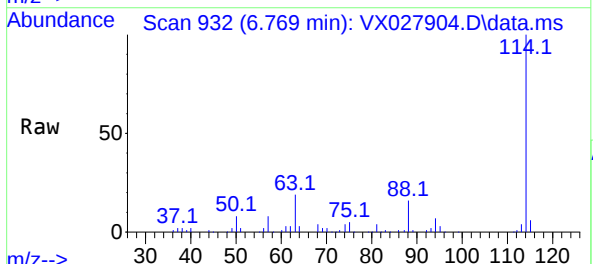

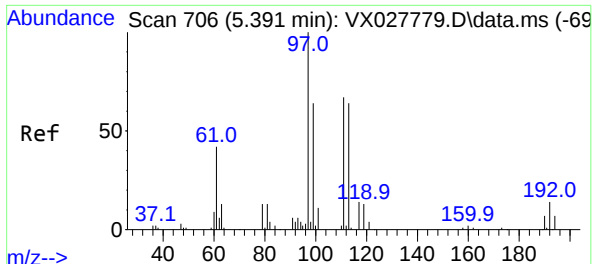




#35
Dibromofluoromethane
Concen: 52.957 ug/l
RT: 5.385 min Scan# 706
Delta R.T. -0.006 min
Lab File: VX027904.D
Acq: 02 Apr 2022 00:53

Instrument :
MSVOA_X
ClientSampleId :
MW-3R

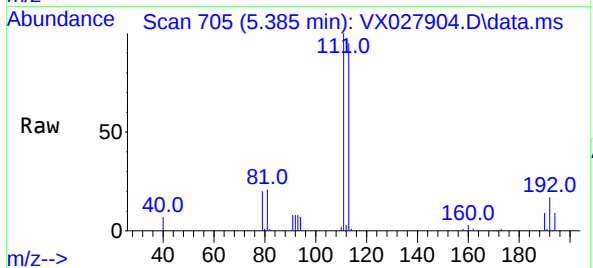

Tgt Ion:113 Resp: 47488




Ion	Ratio	Lower	Upper
113	100		
111	103.4	82.8	124.2
192	18.1	16.9	25.3

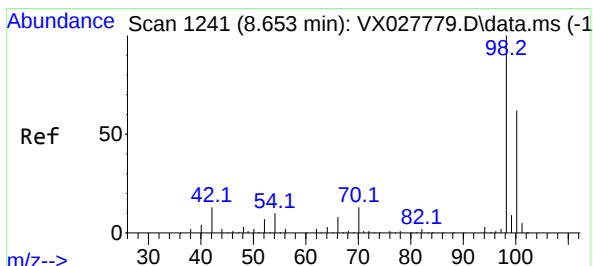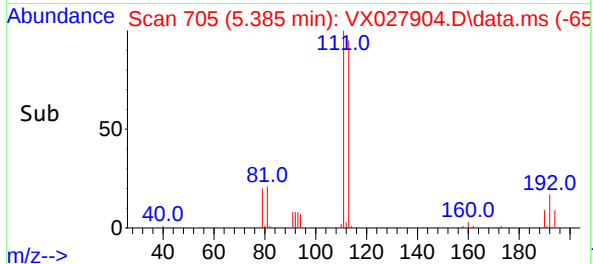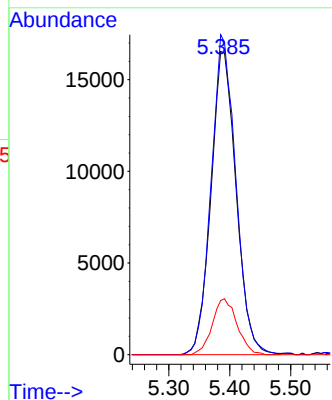


#50
Toluene-d8
Concen: 48.818 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. -0.000 min
Lab File: VX027904.D
Acq: 02 Apr 2022 00:53

Tgt Ion: 98 Resp: 154024

Ion	Ratio	Lower	Upper
98	100		
100	65.6	52.6	78.8


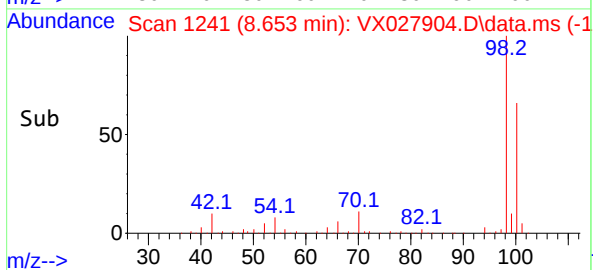
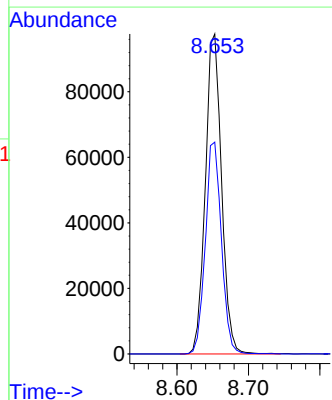
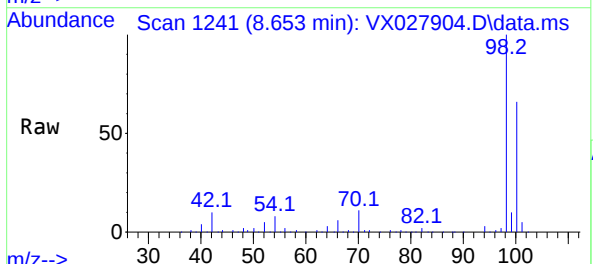


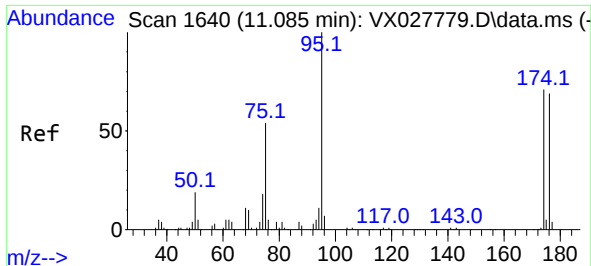

#62
4-Bromofluorobenzene
Concen: 45.472 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.006 min
Lab File: VX027904.D
Acq: 02 Apr 2022 00:53




Instrument :
MSVOA_X
ClientSampleId :
MW-3R

Tgt Ion: 95 Resp: 60969
Ion Ratio Lower Upper
95 100
174 76.2 0.0 163.0
176 74.2 0.0 155.0

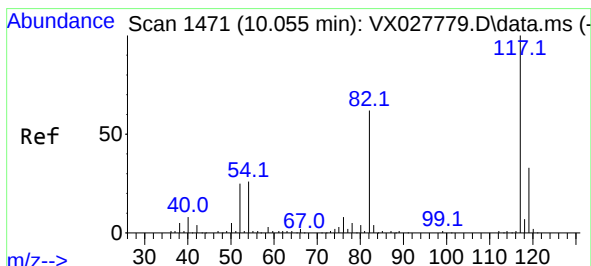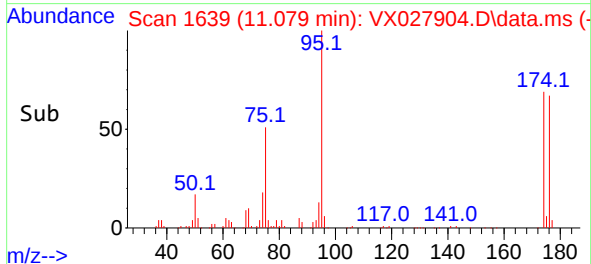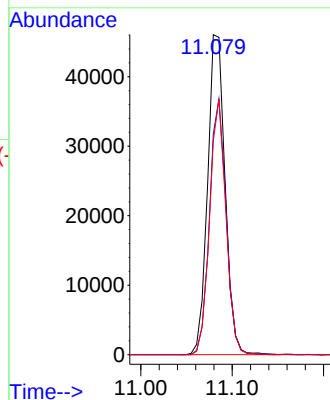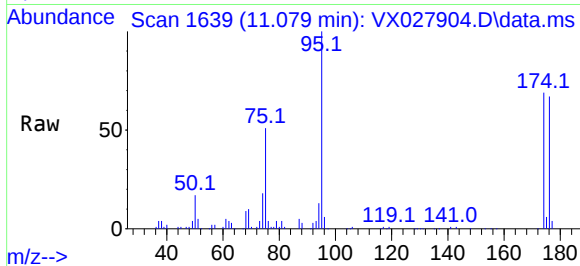


#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX027904.D
Acq: 02 Apr 2022 00:53


Tgt Ion: 117 Resp: 124514
Ion Ratio Lower Upper
117 100
82 53.0 41.8 62.8
119 32.1 24.8 37.2

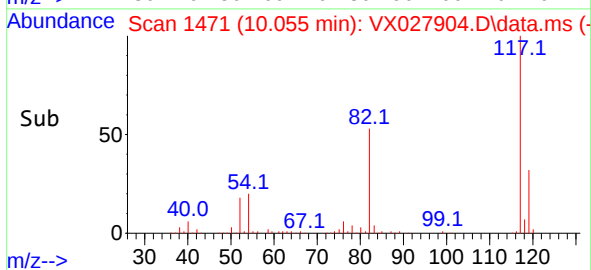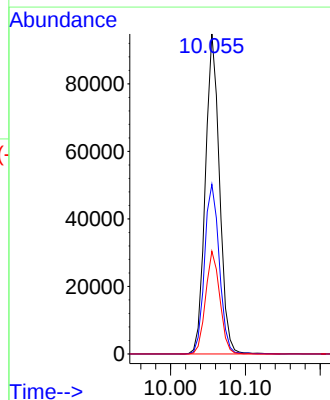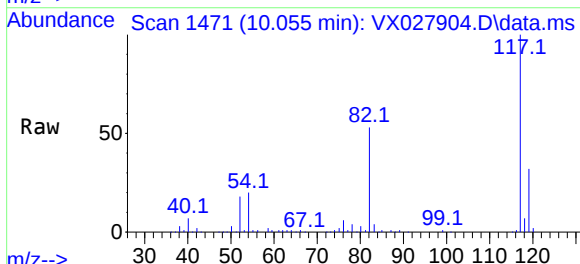


Abundance Scan 1794 (12.024 min): VX027779.D\data.ms (-

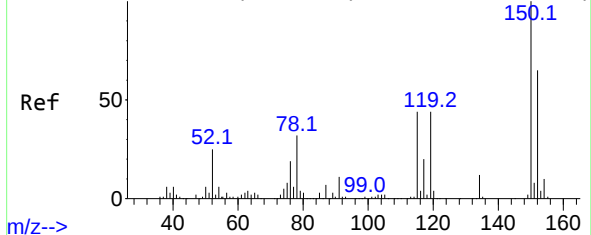

Abundance Scan 1794 (12.024 min): VX027904.D\data.ms (-

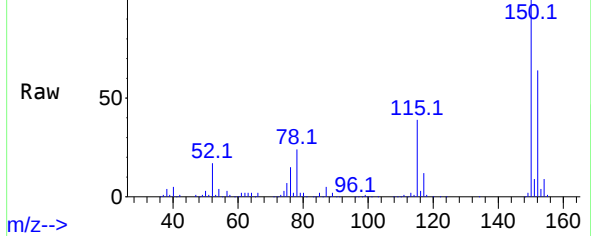

Abundance Scan 1794 (12.024 min): VX027904.D\data.ms (-

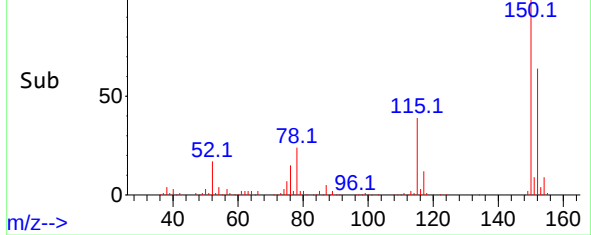

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX027904.D
Acq: 02 Apr 2022 00:53

Instrument :
MSVOA_X
ClientSampleId :
MW-3R

Tgt Ion	Ratio	Lower	Upper
152	100		
115	61.3	37.5	112.7
150	156.7	0.0	338.2

