

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX040122\
 Data File : VX027890.D
 Acq On : 01 Apr 2022 18:42
 Operator : JC/MD
 Sample : N2074-09RE
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 RW8-MW01S-20220320RE

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032922W.M

Title : SW846 8260

Signal : TIC: VX027890.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	22	26	36	rBV2	3968	7952	1.83%	0.328%
2	2.532	230	237	245	rVB	5231	10372	2.38%	0.428%
3	5.019	638	645	657	rBV3	3548	10776	2.48%	0.444%
4	5.391	695	706	719	rBV	54429	156393	35.95%	6.451%
5	5.556	723	733	747	rVV	85607	244328	56.16%	10.077%
6	5.958	789	799	813	rBV	60873	161049	37.02%	6.643%
7	6.763	923	931	944	rVB	139421	328248	75.45%	13.539%
8	8.653	1234	1241	1254	rBV	274430	435055	100.00%	17.944%
9	10.055	1465	1471	1481	rBV	300792	399086	91.73%	16.461%
10	11.085	1634	1640	1648	rBV	240811	305554	70.23%	12.603%
11	12.024	1789	1794	1803	rVB	300580	365685	84.05%	15.083%




Sum of corrected areas: 2424498

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX040122\
Data File : VX027890.D
Acq On : 01 Apr 2022 18:42
Operator : JC/MD
Sample : N2074-09RE
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RW8-MW01S-20220320RE

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032922W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

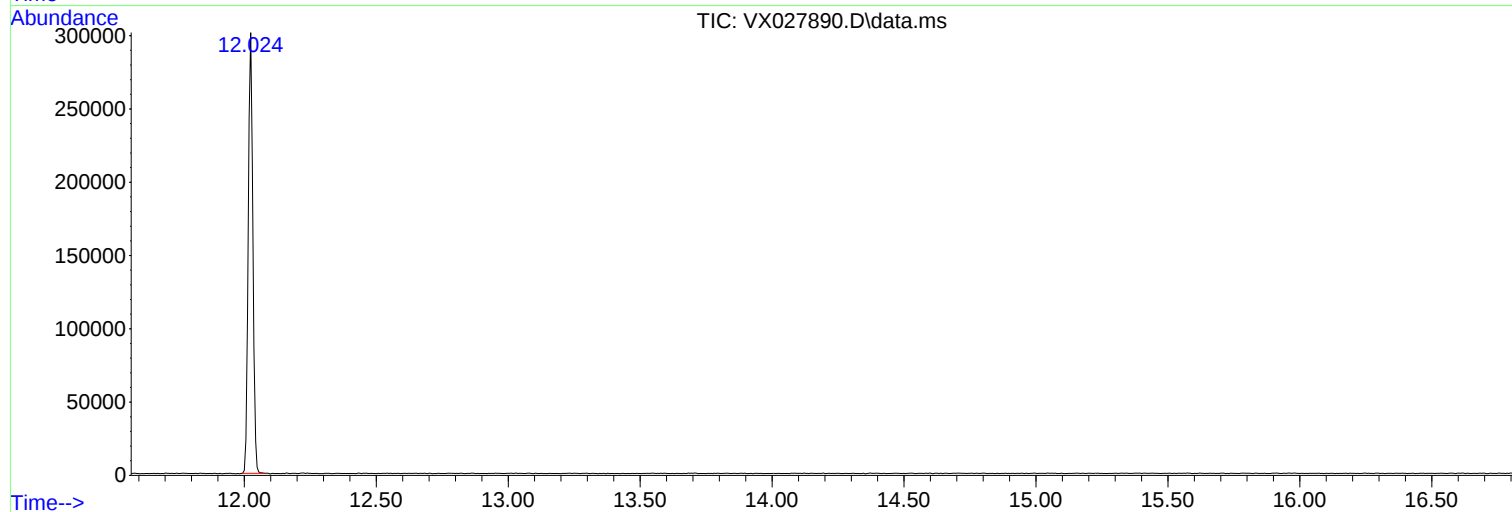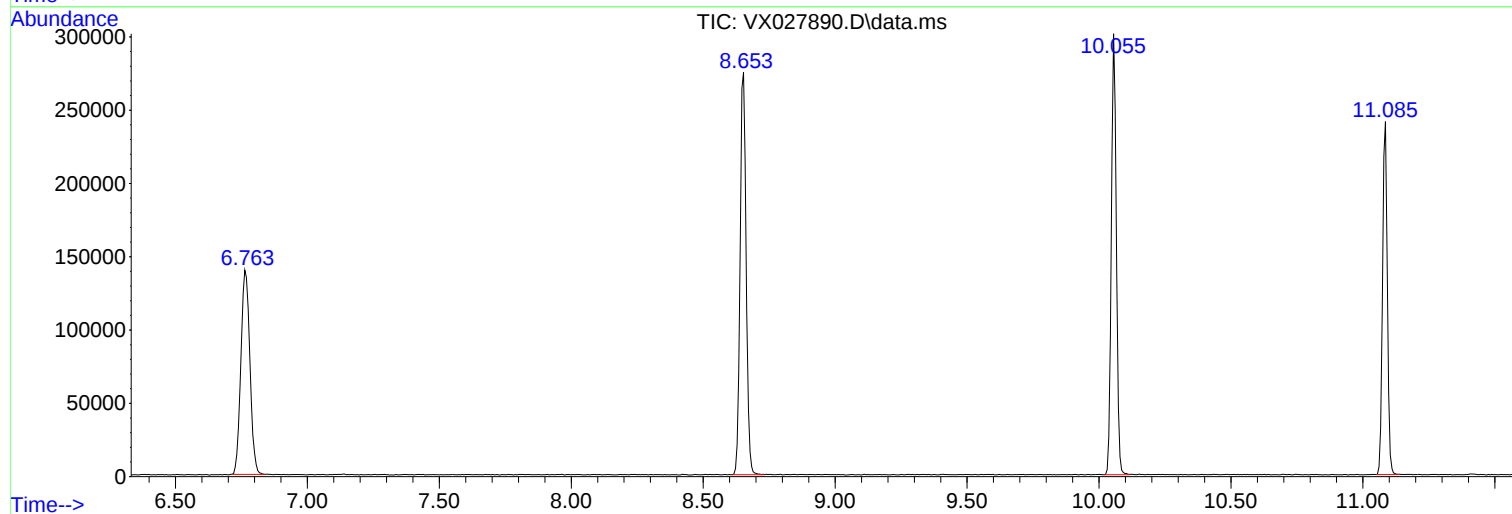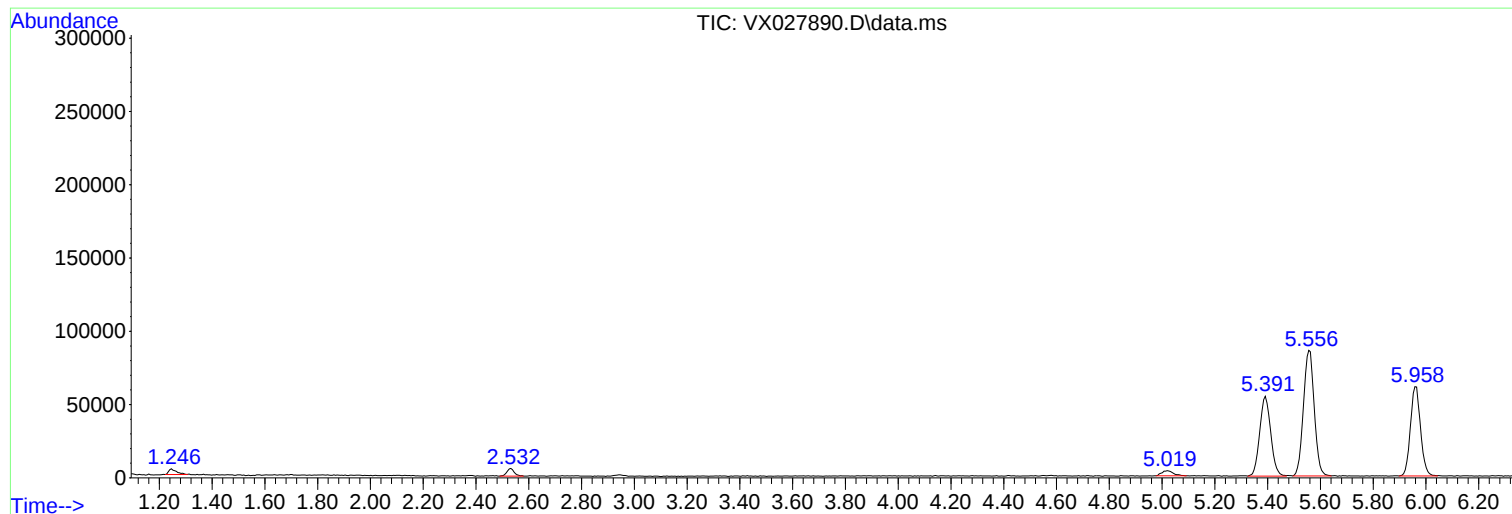

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX040122\
Data File : VX027890.D
Acq On : 01 Apr 2022 18:42
Operator : JC/MD
Sample : N2074-09RE
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RW8-MW01S-20220320RE

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032922W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX040122\
Data File : VX027890.D
Acq On : 01 Apr 2022 18:42
Operator : JC/MD
Sample : N2074-09RE
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RW8-MW01S-20220320RE

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032922W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc