

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX040122\  
Data File : VX027906.D  
Acq On : 02 Apr 2022 01:39  
Operator : JC/MD  
Sample : N2172-05  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 35 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-6R

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X032922W.M

Title : SW846 8260

Signal : TIC: VX027906.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 1.172       | 11            | 14          | 22           | rVB      | 176485         | 149077        | 34.00%          | 5.875%        |
| 2         | 2.526       | 231           | 236         | 247          | rVB      | 4845           | 9179          | 2.09%           | 0.362%        |
| 3         | 5.391       | 695           | 706         | 720          | rBV      | 53910          | 155900        | 35.56%          | 6.144%        |
| 4         | 5.556       | 723           | 733         | 747          | rVV      | 86506          | 241135        | 55.00%          | 9.502%        |
| 5         | 5.964       | 789           | 800         | 818          | rVB2     | 58638          | 158811        | 36.22%          | 6.258%        |
| 6         | 6.763       | 922           | 931         | 943          | rBV      | 136884         | 328545        | 74.94%          | 12.947%       |
| 7         | 8.653       | 1234          | 1241        | 1253         | rBV      | 278214         | 438407        | 100.00%         | 17.276%       |
| 8         | 10.055      | 1464          | 1471        | 1480         | rBV      | 293682         | 397735        | 90.72%          | 15.674%       |
| 9         | 11.085      | 1634          | 1640        | 1647         | rBV      | 231943         | 302431        | 68.98%          | 11.918%       |
| 10        | 12.024      | 1789          | 1794        | 1800         | rBV      | 299824         | 356392        | 81.29%          | 14.044%       |




Sum of corrected areas: 2537612

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX040122\  
Data File : VX027906.D  
Acq On : 02 Apr 2022 01:39  
Operator : JC/MD  
Sample : N2172-05  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 35 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-6R

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X032922W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

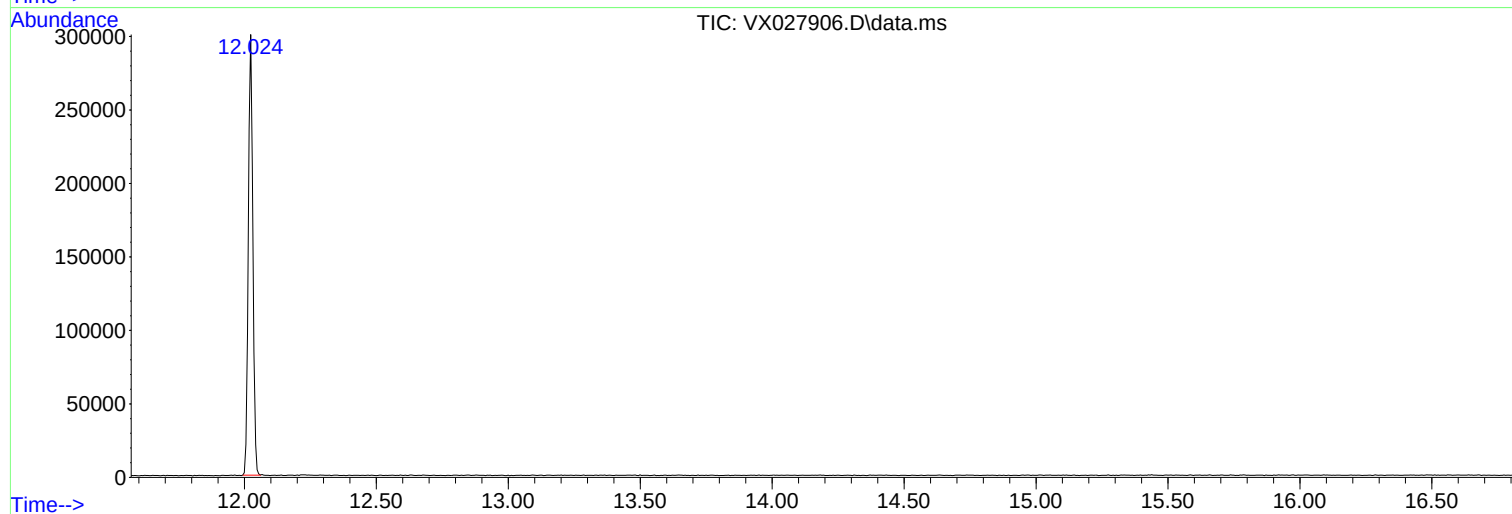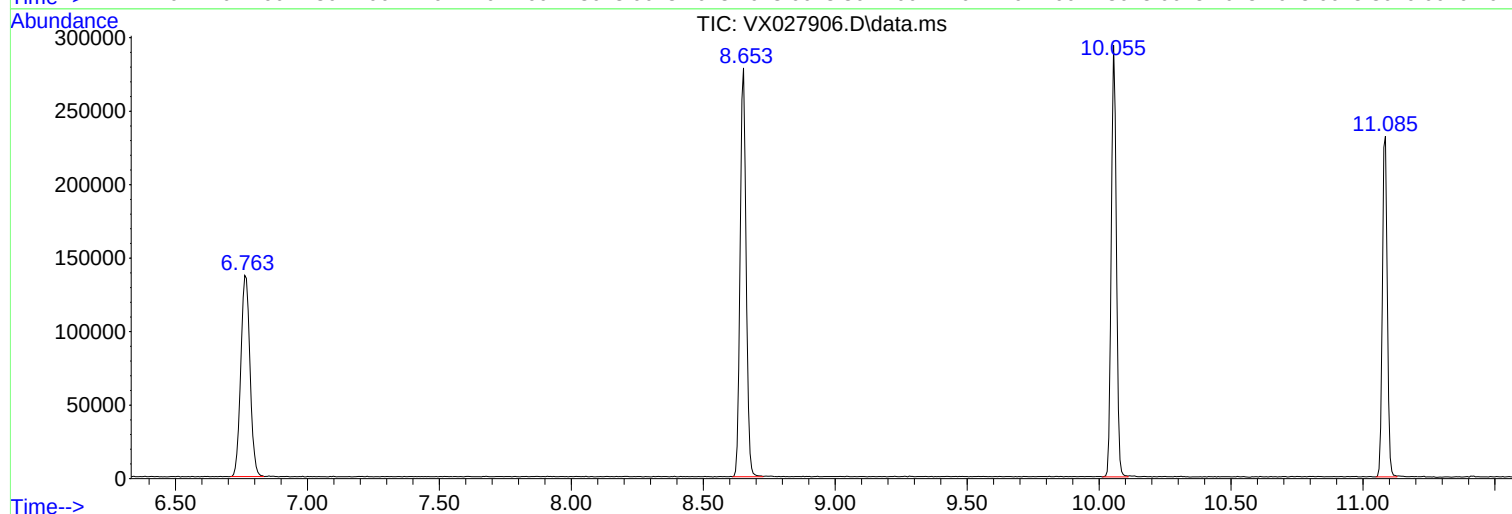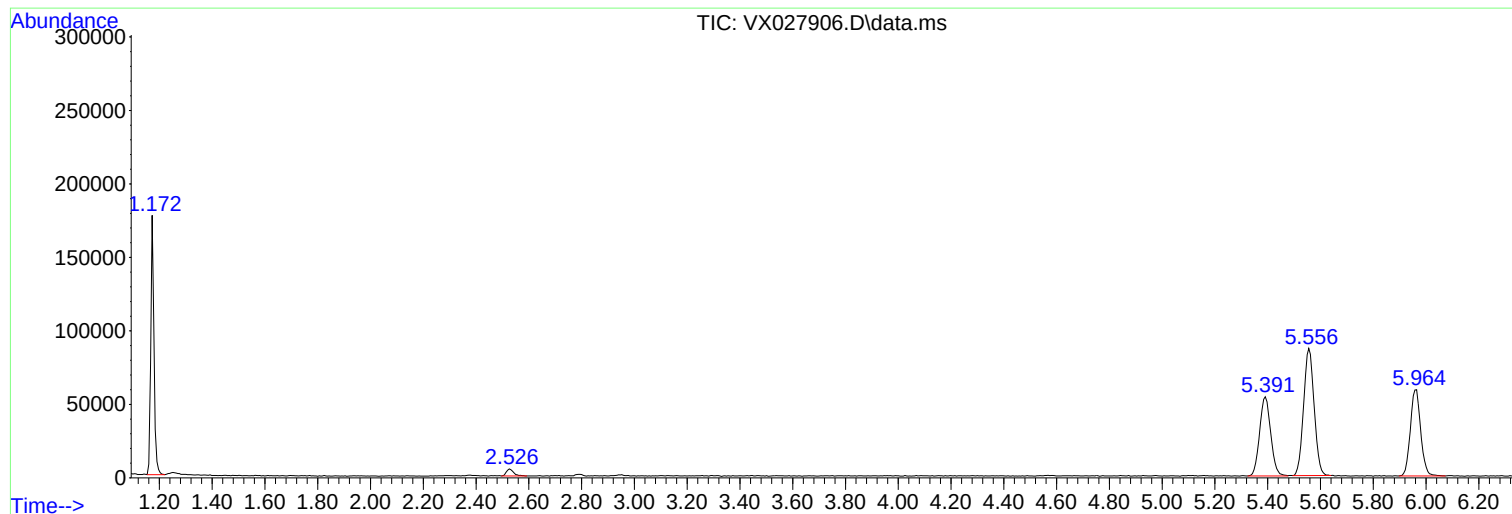

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX040122\  
Data File : VX027906.D  
Acq On : 02 Apr 2022 01:39  
Operator : JC/MD  
Sample : N2172-05  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 35 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-6R

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X032922W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX040122\  
Data File : VX027906.D  
Acq On : 02 Apr 2022 01:39  
Operator : JC/MD  
Sample : N2172-05  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 35 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-6R

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X032922W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|