



BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX040124\
Data File : VX040839.D
Acq On : 01 Apr 2024 09:28
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032124W.M
Title : SW846 8260
Last Update : Fri Mar 22 02:44:48 2024

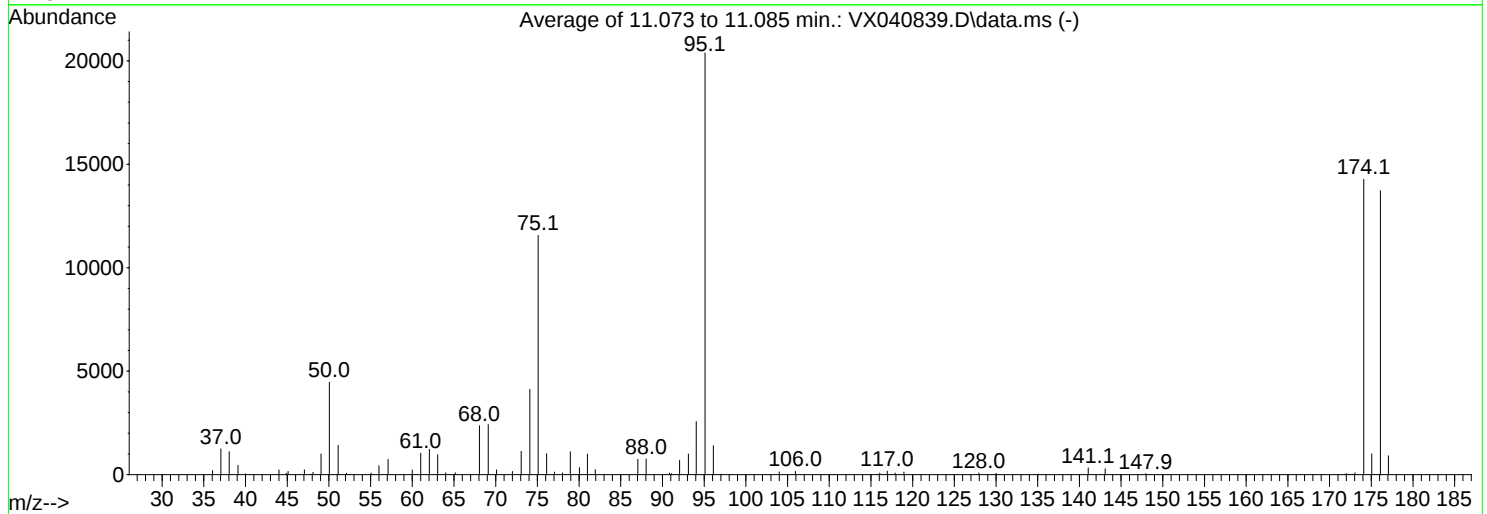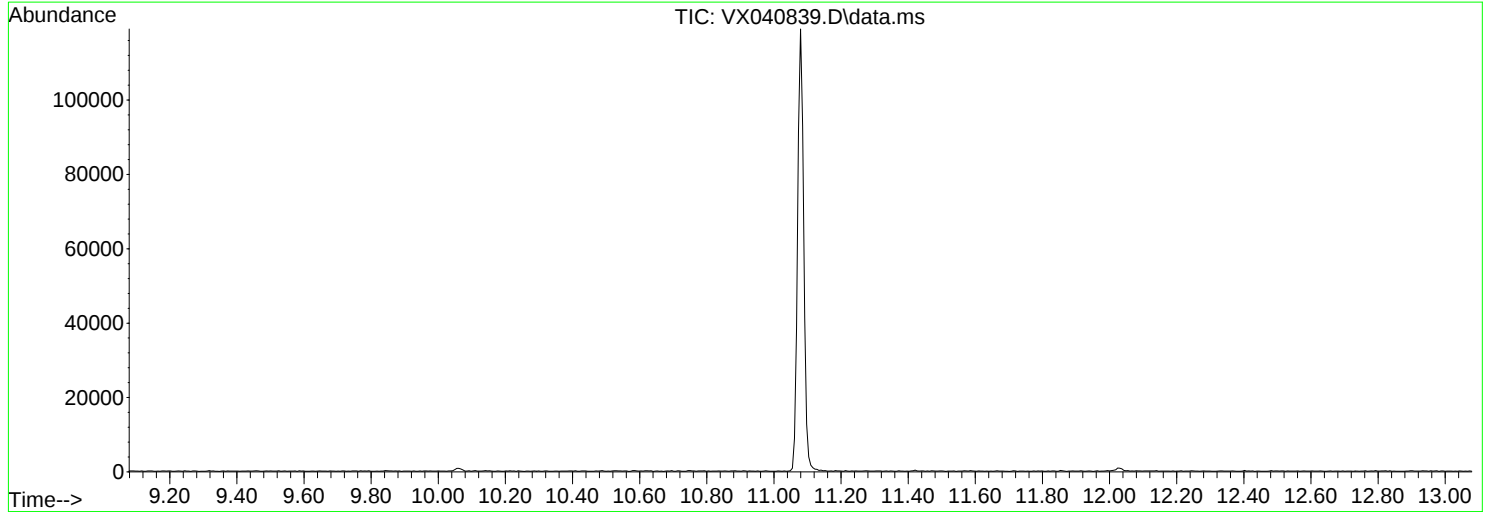

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	21.9	4473	PASS
75	95	30	60	56.7	11565	PASS
95	95	100	100	100.0	20387	PASS
96	95	5	9	6.9	1401	PASS
173	174	0.00	2	0.7	93	PASS
174	95	50	100	70.0	14274	PASS
175	174	5	9	7.0	1003	PASS
176	174	95	101	96.2	13725	PASS
177	176	5	9	6.7	914	PASS