

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX040219\
 Data File : VX008590.D
 Acq On : 02 Apr 2019 12:50
 Operator : JC/SP
 Sample : K2187-01
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TP-TRACK-89-90

Quant Time: Apr 03 11:28:05 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA X\METHOD\624X032719W.M
 Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 QLast Update : Wed Mar 27 12:01:15 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Bromochloromethane	5.02	128	34324	30.00	ug/l	0.00
28) 1,4-Difluorobenzene	6.86	114	198615	30.00	ug/l	0.00
57) Chlorobenzene-d5	10.11	117	169053	30.00	ug/l	0.00

System Monitoring Compounds						
27) 1,2-Dichloroethane-d4	6.06	65	88060	30.67	ug/l	0.00
Spiked Amount	30.000	Range	50 - 169	Recovery	=	102.23%
60) 4-Bromofluorobenzene	11.13	95	81584	27.70	ug/l	0.00
Spiked Amount	30.000	Range	56 - 143	Recovery	=	92.33%
63) Toluene-d8	8.71	98	246179	30.68	ug/l	0.00
Spiked Amount	30.000	Range	66 - 137	Recovery	=	102.27%


Target Compounds	Ovalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX040219\
Data File : VX008590.D
Acq On : 02 Apr 2019 12:50
Operator : JC/SP
Sample : K2187-01
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TP-TRACK-89-90

Quant Time: Apr 03 11:28:05 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA X\METHOD\624X032719W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
QLast Update : Wed Mar 27 12:01:15 2019
Response via : Initial Calibration

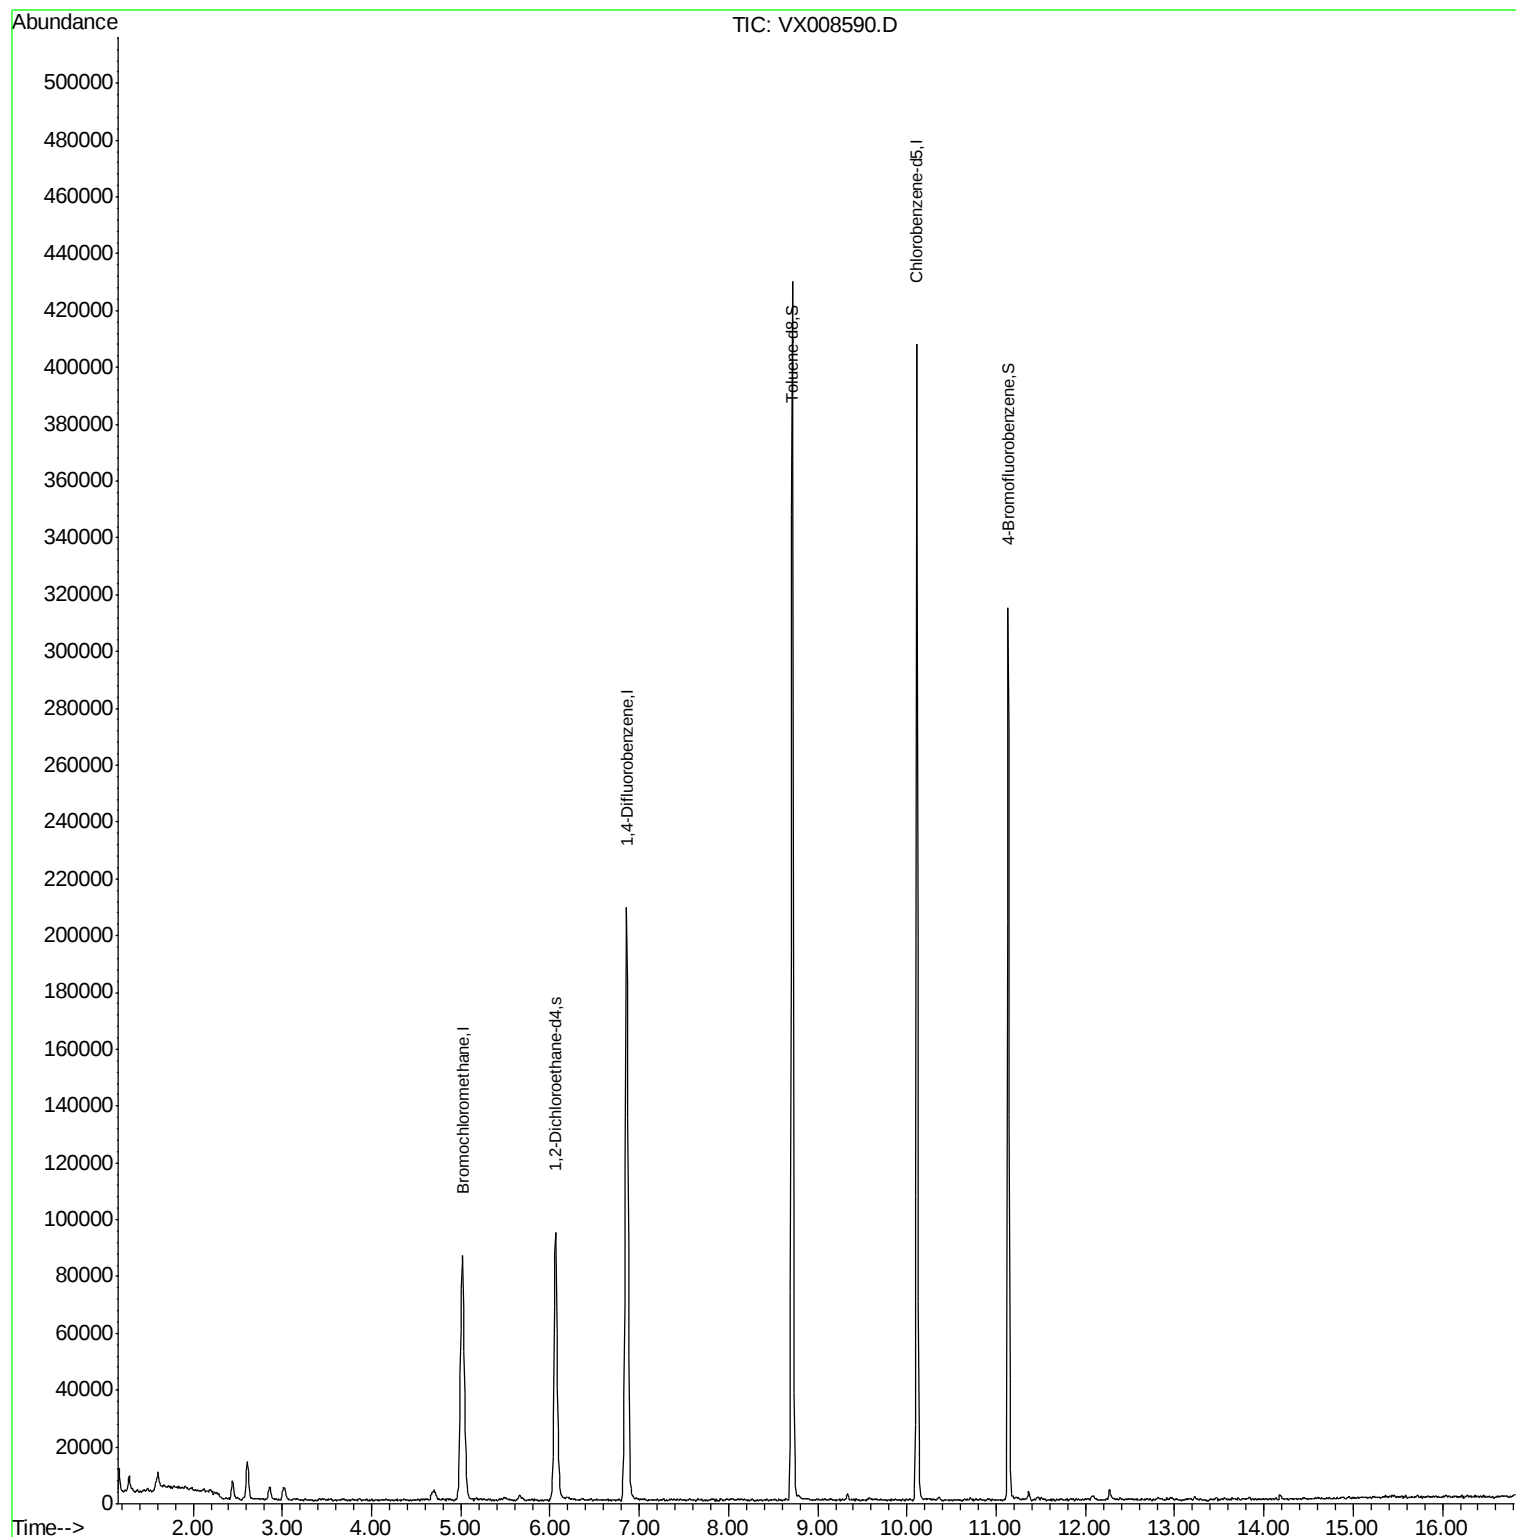

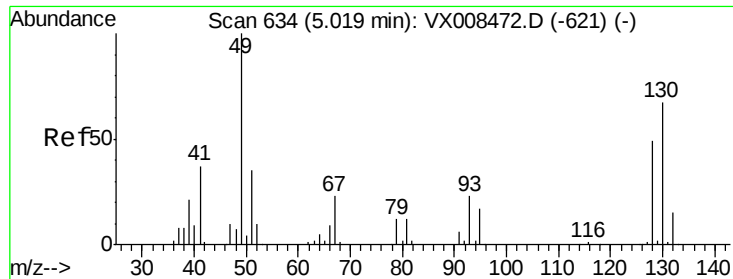

#1

Bromochloromethane

Concen: 30.000 ug/l

RT: 5.02 min Scan# 634

Delta R.T. -0.00 min

Lab File: VX008590.D

Acq: 02 Apr 2019 12:50

Instrument :

MSVOA_X

ClientSampleId :

TP-TRACK-89-90


Tot Ion:128 Resp: 34324

Ion Ratio Lower Upper

128 100

49 205.1 0.0 350.8




130 129.6 0.0 325.8

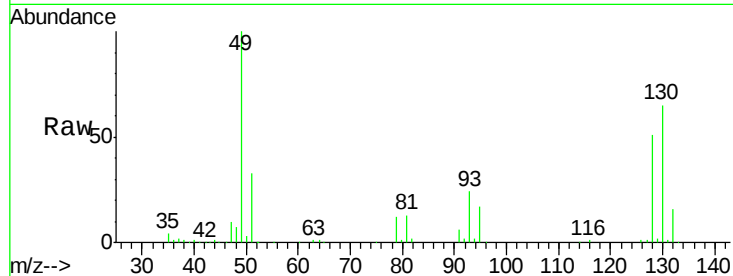

Abundance Ion 128.00 (127.70 to 128.70): V

Ion 49.00 (48.70 to 49.70): VX0

Ion 130.00 (129.70 to 130.70): V

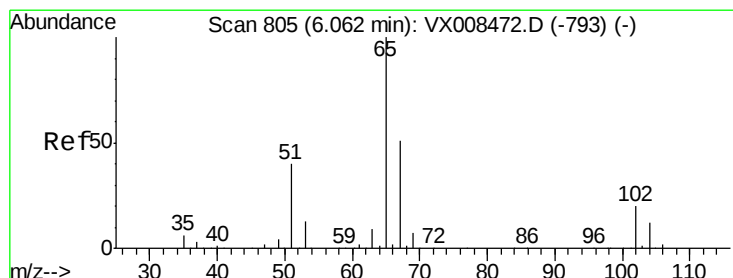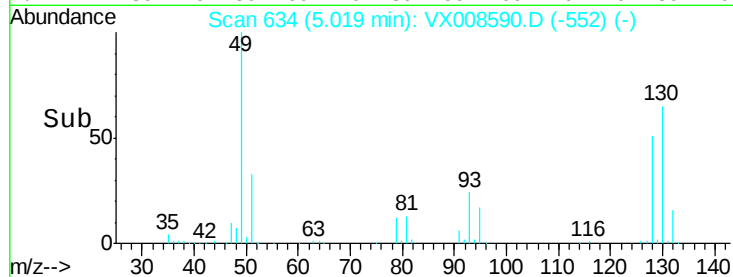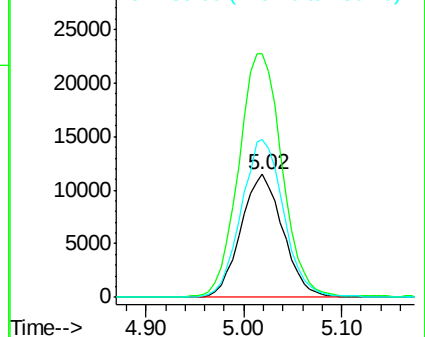

#27

1,2-Dichloroethane-d4

Concen: 30.668 ug/l

RT: 6.06 min Scan# 805

Delta R.T. -0.00 min

Lab File: VX008590.D


Acq: 02 Apr 2019 12:50

Tgt Ion: 65 Resp: 88060

Ion Ratio Lower Upper



65 100


67 54.3 42.9 64.3

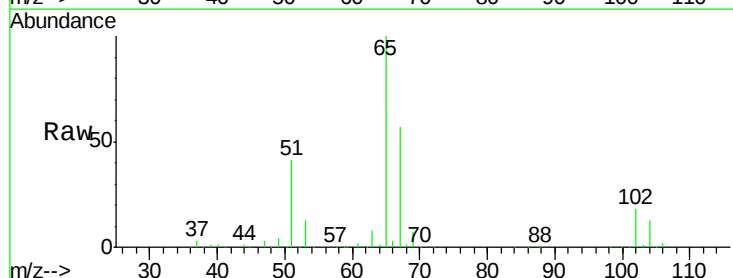

Abundance Ion 65.00 (64.70 to 65.70): VX0

Ion 67.00 (66.70 to 67.70): VX0

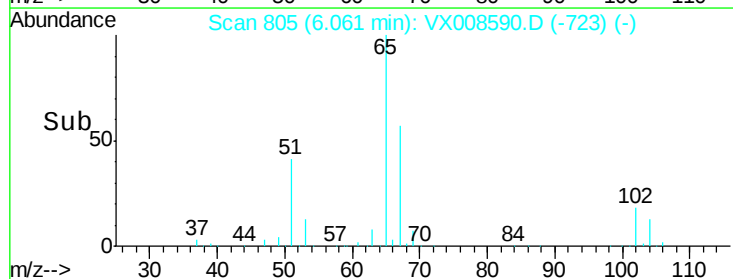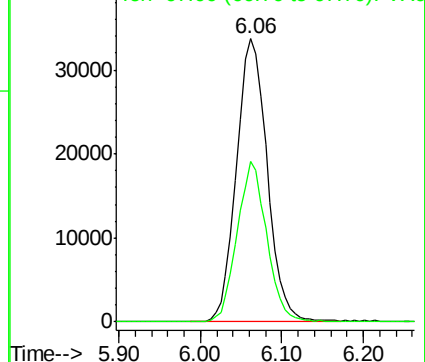


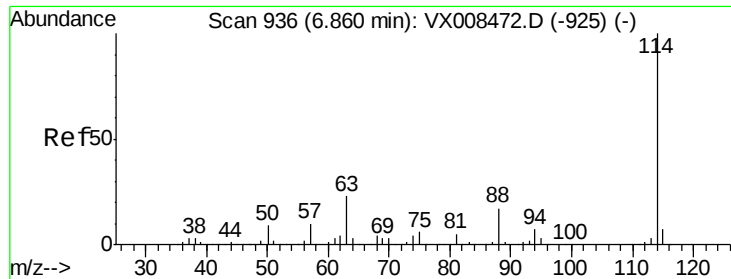




#28
 1,4-Difluorobenzene
 Concen: 30.000 ug/l
 RT: 6.86 min Scan# 936
 Delta R.T. -0.00 min
 Lab File: VX008590.D
 Acq: 02 Apr 2019 12:50

Instrument :
 MSVOA_X
 ClientSampleId :
 TP-TRACK-89-90

Tot Ion:114 Resp: 198615
 Ion Ratio Lower Upper
 114 100
 63 23.9 14.2 21.4#
 88 17.0 11.9 17.9

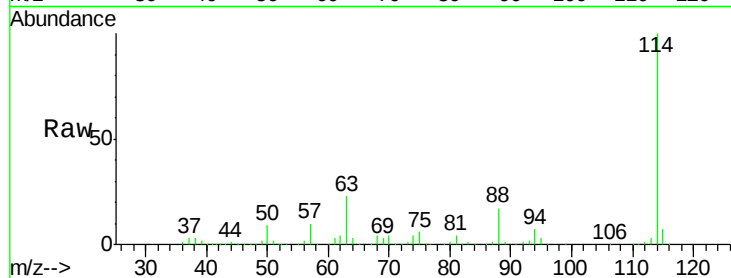


Abundance Ion 114.00 (113.70 to 114.70): V
 Ion 63.00 (62.70 to 63.70): VX0
 Ion 88.00 (87.70 to 88.70): VX0

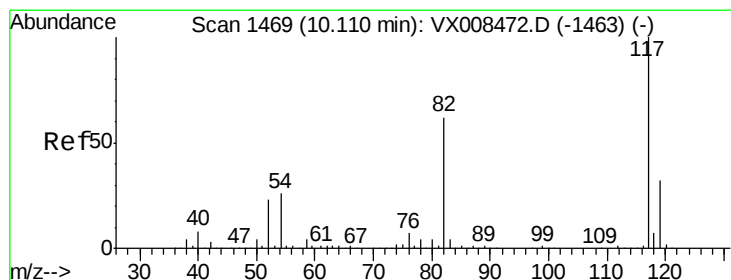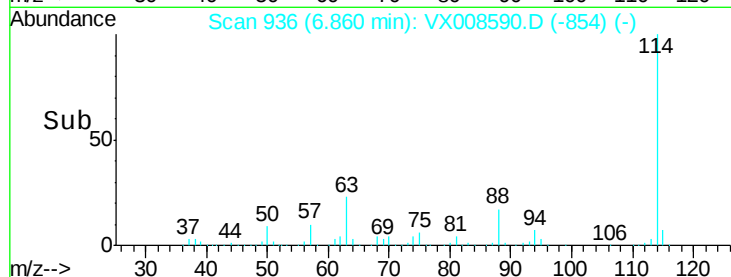
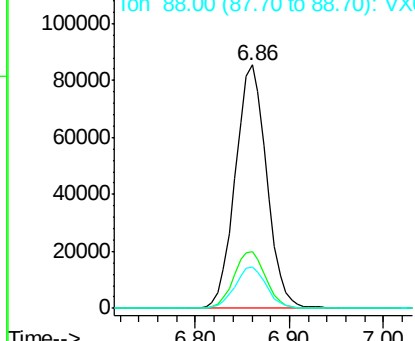



#57
 Chlorobenzene-d5
 Concen: 30.000 ug/l
 RT: 10.11 min Scan# 1469
 Delta R.T. -0.00 min
 Lab File: VX008590.D
 Acq: 02 Apr 2019 12:50

Tgt Ion:117 Resp: 169053
 Ion Ratio Lower Upper
 117 100
 82 60.7 40.4 60.6#
 119 31.9 25.8 38.6

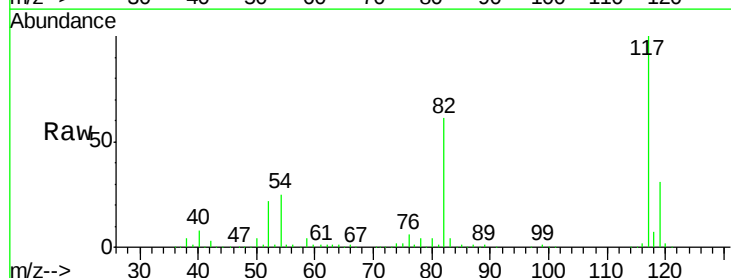

Abundance Ion 117.00 (116.70 to 117.70): V
 Ion 82.00 (81.70 to 82.70): VX0
 Ion 119.00 (118.70 to 119.70): V



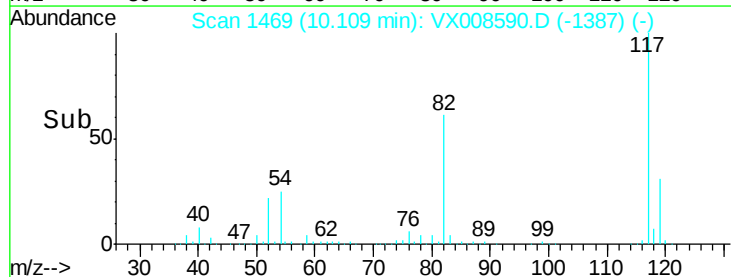
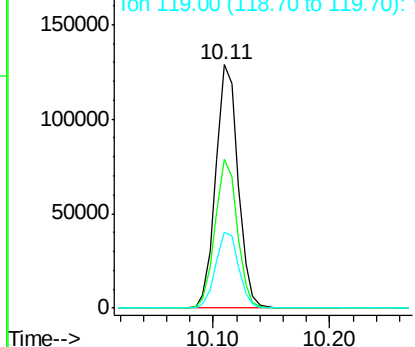


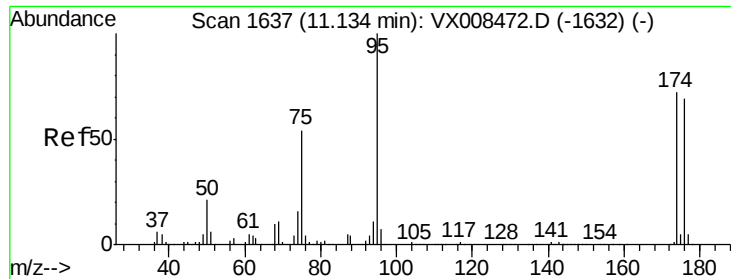

#60
4-Bromofluorobenzene
Concen: 27.698 ug/l
RT: 11.13 min Scan# 1637
Delta R.T. -0.00 min
Lab File: VX008590.D
Acq: 02 Apr 2019 12:50

Instrument :
MSVOA_X
ClientSampleId :
TP-TRACK-89-90

Tot Ion: 95 Resp: 81584
Ion Ratio Lower Upper
95 100
174 76.3 74.9 112.3
176 73.3 70.7 106.1

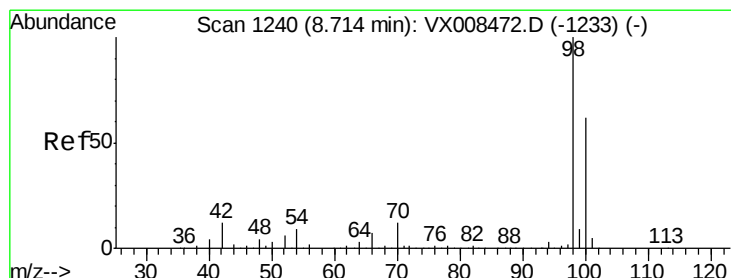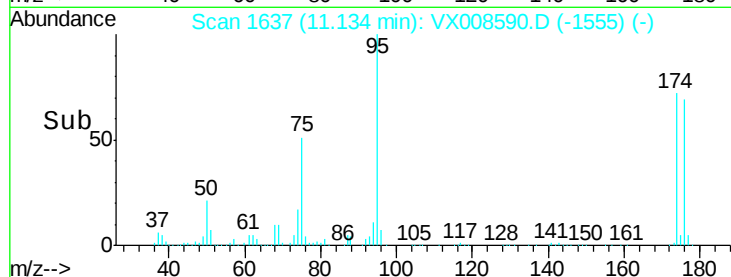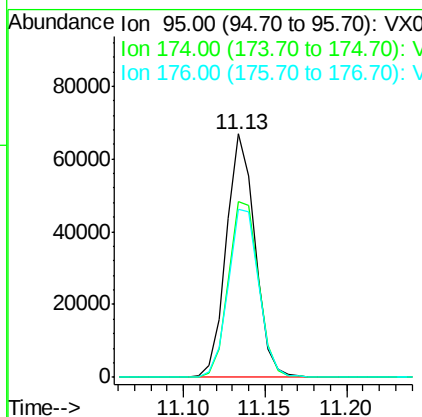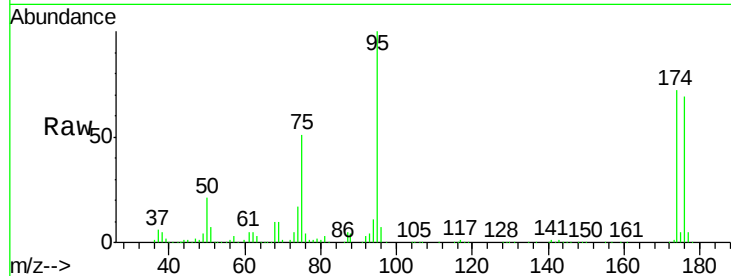

#63
Toluene-d8
Concen: 30.678 ug/l
RT: 8.71 min Scan# 1240
Delta R.T. -0.00 min
Lab File: VX008590.D
Acq: 02 Apr 2019 12:50

Tgt Ion: 98 Resp: 246179
Ion Ratio Lower Upper
98 100
100 64.2 50.9 76.3

