

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX040222\
 Data File : VX027940.D
 Acq On : 02 Apr 2022 17:51
 Operator : JC/MD
 Sample : N2249-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-6S

Quant Time: Apr 04 04:17:16 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032922W.M
 Quant Title : SW846 8260
 QLast Update : Wed Mar 30 04:39:27 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.556	168	79118	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	6.763	114	143068	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	129888	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	58480	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	61219	59.969	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery = 119.940%			
35) Dibromofluoromethane	5.391	113	47909	51.879	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery = 103.760%			
50) Toluene-d8	8.653	98	170751	52.552	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery = 105.100%			
62) 4-Bromofluorobenzene	11.079	95	67332	48.764	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery = 97.520%			
Target Compounds						Qvalue
3) Chloromethane	1.294	50	169	0.267	ug/l	# 42
6) Chloroethane	1.685	64	496	1.132	ug/l	# 43
11) Tert butyl alcohol	2.953	59	393	2.004	ug/l	# 72
13) Acrolein	2.337	56	1048	7.136	ug/l	# 71
14) Allyl chloride	2.782	41	10019	8.028	ug/l	# 62
15) Acrylonitrile	3.105	53	526	1.142	ug/l	# 34
16) Acetone	2.337	43	3959	8.763	ug/l	# 49
18) Methyl Acetate	2.782	43	22815	20.486	ug/l	# 46
25) 2-Butanone	4.477	43	364	0.554	ug/l	# 44
30) Chloroform	5.172	83	489	0.313	ug/l	# 17
31) Cyclohexane	5.464	56	576	0.510	ug/l	# 74
36) 1,1-Dichloropropene	5.556	75	6908	5.939	ug/l	# 51
37) Ethyl Acetate	4.477	43	364	0.252	ug/l	# 58
38) Carbon Tetrachloride	5.550	117	9011	7.012	ug/l	# 16
40) Benzene	6.044	78	2302	0.653	ug/l	# 98
41) Methacrylonitrile	5.123	41	156	0.203	ug/l	# 18
43) Isopropyl Acetate	6.245	43	4986	2.159	ug/l	# 56
51) 4-Methyl-2-Pentanone	8.647	43	828	0.517	ug/l	# 1
52) Toluene	8.720	92	883	0.398	ug/l	# 92
55) 1,1,2-Trichloroethane	9.098	97	260	0.264	ug/l	# 16
59) 2-Hexanone	9.445	43	277	0.225	ug/l	# 18
67) Ethyl Benzene	10.195	91	3075	0.662	ug/l	# 100
68) m/p-Xylenes	10.305	106	3870	2.267	ug/l	# 93
69) o-Xylene	10.646	106	950	0.570	ug/l	# 70
76) 1,2,3-Trichloropropane	11.079	75	36097	26.313	ug/l	# 38
80) 1,3,5-Trimethylbenzene	11.451	105	881	0.233	ug/l	# 91
81) trans-1,4-Dichloro-2-b...	11.079	75	36097	77.073	ug/l	# 15
84) 1,2,4-Trimethylbenzene	11.756	105	2822	0.749	ug/l	# 93
90) Hexachloroethane	12.646	117	579	0.961	ug/l	# 10
92) 1,2-Dibromo-3-Chloropr...	12.695	75	104	0.292	ug/l	# 1
95) Naphthalene	13.780	128	1446	0.351	ug/l	# 94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX040222\
Data File : VX027940.D
Acq On : 02 Apr 2022 17:51
Operator : JC/MD
Sample : N2249-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-6S

Quant Time: Apr 04 04:17:16 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032922W.M
Quant Title : SW846 8260
QLast Update : Wed Mar 30 04:39:27 2022
Response via : Initial Calibration




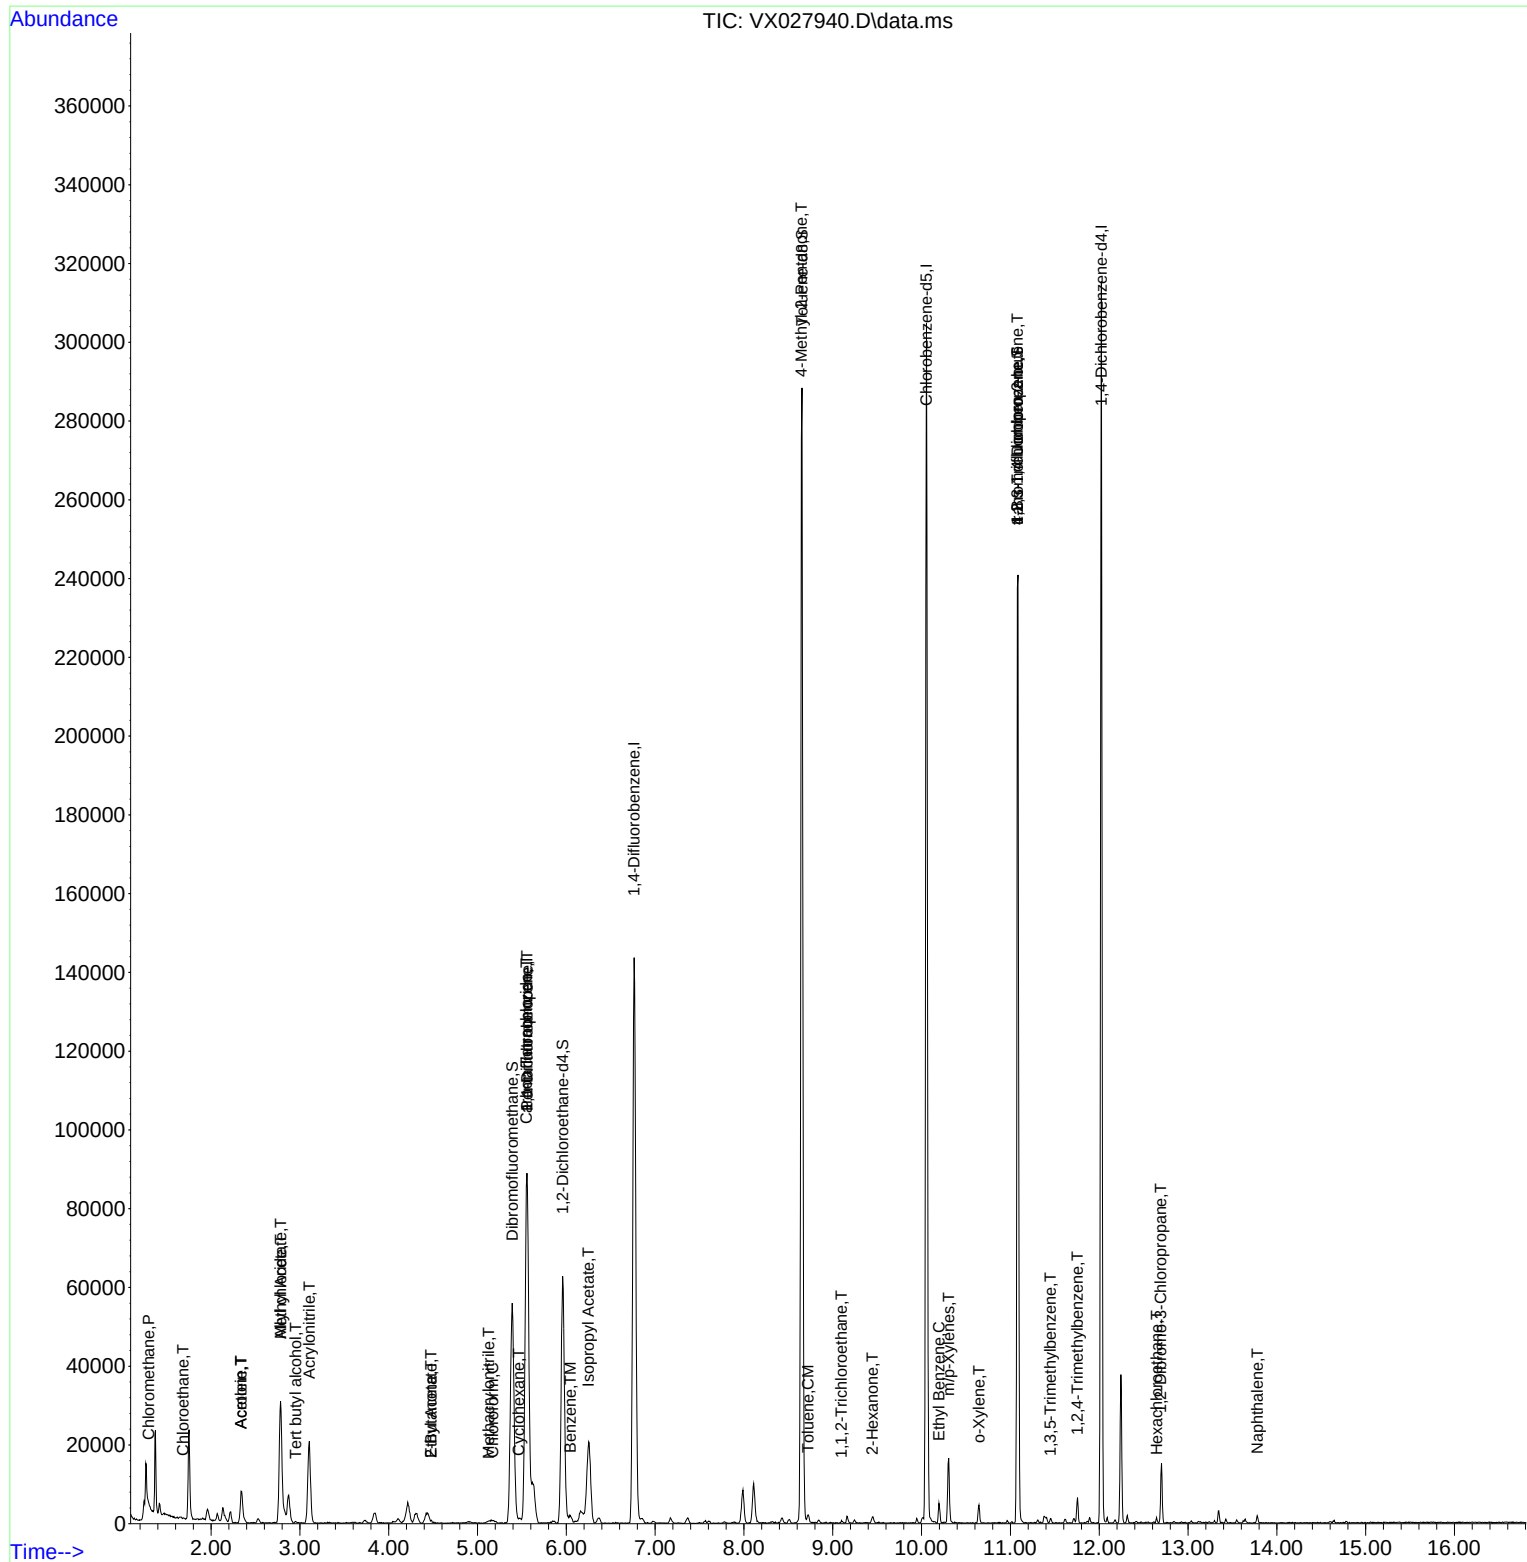




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX027940.D
Acq: 02 Apr 2022 17:51




Instrument :
MSVOA_X
ClientSampleId :
MW-6S

Tgt Ion:168 Resp: 79118
Ion Ratio Lower Upper
168 100
99 68.9 41.7 62.5#

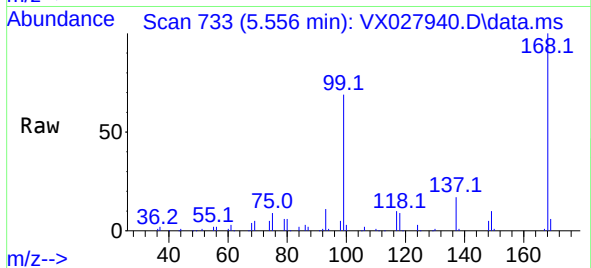


#3
Chloromethane
Concen: 0.267 ug/l
RT: 1.294 min Scan# 34
Delta R.T. 0.000 min
Lab File: VX027940.D
Acq: 02 Apr 2022 17:51

Tgt Ion: 50 Resp: 169
Ion Ratio Lower Upper
50 100
52 0.0 26.4 39.6#

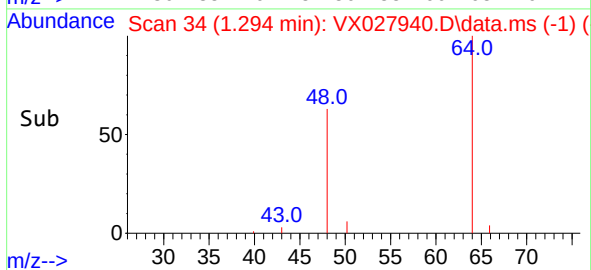

Abundance Scan 97 (1.678 min): VX027779.D\data.ms (-90)


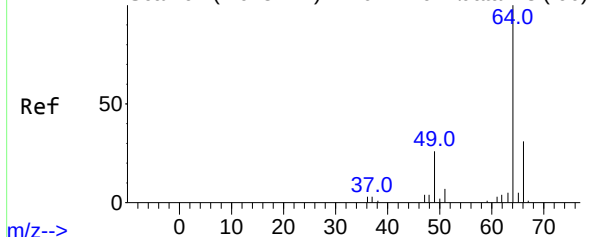


#6
Chloroethane
Concen: 1.132 ug/l
RT: 1.685 min Scan# 91
Delta R.T. 0.007 min
Lab File: VX027940.D
Acq: 02 Apr 2022 17:51


Instrument :
MSVOA_X
ClientSampleId :
MW-6S

Tgt Ion: 64 Resp: 496
Ion Ratio Lower Upper
64 100
66 0.0 25.3 37.9#


Abundance Scan 98 (1.685 min): VX027940.D\data.ms

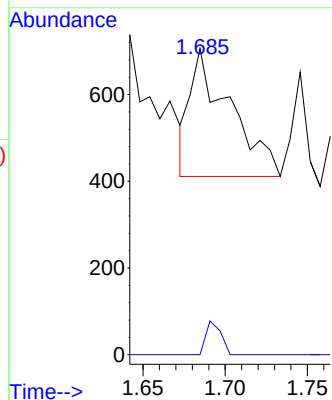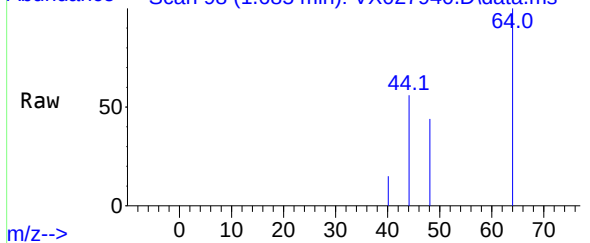

Abundance Scan 98 (1.685 min): VX027940.D\data.ms (-48)

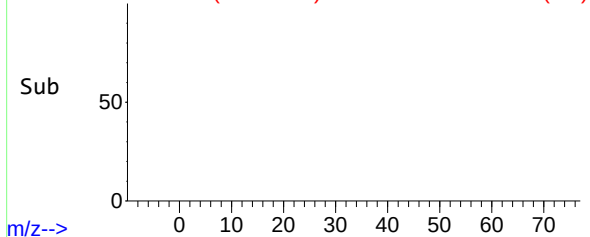



Abundance Scan 308 (2.965 min): VX027779.D\data.ms (-29)

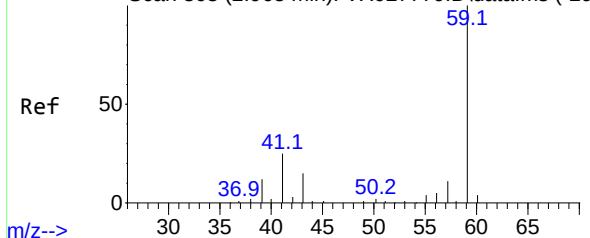


#11
Tert butyl alcohol
Concen: 2.004 ug/l
RT: 2.953 min Scan# 306
Delta R.T. -0.012 min
Lab File: VX027940.D
Acq: 02 Apr 2022 17:51


Tgt Ion: 59 Resp: 393
Ion Ratio Lower Upper
59 100
57 0.0 8.3 12.5#

Abundance Scan 306 (2.953 min): VX027940.D\data.ms

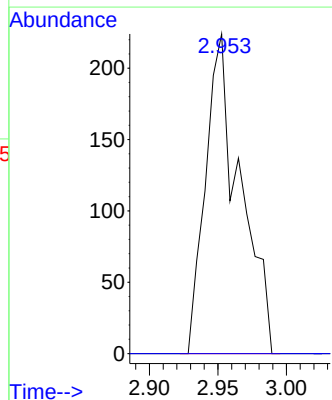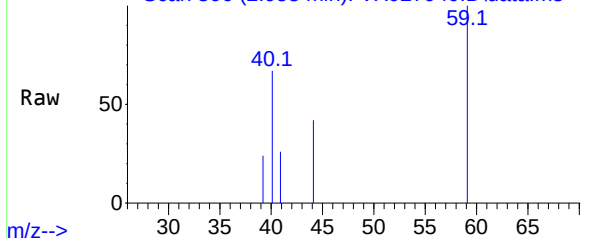

Abundance Scan 306 (2.953 min): VX027940.D\data.ms (-25)

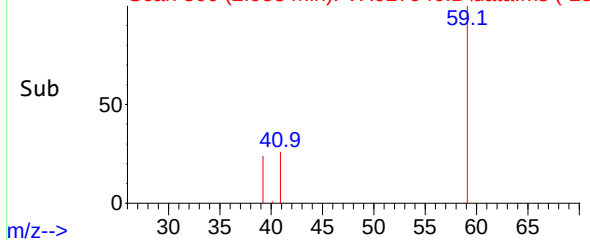



#13

Acrolein

Concen: 7.136 ug/l

RT: 2.337 min Scan# 205

Delta R.T. 0.104 min

Lab File: VX027940.D

Acq: 02 Apr 2022 17:51

Instrument :

MSVOA_X

ClientSampleId :





MW-6S

Tgt Ion: 56 Resp: 1048

Ion Ratio Lower Upper

56 100

55 45.5 55.0 82.6#

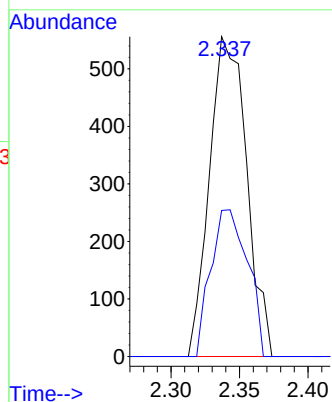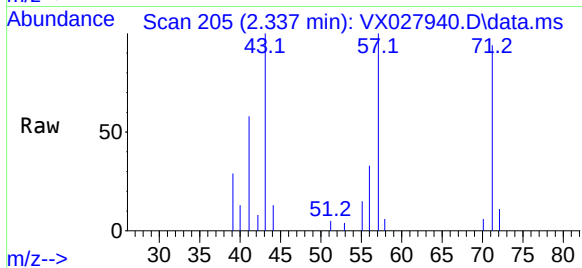

#14

Allyl chloride

Concen: 8.028 ug/l

RT: 2.782 min Scan# 278

Delta R.T. 0.116 min

Lab File: VX027940.D

Acq: 02 Apr 2022 17:51




Tgt Ion: 41 Resp: 10019


Ion Ratio Lower Upper

41 100

39 47.2 50.4 75.6#

76 0.0 32.7 49.1#


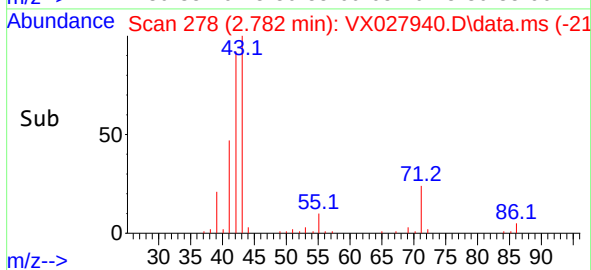
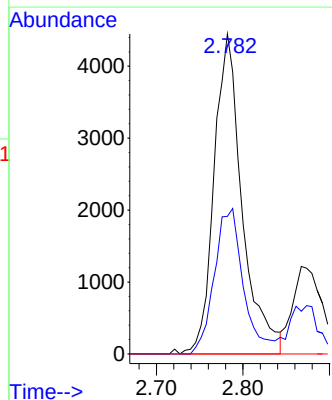
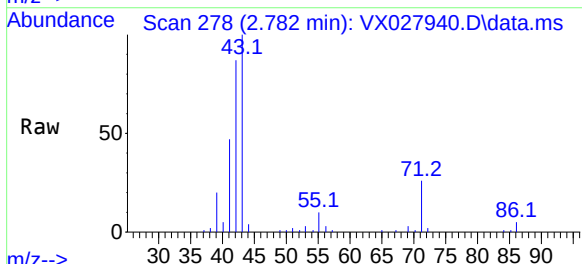




#15
Acrylonitrile
Concen: 1.142 ug/l
RT: 3.105 min Scan# 31
Delta R.T. 0.043 min
Lab File: VX027940.D
Acq: 02 Apr 2022 17:51




Instrument :
MSVOA_X
ClientSampleId :
MW-6S


Tgt Ion: 53 Resp: 526
Ion Ratio Lower Upper
53 100
52 0.0 65.7 98.5#
51 31.2 28.4 42.6



#16
Acetone
Concen: 8.763 ug/l
RT: 2.337 min Scan# 205
Delta R.T. -0.043 min
Lab File: VX027940.D
Acq: 02 Apr 2022 17:51

Tgt Ion: 43 Resp: 3959
Ion Ratio Lower Upper
43 100
58 5.8 28.8 43.2#

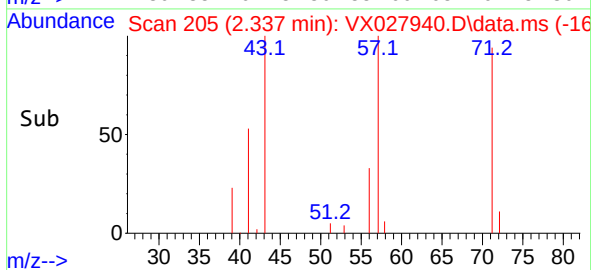



#18

Methyl Acetate

Concen: 20.486 ug/l

RT: 2.782 min Scan# 21

Delta R.T. 0.079 min

Lab File: VX027940.D

Acq: 02 Apr 2022 17:51

Instrument :

MSVOA_X

ClientSampleId :





MW-6S

Tgt Ion: 43 Resp: 22815

Ion Ratio Lower Upper

43 100

74 0.0 22.8 34.2#

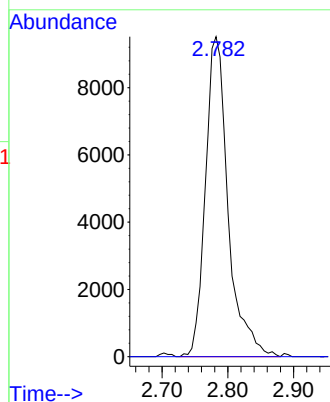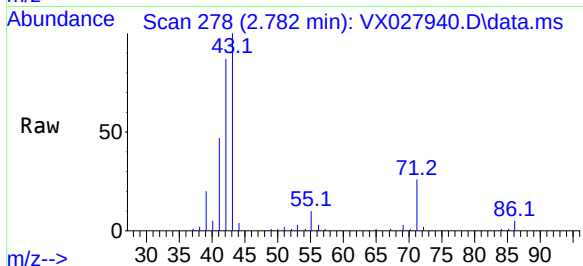

#25

2-Butanone

Concen: 0.554 ug/l

RT: 4.477 min Scan# 556

Delta R.T. -0.079 min

Lab File: VX027940.D




Acq: 02 Apr 2022 17:51


Tgt Ion: 43 Resp: 364

Ion Ratio Lower Upper

43 100

72 0.0 24.4 36.6#

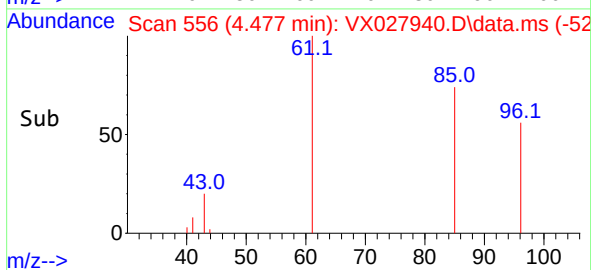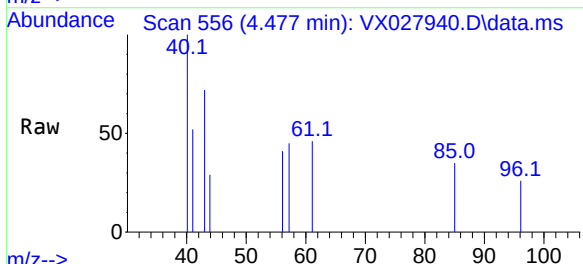



#30

Chloroform

Concen: 0.313 ug/l

RT: 5.172 min Scan# 61

Delta R.T. 0.073 min

Lab File: VX027940.D

Acq: 02 Apr 2022 17:51

Instrument :

MSVOA_X

ClientSampleId :





MW-6S

Tgt Ion: 83 Resp: 489

Ion Ratio Lower Upper

83 100

85 0.0 52.7 79.1#

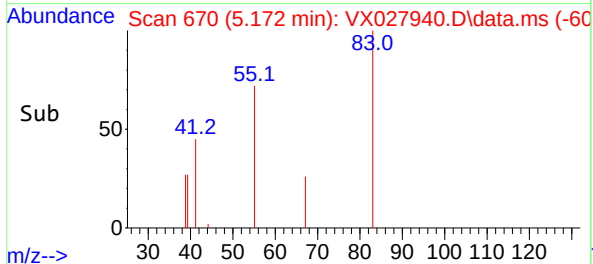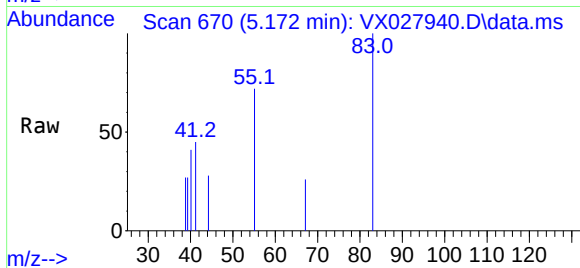

#31

Cyclohexane

Concen: 0.510 ug/l

RT: 5.464 min Scan# 718

Delta R.T. -0.013 min

Lab File: VX027940.D

Acq: 02 Apr 2022 17:51




Tgt Ion: 56 Resp: 576


Ion Ratio Lower Upper

56 100

69 44.3 26.7 40.1#

84 68.4 77.2 115.8#


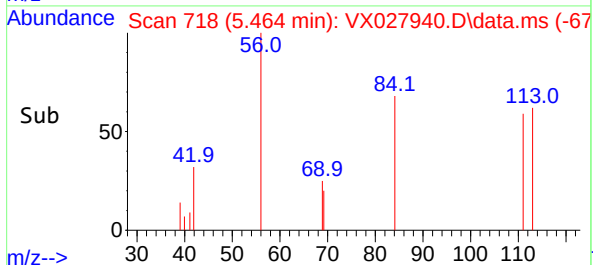
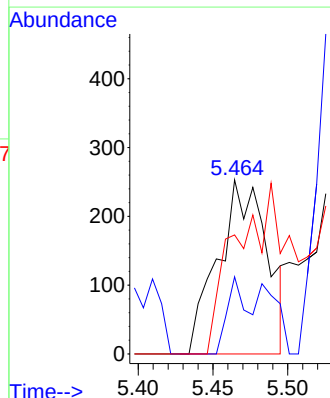
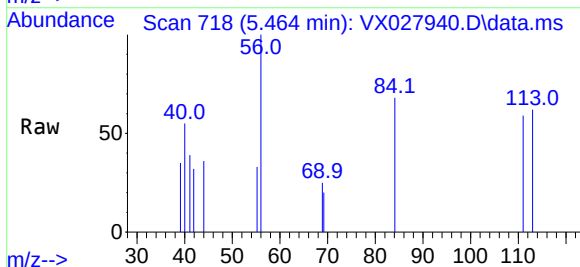


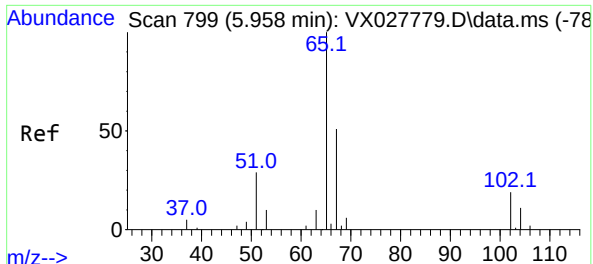

#33
1,2-Dichloroethane-d4
Concen: 59.969 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.000 min
Lab File: VX027940.D
Acq: 02 Apr 2022 17:51




Instrument :
MSVOA_X
ClientSampleId :
MW-6S


Tgt Ion: 65 Resp: 61219
Ion Ratio Lower Upper
65 100
67 51.3 0.0 107.4



#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 931
Delta R.T. 0.000 min
Lab File: VX027940.D
Acq: 02 Apr 2022 17:51

Tgt Ion: 114 Resp: 143068
Ion Ratio Lower Upper
114 100
63 21.1 0.0 36.8
88 17.0 0.0 32.4

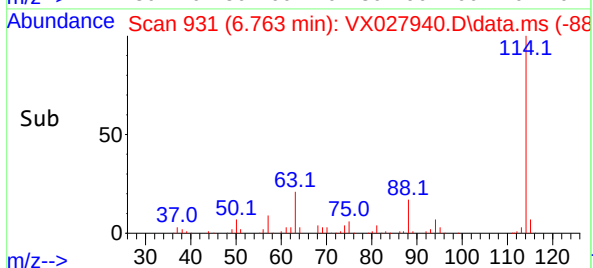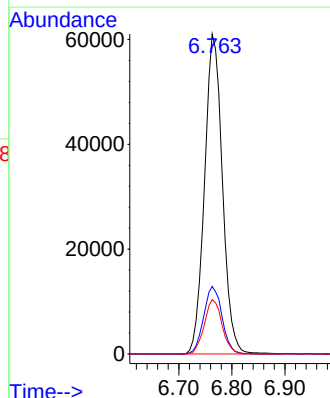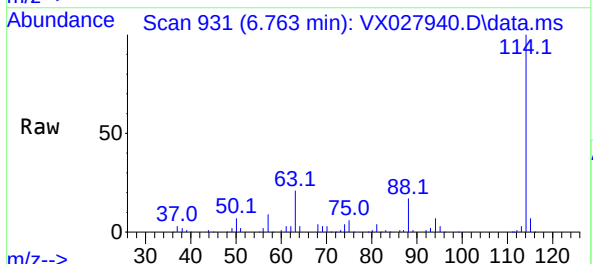




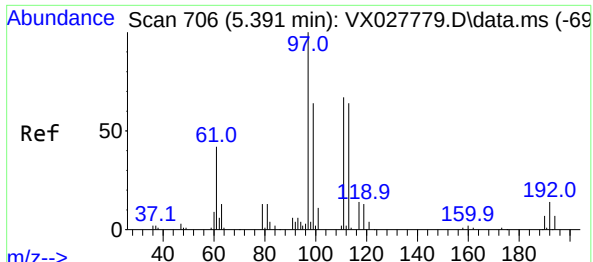


#35
Dibromofluoromethane
Concen: 51.879 ug/l
RT: 5.391 min Scan# 706
Delta R.T. 0.000 min
Lab File: VX027940.D
Acq: 02 Apr 2022 17:51

Instrument :
MSVOA_X
ClientSampleId :
MW-6S

Tgt Ion:113 Resp: 47909




Ion	Ratio	Lower	Upper
113	100		
111	103.2	82.8	124.2
192	16.9	16.9	25.3

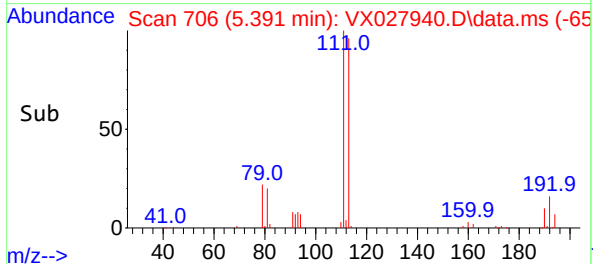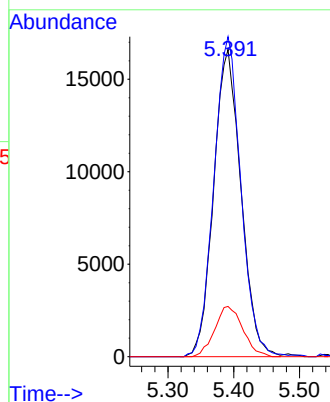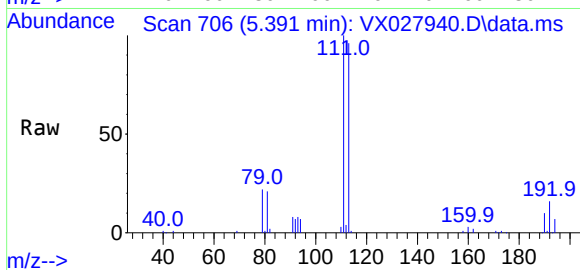


#36
1,1-Dichloropropene
Concen: 5.939 ug/l
RT: 5.556 min Scan# 733
Delta R.T. -0.134 min
Lab File: VX027940.D
Acq: 02 Apr 2022 17:51

Tgt Ion: 75 Resp: 6908

Ion	Ratio	Lower	Upper
75	100		
110	11.0	18.3	54.8#
77	0.0	24.8	37.2#

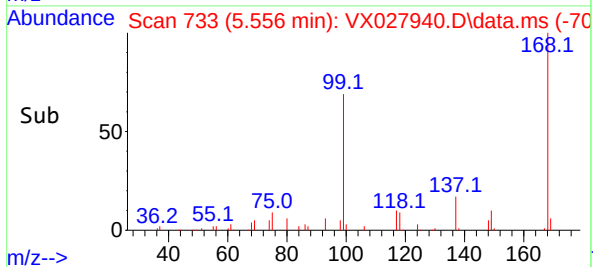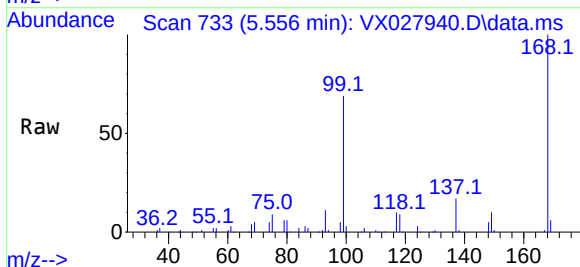



#37

Ethyl Acetate

Concen: 0.252 ug/l

RT: 4.477 min Scan# 51

Delta R.T. -0.238 min

Lab File: VX027940.D

Acq: 02 Apr 2022 17:51





Instrument :

MSVOA_X

ClientSampleId :

MW-6S

Tgt Ion: 43	Resp:	364
Ion	Ratio	Lower Upper
43	100	
61	37.1	12.6 19.0#
70	0.0	10.2 15.2#

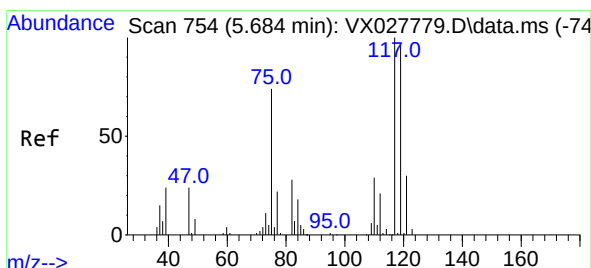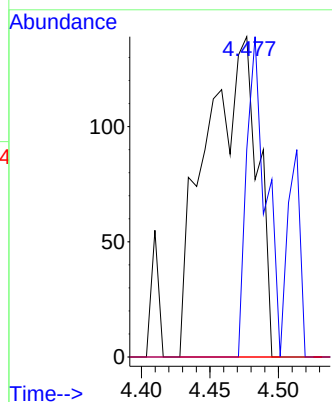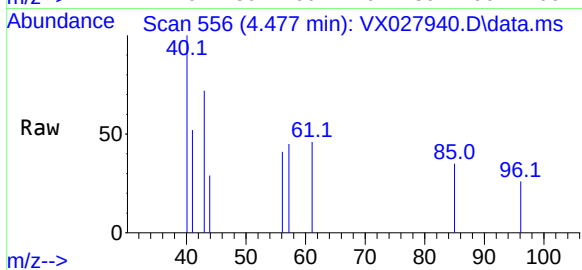

#38

Carbon Tetrachloride

Concen: 7.012 ug/l




RT: 5.550 min Scan# 732


Delta R.T. -0.134 min

Lab File: VX027940.D

Acq: 02 Apr 2022 17:51

Tgt Ion: 117	Resp:	9011
Ion	Ratio	Lower Upper
117	100	
119	6.0	77.3 115.9#
121	0.0	24.2 36.2#


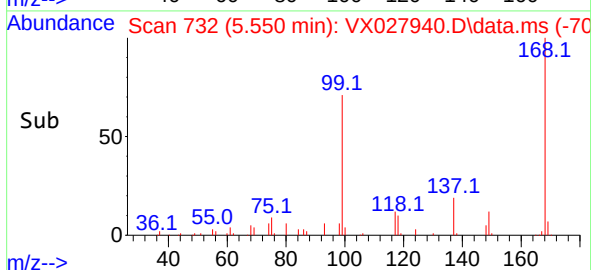
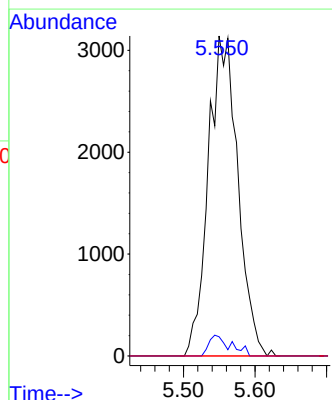
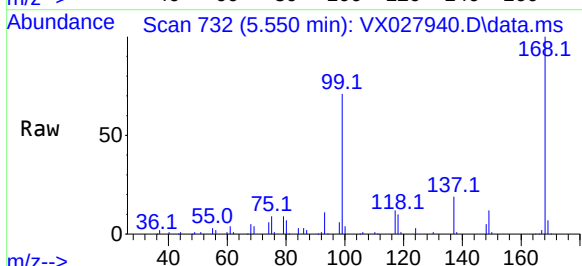


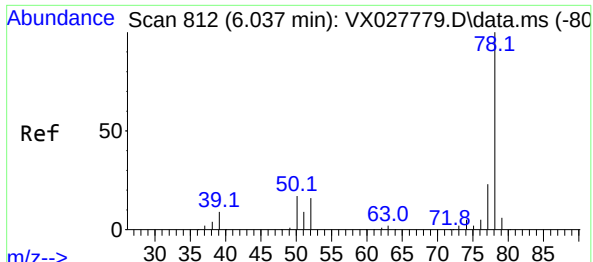

#40
Benzene
Concen: 0.653 ug/l
RT: 6.044 min Scan# 812
Delta R.T. 0.007 min
Lab File: VX027940.D
Acq: 02 Apr 2022 17:51




Instrument :
MSVOA_X
ClientSampleId :
MW-6S


Tgt Ion: 78 Resp: 2302
Ion Ratio Lower Upper
78 100
77 25.3 19.3 28.9

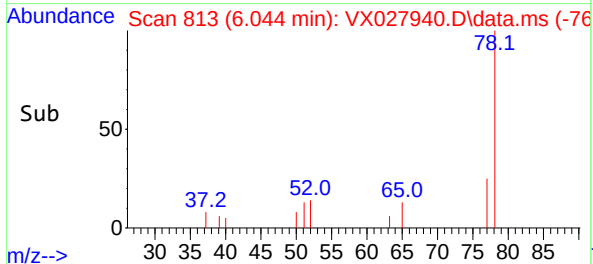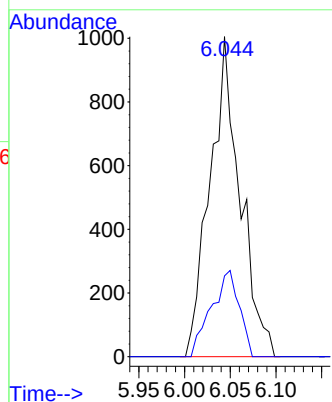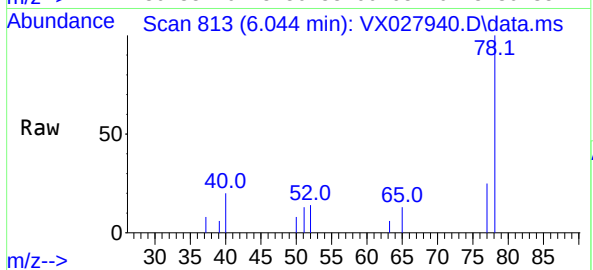

#41
Methacrylonitrile
Concen: 0.203 ug/l
RT: 5.123 min Scan# 662
Delta R.T. 0.201 min
Lab File: VX027940.D
Acq: 02 Apr 2022 17:51

Tgt Ion: 41 Resp: 156
Ion Ratio Lower Upper
41 100
39 0.0 43.0 64.4#
67 0.0 70.2 105.4#
52 0.0 26.0 39.0#


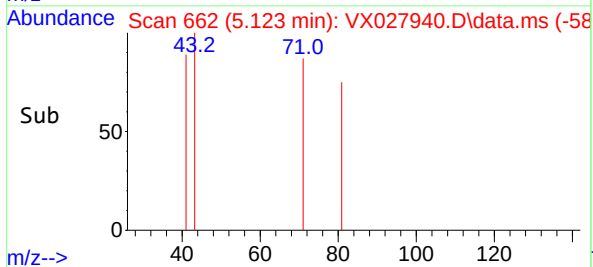
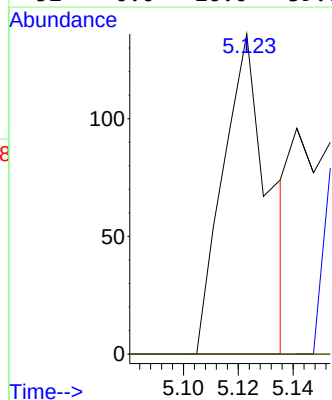
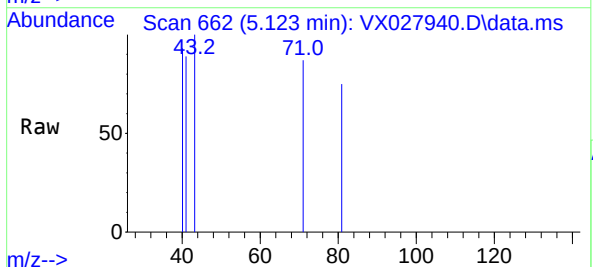




#43
Isopropyl Acetate
Concen: 2.159 ug/l
RT: 6.245 min Scan# 84
Delta R.T. -0.097 min
Lab File: VX027940.D
Acq: 02 Apr 2022 17:51




Instrument :
MSVOA_X
ClientSampleId :
MW-6S


Tgt Ion: 43 Resp: 4986
Ion Ratio Lower Upper
43 100
61 0.0 18.5 27.7#
87 0.0 13.0 19.6#

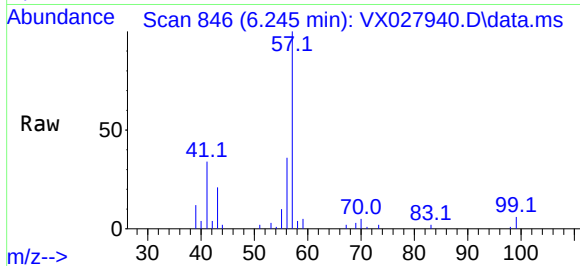

#50
Toluene-d8
Concen: 52.552 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. -0.000 min
Lab File: VX027940.D
Acq: 02 Apr 2022 17:51

Tgt Ion: 98 Resp: 170751
Ion Ratio Lower Upper
98 100
100 64.3 52.6 78.8

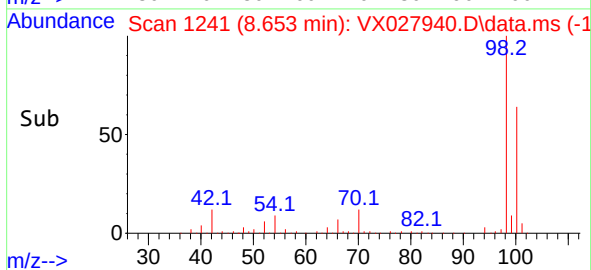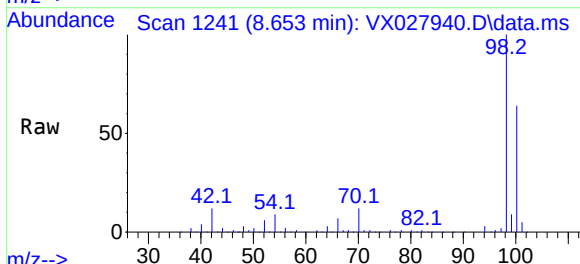



#51

4-Methyl-2-Pentanone

Concen: 0.517 ug/l

RT: 8.647 min Scan# 11

Delta R.T. 0.073 min

Lab File: VX027940.D

Acq: 02 Apr 2022 17:51

Instrument :

MSVOA_X

ClientSampleId :


MW-6S

Tgt Ion: 43 Resp: 828




Ion Ratio Lower Upper

43 100

58 177.2 36.1 54.1#

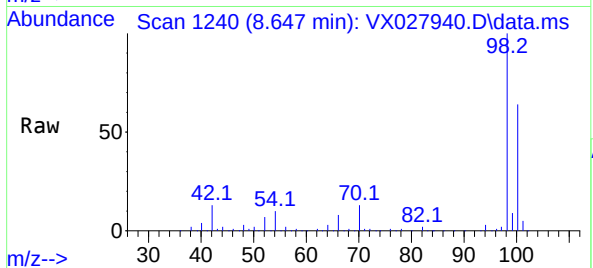

Abundance

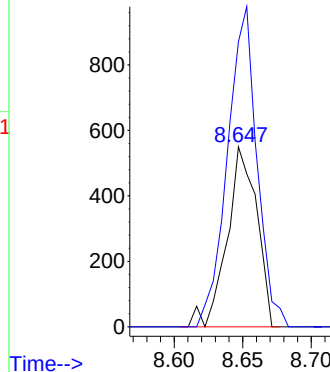

#52

Toluene

Concen: 0.398 ug/l

RT: 8.720 min Scan# 1252

Delta R.T. -0.000 min

Lab File: VX027940.D


Acq: 02 Apr 2022 17:51

Tgt Ion: 92 Resp: 883



Ion Ratio Lower Upper


92 100

91 183.0 137.5 206.3



Abundance



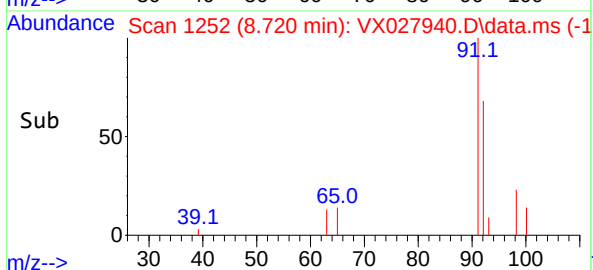
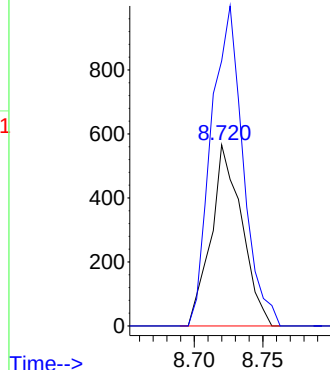




#55
1,1,2-Trichloroethane
Concen: 0.264 ug/l
RT: 9.098 min Scan# 11
Delta R.T. -0.055 min
Lab File: VX027940.D
Acq: 02 Apr 2022 17:51




Instrument :
MSVOA_X
ClientSampleId :
MW-6S


Tgt Ion: 97	Resp:	260
Ion	Ratio	Lower Upper
97	100	
83	0.0	66.2 99.4#
85	0.0	42.9 64.3#
99	0.0	49.0 73.6#

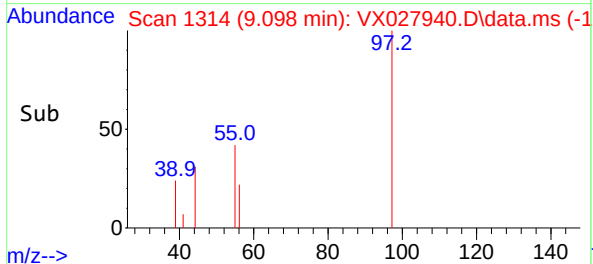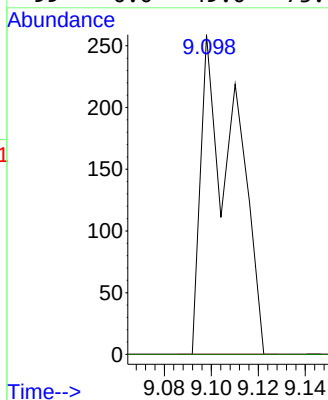

#59
2-Hexanone
Concen: 0.225 ug/l
RT: 9.445 min Scan# 1371
Delta R.T. 0.012 min
Lab File: VX027940.D
Acq: 02 Apr 2022 17:51

Tgt Ion: 43	Resp:	277
Ion	Ratio	Lower Upper
43	100	
58	0.0	31.9 95.7#


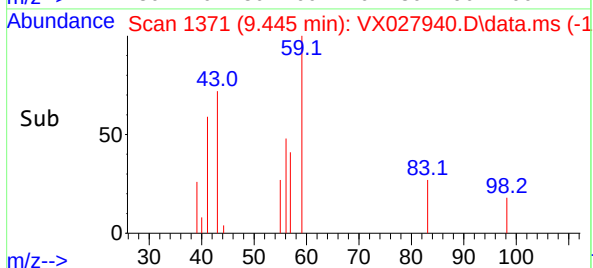
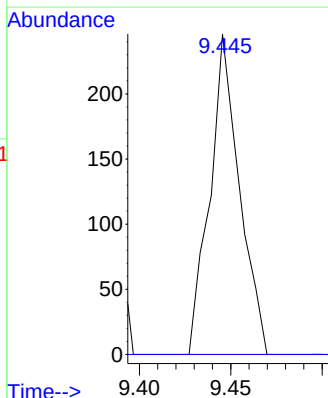
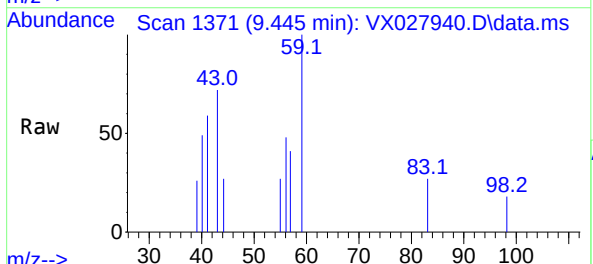




#62
4-Bromofluorobenzene
Concen: 48.764 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.006 min
Lab File: VX027940.D
Acq: 02 Apr 2022 17:51




Instrument :
MSVOA_X
ClientSampleId :
MW-6S


Tgt Ion: 95 Resp: 67332
Ion Ratio Lower Upper
95 100
174 69.0 0.0 163.0
176 66.9 0.0 155.0

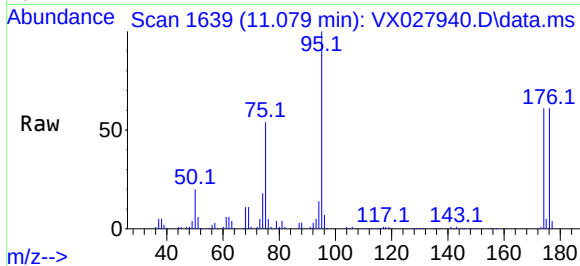

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX027940.D
Acq: 02 Apr 2022 17:51

Tgt Ion: 117 Resp: 129888
Ion Ratio Lower Upper
117 100
82 61.0 41.8 62.8
119 32.7 24.8 37.2


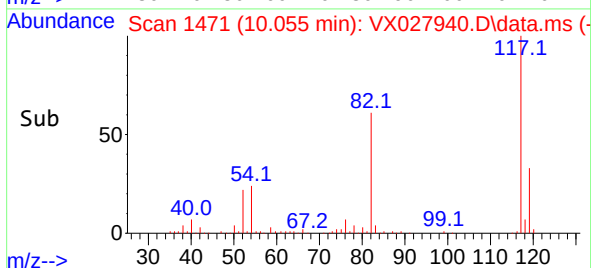
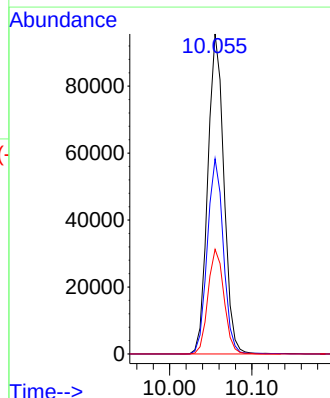
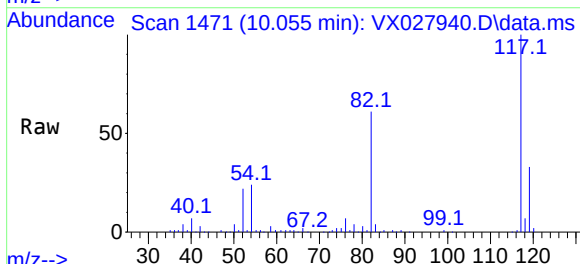




#67
Ethyl Benzene
Concen: 0.662 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. 0.000 min
Lab File: VX027940.D
Acq: 02 Apr 2022 17:51




Instrument :
MSVOA_X
ClientSampleId :
MW-6S


Tgt Ion: 91 Resp: 3075
Ion Ratio Lower Upper
91 100
106 30.7 24.6 36.8

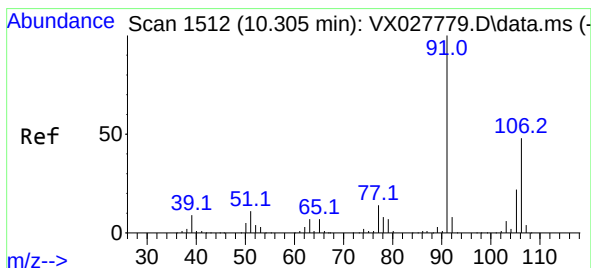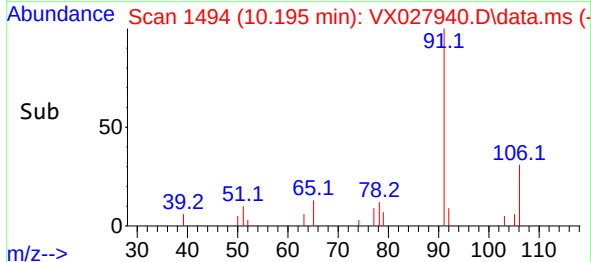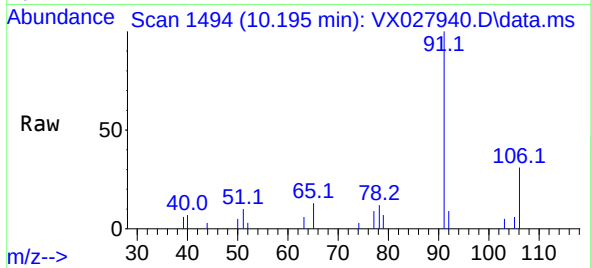

#68
m/p-Xylenes
Concen: 2.267 ug/l
RT: 10.305 min Scan# 1512
Delta R.T. 0.000 min
Lab File: VX027940.D
Acq: 02 Apr 2022 17:51

Tgt Ion: 106 Resp: 3870
Ion Ratio Lower Upper
106 100
91 210.8 160.4 240.6


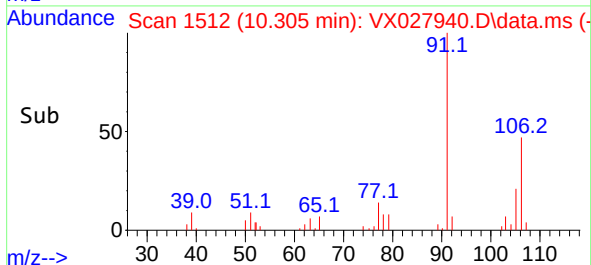
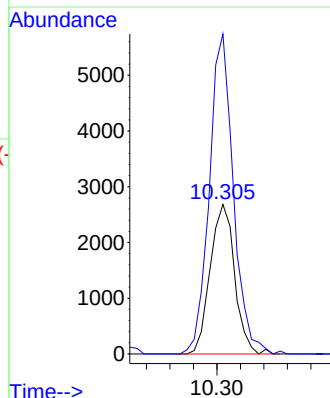
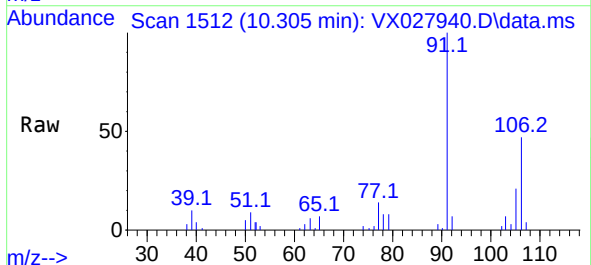




#69
o-Xylene
Concen: 0.570 ug/l
RT: 10.646 min Scan# 11
Delta R.T. 0.006 min
Lab File: VX027940.D
Acq: 02 Apr 2022 17:51




Instrument :
MSVOA_X
ClientSampleId :
MW-6S


Tgt Ion:106 Resp: 950
Ion Ratio Lower Upper
106 100
91 260.0 106.1 318.1

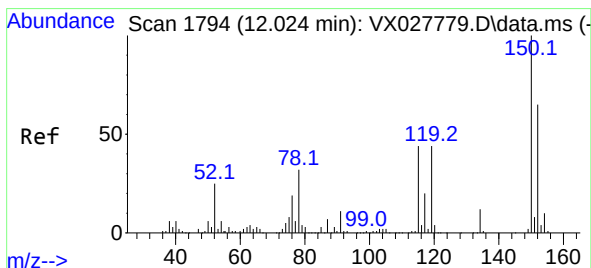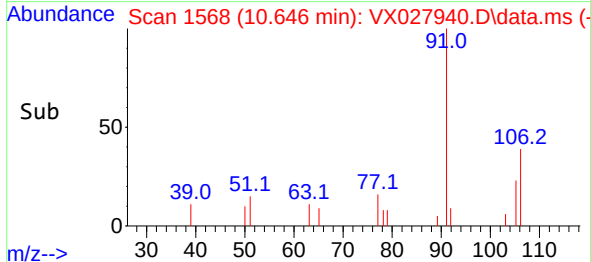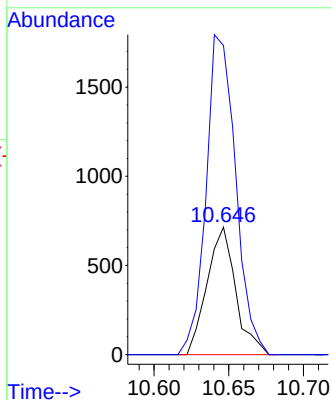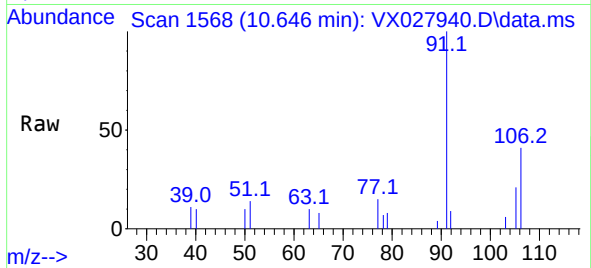

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX027940.D
Acq: 02 Apr 2022 17:51

Tgt Ion:152 Resp: 58480
Ion Ratio Lower Upper
152 100
115 64.2 37.5 112.7
150 157.0 0.0 338.2


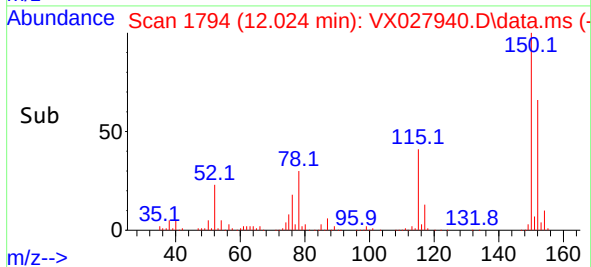
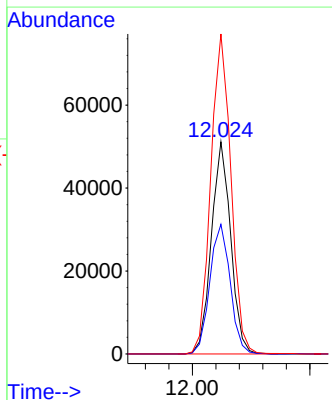
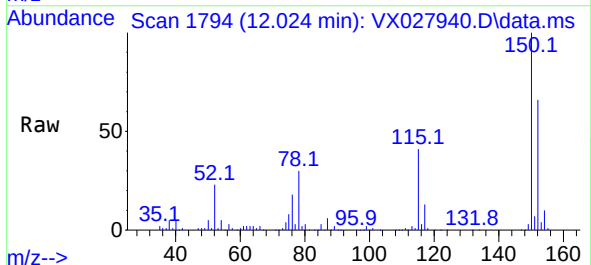




#76
1,2,3-Trichloropropane
Concen: 26.313 ug/l
RT: 11.079 min Scan# 1666
Delta R.T. -0.165 min
Lab File: VX027940.D
Acq: 02 Apr 2022 17:51




Instrument :
MSVOA_X
ClientSampleId :
MW-6S


Tgt Ion: 75 Resp: 36097
Ion Ratio Lower Upper
75 100
77 1.0 19.4 58.2#

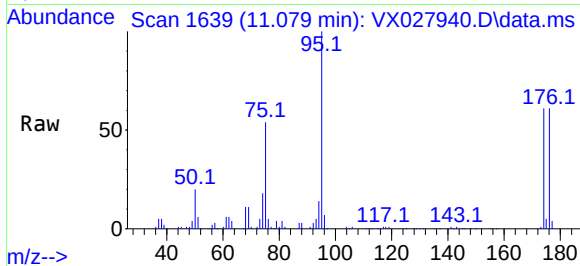

#80
1,3,5-Trimethylbenzene
Concen: 0.233 ug/l
RT: 11.451 min Scan# 1700
Delta R.T. 0.000 min
Lab File: VX027940.D
Acq: 02 Apr 2022 17:51

Tgt Ion: 105 Resp: 881
Ion Ratio Lower Upper
105 100
120 42.7 24.3 72.9


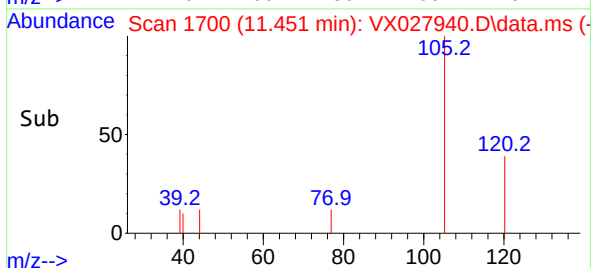

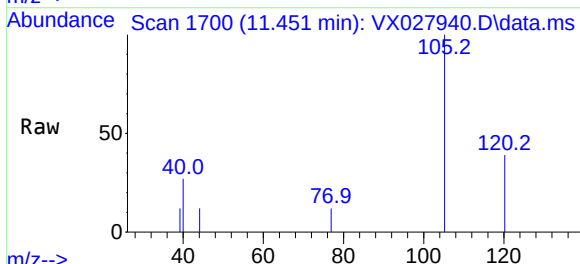




#81
trans-1,4-Dichloro-2-butene
Concen: 77.073 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.061 min
Lab File: VX027940.D
Acq: 02 Apr 2022 17:51




Instrument :
MSVOA_X
ClientSampleId :
MW-6S


Tgt Ion: 75 Resp: 36097
Ion Ratio Lower Upper
75 100
53 0.0 69.0 103.4#
89 0.0 37.0 55.6#

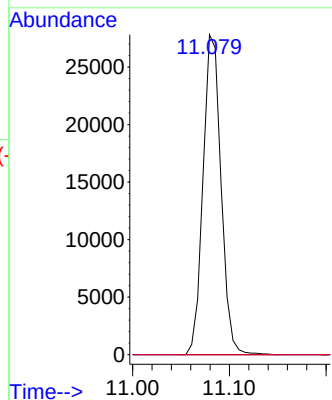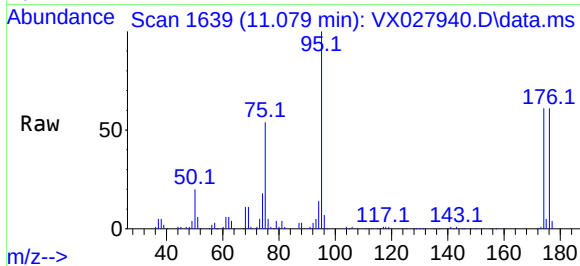

#84
1,2,4-Trimethylbenzene
Concen: 0.749 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. 0.000 min
Lab File: VX027940.D
Acq: 02 Apr 2022 17:51

Tgt Ion: 105 Resp: 2822
Ion Ratio Lower Upper
105 100
120 49.6 22.6 67.8


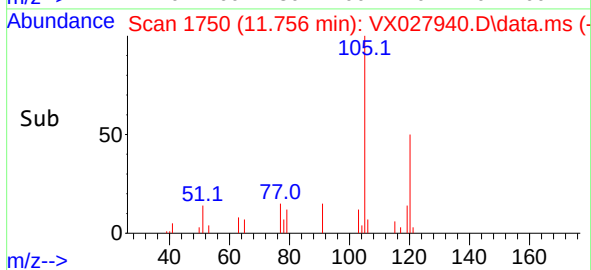
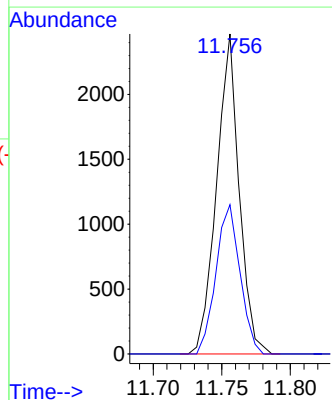
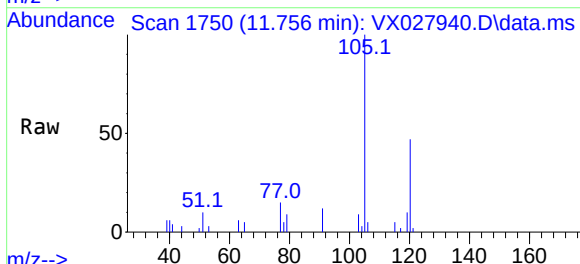




#90
Hexachloroethane
Concen: 0.961 ug/l
RT: 12.646 min Scan# 117
Delta R.T. 0.104 min
Lab File: VX027940.D
Acq: 02 Apr 2022 17:51




Instrument :
MSVOA_X
ClientSampleId :
MW-6S


Tgt Ion:117 Resp: 579
Ion Ratio Lower Upper
117 100
201 0.0 39.5 118.5#

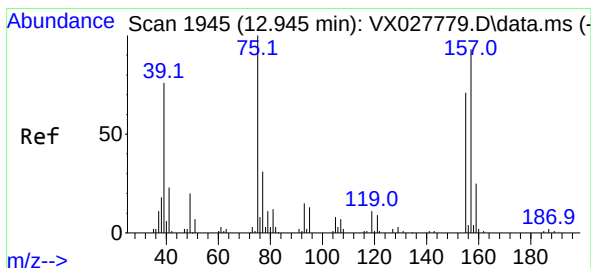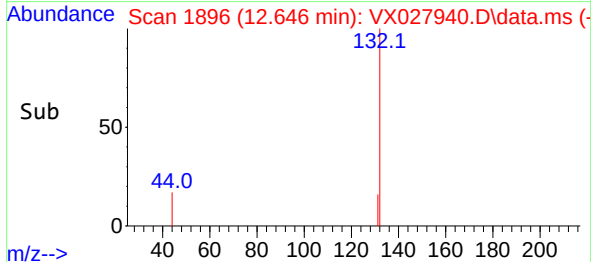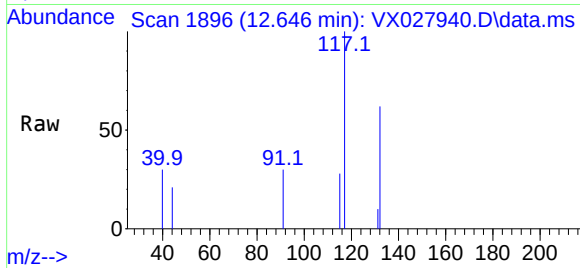

#92
1,2-Dibromo-3-Chloropropane
Concen: 0.292 ug/l
RT: 12.695 min Scan# 1904
Delta R.T. -0.250 min
Lab File: VX027940.D
Acq: 02 Apr 2022 17:51


Tgt Ion: 75 Resp: 104
Ion Ratio Lower Upper
75 100
155 0.0 47.0 141.2#
157 0.0 57.9 173.6#

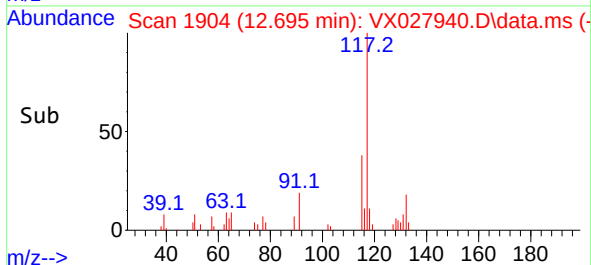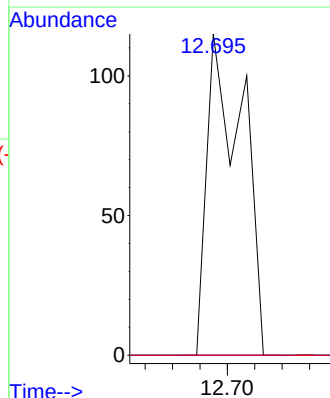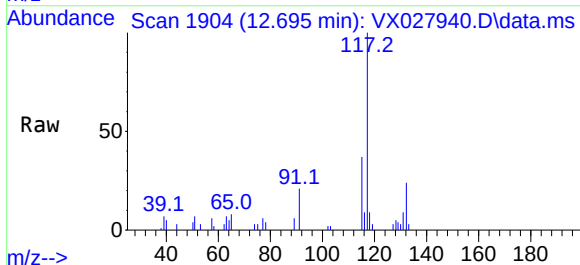

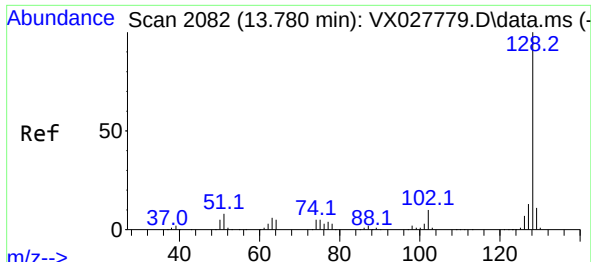

#95
Naphthalene
Concen: 0.351 ug/l
RT: 13.780 min Scan# 20
Delta R.T. 0.000 min
Lab File: VX027940.D
Acq: 02 Apr 2022 17:51

Instrument :
MSVOA_X
ClientSampleId :
MW-6S

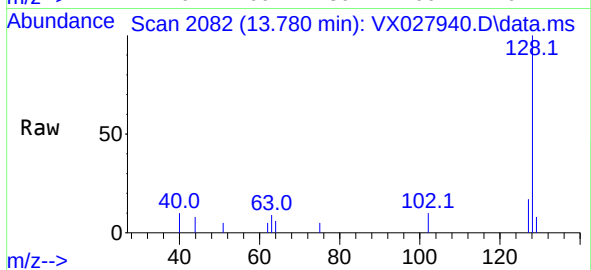

Tgt Ion:	128	Resp:	1446
Ion	Ratio	Lower	Upper
128	100		
127	11.2	10.2	15.4
129	8.1	8.7	13.1#

