

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX040222\
 Data File : VX027941.D
 Acq On : 02 Apr 2022 18:15
 Operator : JC/MD
 Sample : N2249-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-6D

Quant Time: Apr 04 04:17:36 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032922W.M
 Quant Title : SW846 8260
 QLast Update : Wed Mar 30 04:39:27 2022
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	79805	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	6.763	114	142380	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	133073	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	58587	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	60971	59.212	ug/l	0.00
Spiked Amount 50.000	Range	61 - 141	Recovery	=	118.420%	
35) Dibromofluoromethane	5.391	113	48020	52.251	ug/l	0.00
Spiked Amount 50.000	Range	69 - 133	Recovery	=	104.500%	
50) Toluene-d8	8.653	98	170543	52.742	ug/l	0.00
Spiked Amount 50.000	Range	65 - 126	Recovery	=	105.480%	
62) 4-Bromofluorobenzene	11.079	95	67178	48.887	ug/l	0.00
Spiked Amount 50.000	Range	58 - 135	Recovery	=	97.780%	
Target Compounds						
						Qvalue
5) Bromomethane	1.624	94	87	0.294	ug/l	# 73
6) Chloroethane	1.679	64	206	0.466	ug/l	# 43
9) 1,1,2-Trichlorotrifluo...	2.325	101	373	0.499	ug/l	93
11) Tert butyl alcohol	2.953	59	3676	18.585	ug/l	96
12) 1,1-Dichloroethene	2.319	96	235	0.343	ug/l	83
13) Acrolein	2.209	56	118	0.797	ug/l	# 1
14) Allyl chloride	2.782	41	6527	5.185	ug/l	# 68
15) Acrylonitrile	3.105	53	555	1.195	ug/l	# 27
16) Acetone	2.380	43	1294	2.840	ug/l	# 87
18) Methyl Acetate	2.782	43	14543	12.946	ug/l	# 46
19) Methyl tert-butyl Ether	3.117	73	19456	7.448	ug/l	# 55
20) Methylene Chloride	2.794	84	295	0.360	ug/l	# 30
22) Diisopropyl ether	3.770	45	1155	0.458	ug/l	# 76
23) Vinyl Acetate	3.757	43	755	0.346	ug/l	# 66
25) 2-Butanone	4.574	43	140	0.211	ug/l	# 44
29) Tetrahydrofuran	5.038	42	288	0.676	ug/l	# 30
30) Chloroform	5.093	83	765	0.485	ug/l	# 77
31) Cyclohexane	5.483	56	864	0.759	ug/l	# 69
36) 1,1-Dichloropropene	5.550	75	7012	6.058	ug/l	# 49
38) Carbon Tetrachloride	5.550	117	9167	7.168	ug/l	# 15
40) Benzene	6.050	78	23255	6.629	ug/l	91
43) Isopropyl Acetate	6.233	43	7772	3.381	ug/l	# 56
44) Trichloroethene	7.129	130	1631	1.711	ug/l	82
52) Toluene	8.720	92	741	0.335	ug/l	94
56) Ethyl methacrylate	8.842	69	1272	0.820	ug/l	# 44
59) 2-Hexanone	9.561	43	268	0.218	ug/l	87
60) Dibromochloromethane	9.281	129	292	0.287	ug/l	# 9
64) Tetrachloroethene	9.275	164	241	0.267	ug/l	# 71
67) Ethyl Benzene	10.195	91	3111	0.654	ug/l	99
68) m/p-Xylenes	10.305	106	2472	1.413	ug/l	95
69) o-Xylene	10.646	106	656	0.384	ug/l	78
76) 1,2,3-Trichloropropane	11.079	75	34333	24.981	ug/l	# 38
81) trans-1,4-Dichloro-2-b...	11.079	75	34333	73.350	ug/l	# 15
84) 1,2,4-Trimethylbenzene	11.756	105	2077	0.550	ug/l	96
85) sec-Butylbenzene	11.890	105	909	0.201	ug/l	91
90) Hexachloroethane	12.646	117	544	0.902	ug/l	# 10

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX040222\
Data File : VX027941.D
Acq On : 02 Apr 2022 18:15
Operator : JC/MD
Sample : N2249-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-6D


Quant Time: Apr 04 04:17:36 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032922W.M
Quant Title : SW846 8260
QLast Update : Wed Mar 30 04:39:27 2022
Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
95) Naphthalene	13.780	128	842	0.204	ug/l #	85

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Apr 04 04:17:36 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032922W.M
Quant Title : SW846 8260
QLast Update : Wed Mar 30 04:39:27 2022
Response via : Initial Calibration









#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX027941.D
Acq: 02 Apr 2022 18:15




Instrument :
MSVOA_X
ClientSampleId :
MW-6D

Tgt Ion:168 Resp: 79805
Ion Ratio Lower Upper
168 100
99 65.9 41.7 62.5#

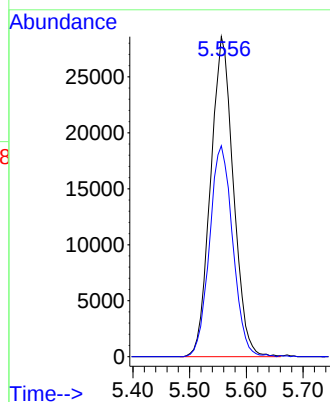


#5
Bromomethane
Concen: 0.294 ug/l
RT: 1.624 min Scan# 88
Delta R.T. 0.025 min
Lab File: VX027941.D
Acq: 02 Apr 2022 18:15


Tgt Ion: 94 Resp: 87
Ion Ratio Lower Upper
94 100
96 67.8 75.3 112.9#

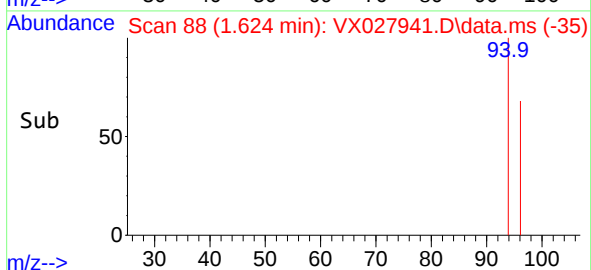


Abundance Scan 97 (1.678 min): VX027779.D\data.ms (-90)

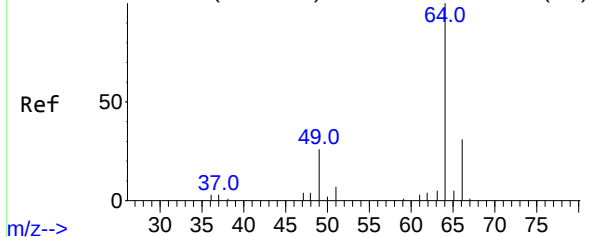

m/z--> Scan 97 (1.679 min): VX027941.D\data.ms

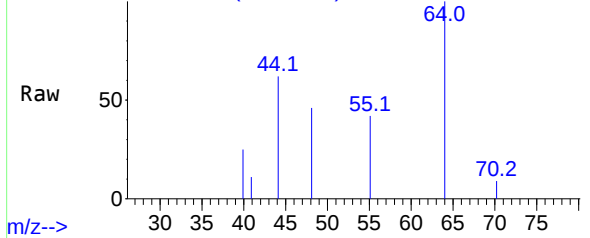

Abundance Scan 97 (1.679 min): VX027941.D\data.ms (-48)

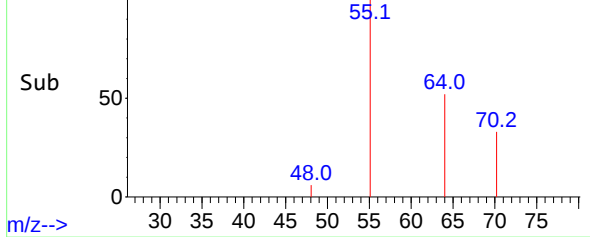

m/z-->

#6

Chloroethane

Concen: 0.466 ug/l

RT: 1.679 min Scan# 91

Delta R.T. 0.001 min

Lab File: VX027941.D

Acq: 02 Apr 2022 18:15

Instrument :

MSVOA_X

ClientSampleId :

MW-6D


Tgt Ion: 64 Resp: 206

Ion Ratio Lower Upper


64 100

66 0.0 25.3 37.9#


Abundance

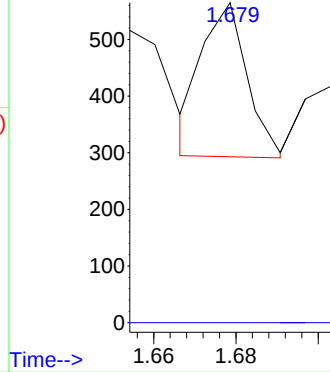


Abundance Scan 204 (2.331 min): VX027779.D\data.ms (-19)

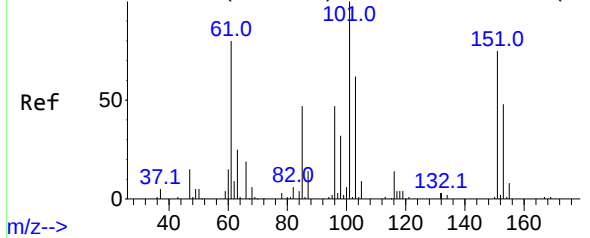

m/z--> Scan 203 (2.325 min): VX027941.D\data.ms

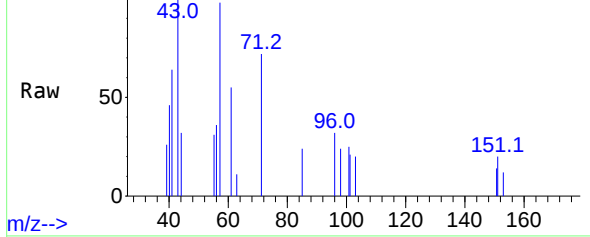

Abundance Scan 203 (2.325 min): VX027941.D\data.ms (-15)

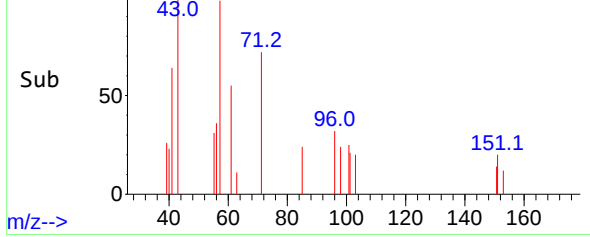

m/z-->

#9

1,1,2-Trichlorotrifluoroethane

Concen: 0.499 ug/l

RT: 2.325 min Scan# 203

Delta R.T. -0.006 min

Lab File: VX027941.D

Acq: 02 Apr 2022 18:15

Tgt Ion:101 Resp: 373


Ion Ratio Lower Upper


101 100

85 49.6 33.5 50.3

151 80.4 61.8 92.6

Abundance

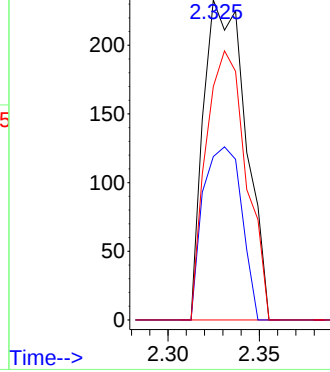



#11

Tert butyl alcohol

Concen: 18.585 ug/l

RT: 2.953 min Scan# 308

Delta R.T. -0.012 min

Lab File: VX027941.D

Acq: 02 Apr 2022 18:15

Instrument :

MSVOA_X

ClientSampleId :





MW-6D

Tgt Ion: 59 Resp: 3676

Ion Ratio Lower Upper

59 100

57 9.1 8.3 12.5



#12

1,1-Dichloroethene

Concen: 0.343 ug/l

RT: 2.319 min Scan# 202

Delta R.T. -0.000 min

Lab File: VX027941.D

Acq: 02 Apr 2022 18:15




Tgt Ion: 96 Resp: 235


Ion Ratio Lower Upper

96 100

61 127.8 124.6 187.0

98 68.3 51.0 76.4



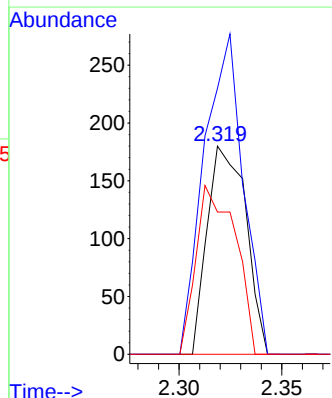





#13
Acrolein
Concen: 0.797 ug/l
RT: 2.209 min Scan# 118
Delta R.T. -0.024 min
Lab File: VX027941.D
Acq: 02 Apr 2022 18:15




Instrument :
MSVOA_X
ClientSampleId :
MW-6D


Tgt Ion: 56 Resp: 118
Ion Ratio Lower Upper
56 100
55 3465.3 55.0 82.6#



#14
Allyl chloride
Concen: 5.185 ug/l
RT: 2.782 min Scan# 278
Delta R.T. 0.116 min
Lab File: VX027941.D
Acq: 02 Apr 2022 18:15

Tgt Ion: 41 Resp: 6527
Ion Ratio Lower Upper
41 100
39 55.5 50.4 75.6
76 0.0 32.7 49.1#


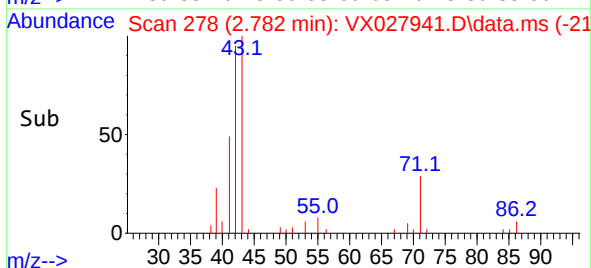
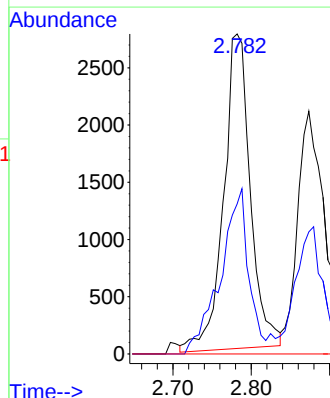





#15
Acrylonitrile
Concen: 1.195 ug/l
RT: 3.105 min Scan# 31
Delta R.T. 0.043 min
Lab File: VX027941.D
Acq: 02 Apr 2022 18:15




Instrument :
MSVOA_X
ClientSampleId :
MW-6D


Tgt Ion: 53 Resp: 555
Ion Ratio Lower Upper
53 100
52 0.0 65.7 98.5#
51 53.5 28.4 42.6#



#16
Acetone
Concen: 2.840 ug/l
RT: 2.380 min Scan# 212
Delta R.T. -0.000 min
Lab File: VX027941.D
Acq: 02 Apr 2022 18:15

Tgt Ion: 43 Resp: 1294
Ion Ratio Lower Upper
43 100
58 28.2 28.8 43.2#

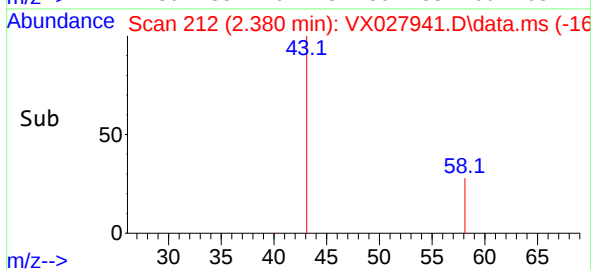



#18

Methyl Acetate

Concen: 12.946 ug/l

RT: 2.782 min Scan# 21

Delta R.T. 0.079 min

Lab File: VX027941.D

Acq: 02 Apr 2022 18:15

Instrument :

MSVOA_X

ClientSampleId :





MW-6D

Tgt Ion: 43 Resp: 14543

Ion Ratio Lower Upper

43 100

74 0.0 22.8 34.2#

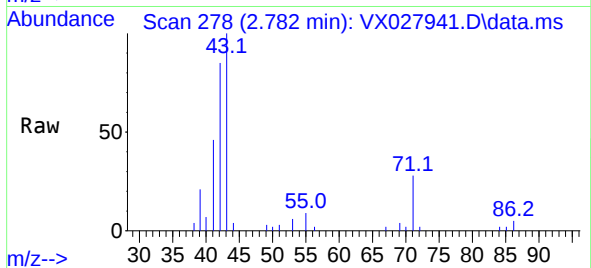

#19

Methyl tert-butyl Ether

Concen: 7.448 ug/l

RT: 3.117 min Scan# 333

Delta R.T. 0.006 min

Lab File: VX027941.D




Acq: 02 Apr 2022 18:15


Tgt Ion: 73 Resp: 19456

Ion Ratio Lower Upper

73 100

57 42.1 16.8 25.2#

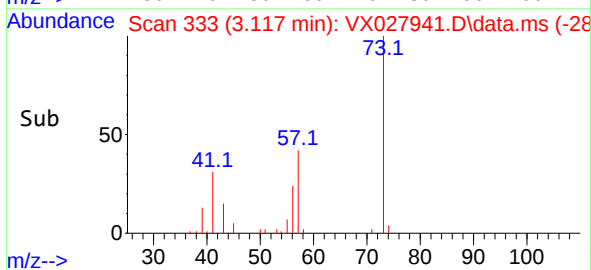







#20
Methylene Chloride
Concen: 0.360 ug/l
RT: 2.794 min Scan# 21
Delta R.T. 0.006 min
Lab File: VX027941.D
Acq: 02 Apr 2022 18:15

Instrument :
MSVOA_X
ClientSampleId :
MW-6D

Tgt Ion: 84 Resp: 295




Ion	Ratio	Lower	Upper
84	100		
49	120.3	85.5	128.3
51	81.6	26.6	39.8#
86	188.6	51.5	77.3#

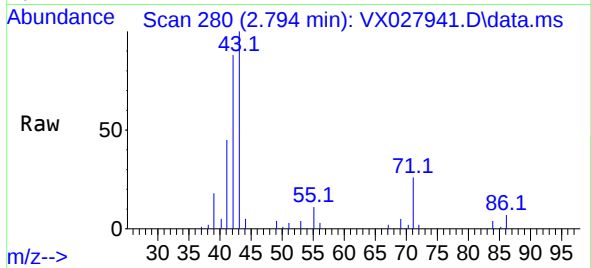


#22
Diisopropyl ether
Concen: 0.458 ug/l
RT: 3.770 min Scan# 440
Delta R.T. 0.007 min
Lab File: VX027941.D
Acq: 02 Apr 2022 18:15

Tgt Ion: 45 Resp: 1155

Ion	Ratio	Lower	Upper
45	100		
43	39.8	50.8	76.2#
87	37.7	26.6	39.8
59	0.0	10.5	15.7#


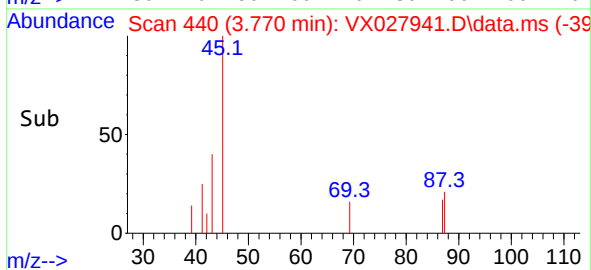






#23
 Vinyl Acetate
 Concen: 0.346 ug/l
 RT: 3.757 min Scan# 41
 Delta R.T. 0.030 min
 Lab File: VX027941.D
 Acq: 02 Apr 2022 18:15




Instrument :
 MSVOA_X
 ClientSampleId :
 MW-6D


Tgt Ion: 43 Resp: 755
 Ion Ratio Lower Upper
 43 100
 86 0.0 10.8 16.2#

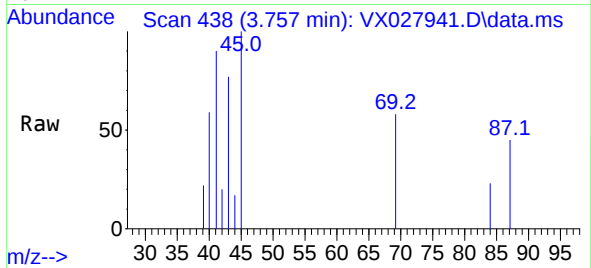

#25
 2-Butanone
 Concen: 0.211 ug/l
 RT: 4.574 min Scan# 572
 Delta R.T. 0.018 min
 Lab File: VX027941.D
 Acq: 02 Apr 2022 18:15

Tgt Ion: 43 Resp: 140
 Ion Ratio Lower Upper
 43 100
 72 0.0 24.4 36.6#

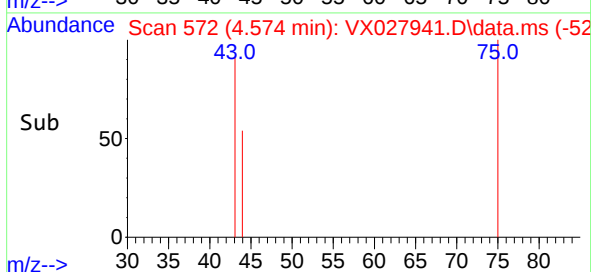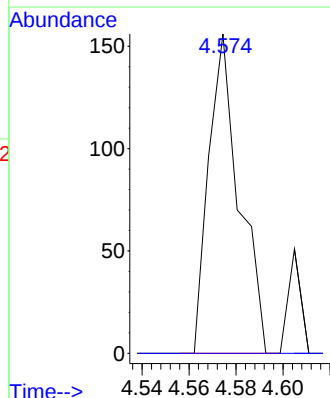



#29

Tetrahydrofuran

Concen: 0.676 ug/l

RT: 5.038 min Scan# 64

Delta R.T. 0.031 min

Lab File: VX027941.D

Acq: 02 Apr 2022 18:15

Instrument :

MSVOA_X

ClientSampleId :

MW-6D





Tgt Ion: 42 Resp: 288

Ion Ratio Lower Upper

42 100

72 6.6 44.1 66.1#

71 0.0 40.5 60.7#

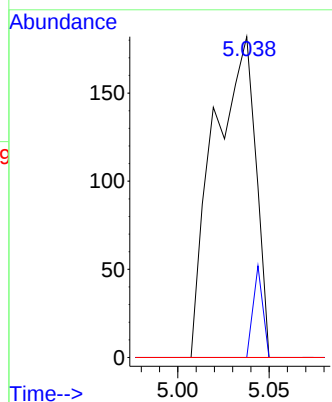

#30

Chloroform

Concen: 0.485 ug/l

RT: 5.093 min Scan# 657

Delta R.T. -0.006 min

Lab File: VX027941.D




Acq: 02 Apr 2022 18:15


Tgt Ion: 83 Resp: 765

Ion Ratio Lower Upper

83 100

85 84.3 52.7 79.1#









#31
Cyclohexane
Concen: 0.759 ug/l
RT: 5.483 min Scan# 721
Delta R.T. 0.006 min
Lab File: VX027941.D
Acq: 02 Apr 2022 18:15




Instrument :
MSVOA_X
ClientSampleId :
MW-6D


Tgt Ion: 56 Resp: 864
Ion Ratio Lower Upper
56 100
69 4.3 26.7 40.1#
84 73.0 77.2 115.8#



#33
1,2-Dichloroethane-d4
Concen: 59.212 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.000 min
Lab File: VX027941.D
Acq: 02 Apr 2022 18:15

Tgt Ion: 65 Resp: 60971
Ion Ratio Lower Upper
65 100
67 51.1 0.0 107.4

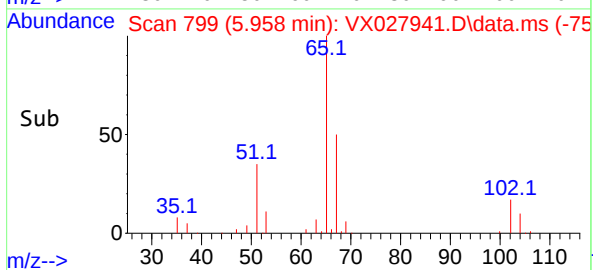



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.763 min Scan# 91

Delta R.T. 0.000 min

Lab File: VX027941.D

Acq: 02 Apr 2022 18:15

Instrument :

MSVOA_X

ClientSampleId :

MW-6D





Tgt Ion:114 Resp: 142380

Ion Ratio Lower Upper

114 100

63 21.7 0.0 36.8

88 16.9 0.0 32.4

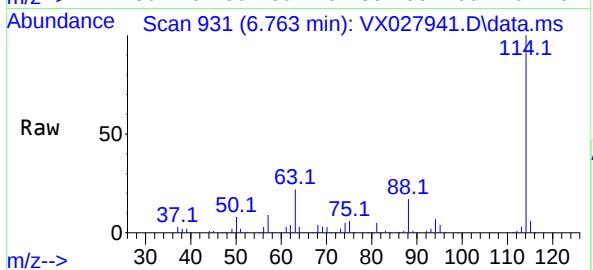

#35

Dibromofluoromethane

Concen: 52.251 ug/l

RT: 5.391 min Scan# 706

Delta R.T. 0.000 min

Lab File: VX027941.D

Acq: 02 Apr 2022 18:15




Tgt Ion:113 Resp: 48020


Ion Ratio Lower Upper

113 100

111 103.1 82.8 124.2

192 17.6 16.9 25.3


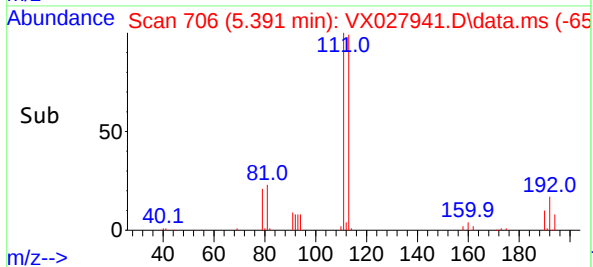

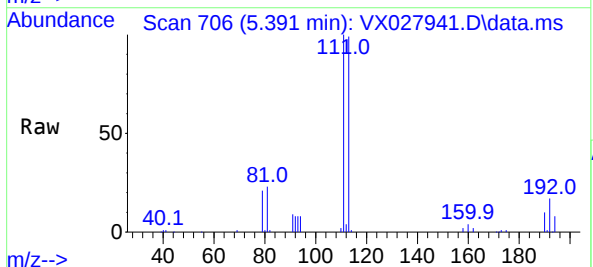




#36
1,1-Dichloropropene
Concen: 6.058 ug/l
RT: 5.550 min Scan# 712
Delta R.T. -0.140 min
Lab File: VX027941.D
Acq: 02 Apr 2022 18:15




Instrument :
MSVOA_X
ClientSampleId :
MW-6D


Tgt Ion: 75 Resp: 7012
Ion Ratio Lower Upper
75 100
110 8.7 18.3 54.8#
77 0.0 24.8 37.2#



#38
Carbon Tetrachloride
Concen: 7.168 ug/l
RT: 5.550 min Scan# 732
Delta R.T. -0.134 min
Lab File: VX027941.D
Acq: 02 Apr 2022 18:15

Tgt Ion: 117 Resp: 9167
Ion Ratio Lower Upper
117 100
119 4.8 77.3 115.9#
121 0.0 24.2 36.2#



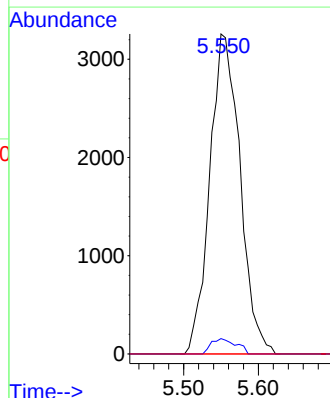





#40
Benzene
Concen: 6.629 ug/l
RT: 6.050 min Scan# 812
Delta R.T. 0.013 min
Lab File: VX027941.D
Acq: 02 Apr 2022 18:15




Instrument :
MSVOA_X
ClientSampleId :
MW-6D


Tgt Ion: 78 Resp: 23255
Ion Ratio Lower Upper
78 100
77 19.5 19.3 28.9



#43
Isopropyl Acetate
Concen: 3.381 ug/l
RT: 6.233 min Scan# 844
Delta R.T. -0.109 min
Lab File: VX027941.D
Acq: 02 Apr 2022 18:15

Tgt Ion: 43 Resp: 7772
Ion Ratio Lower Upper
43 100
61 0.0 18.5 27.7#
87 0.0 13.0 19.6#


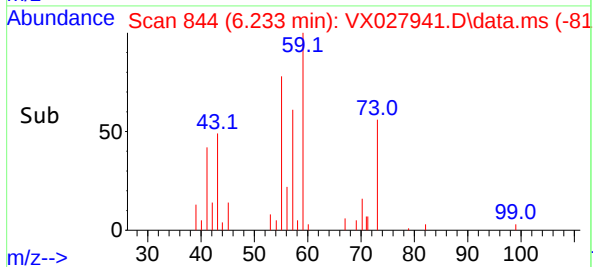

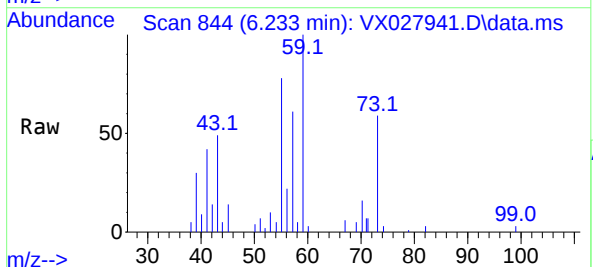




#44
Trichloroethene
Concen: 1.711 ug/l
RT: 7.129 min Scan# 991
Delta R.T. -0.000 min
Lab File: VX027941.D
Acq: 02 Apr 2022 18:15




Instrument :
MSVOA_X
ClientSampleId :
MW-6D


Tgt Ion:130 Resp: 1631
Ion Ratio Lower Upper
130 100
95 112.0 0.0 188.8



#50
Toluene-d8
Concen: 52.742 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. -0.000 min
Lab File: VX027941.D
Acq: 02 Apr 2022 18:15

Tgt Ion: 98 Resp: 170543
Ion Ratio Lower Upper
98 100
100 65.2 52.6 78.8



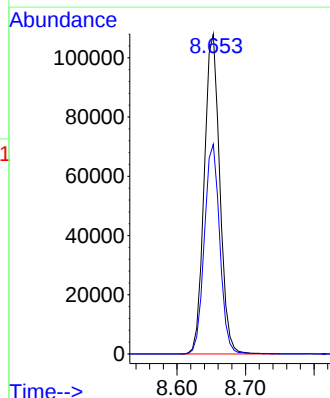





#52
Toluene
Concen: 0.335 ug/l
RT: 8.720 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX027941.D
Acq: 02 Apr 2022 18:15




Instrument :
MSVOA_X
ClientSampleId :
MW-6D


Tgt Ion: 92 Resp: 741
Ion Ratio Lower Upper
92 100
91 163.7 137.5 206.3

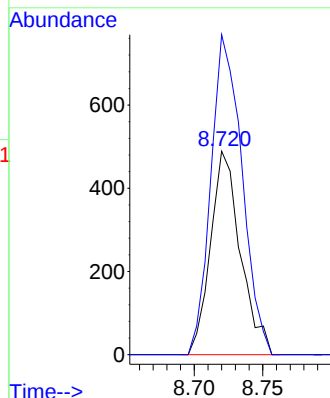

#56
Ethyl methacrylate
Concen: 0.820 ug/l
RT: 8.842 min Scan# 1272
Delta R.T. -0.274 min
Lab File: VX027941.D
Acq: 02 Apr 2022 18:15

Tgt Ion: 69 Resp: 1272
Ion Ratio Lower Upper
69 100
41 101.5 43.8 65.6#
39 47.5 22.2 33.2#

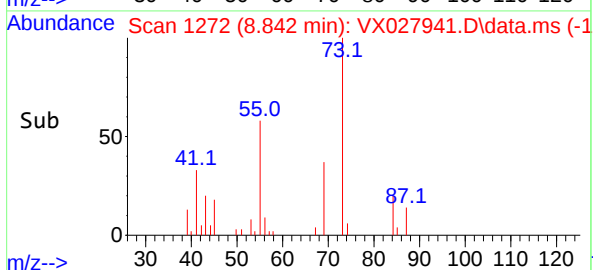



#59

2-Hexanone

Concen: 0.218 ug/l

RT: 9.561 min Scan# 1390

Delta R.T. 0.128 min

Lab File: VX027941.D

Acq: 02 Apr 2022 18:15

Instrument :

MSVOA_X

ClientSampleId :





MW-6D

Tgt Ion: 43 Resp: 268

Ion Ratio Lower Upper

43 100

58 53.7 31.9 95.7

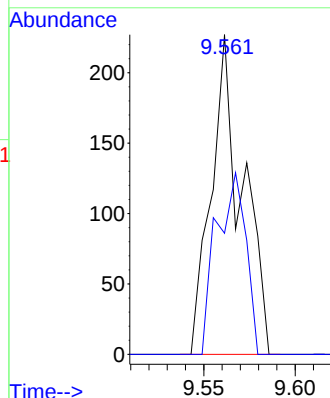

#60

Dibromochloromethane

Concen: 0.287 ug/l

RT: 9.281 min Scan# 1344

Delta R.T. -0.244 min

Lab File: VX027941.D




Acq: 02 Apr 2022 18:15


Tgt Ion: 129 Resp: 292

Ion Ratio Lower Upper

129 100

127 0.0 40.3 120.8#



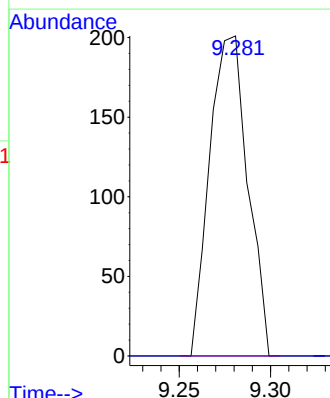





#62
4-Bromofluorobenzene
Concen: 48.887 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.006 min
Lab File: VX027941.D
Acq: 02 Apr 2022 18:15




Instrument :
MSVOA_X
ClientSampleId :
MW-6D


Tgt Ion: 95 Resp: 67178
Ion Ratio Lower Upper
95 100
174 71.8 0.0 163.0
176 70.2 0.0 155.0

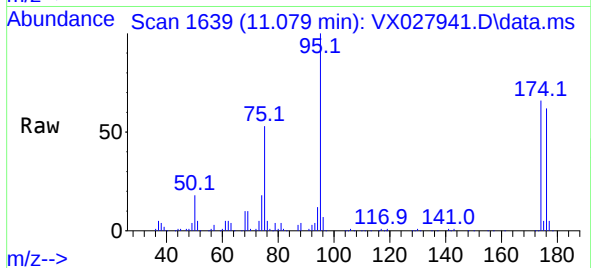

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX027941.D
Acq: 02 Apr 2022 18:15

Tgt Ion: 117 Resp: 133073
Ion Ratio Lower Upper
117 100
82 56.9 41.8 62.8
119 31.7 24.8 37.2


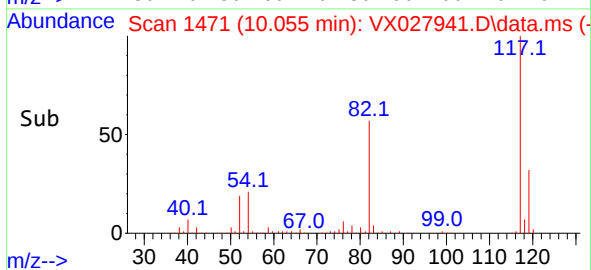




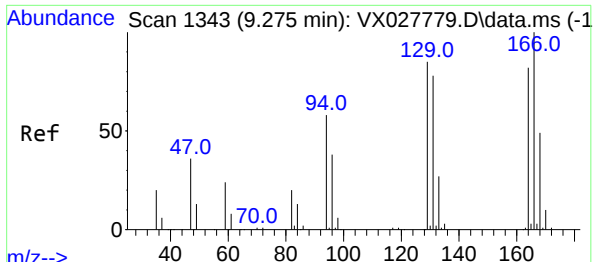

#64
Tetrachloroethene
Concen: 0.267 ug/l
RT: 9.275 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX027941.D
Acq: 02 Apr 2022 18:15




Instrument :
MSVOA_X
ClientSampleId :
MW-6D


Tgt Ion:164 Resp: 241
Ion Ratio Lower Upper
164 100
166 144.0 101.2 151.8
129 108.8 73.0 109.4
131 147.3 74.2 111.2#

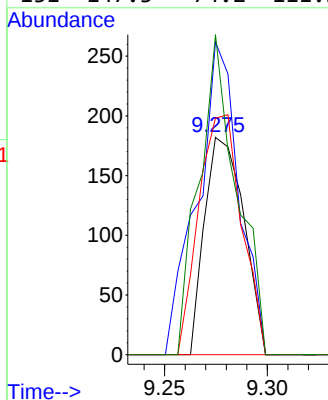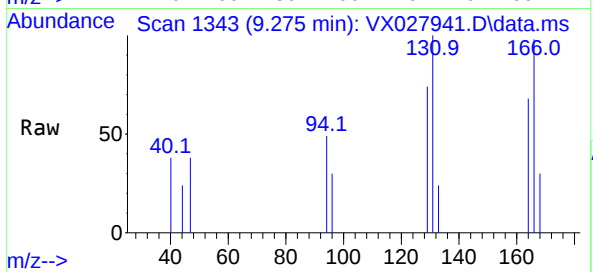

#67
Ethyl Benzene
Concen: 0.654 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. 0.000 min
Lab File: VX027941.D
Acq: 02 Apr 2022 18:15

Tgt Ion: 91 Resp: 3111
Ion Ratio Lower Upper
91 100
106 31.5 24.6 36.8


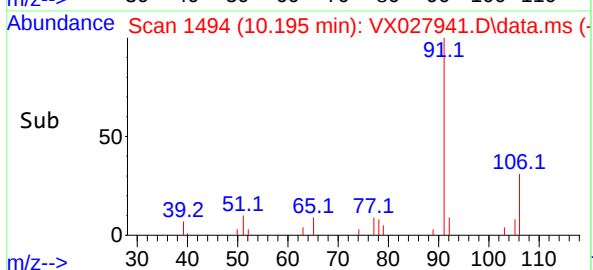
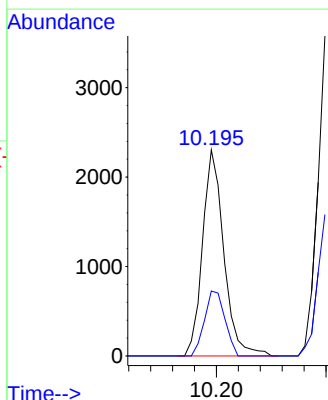
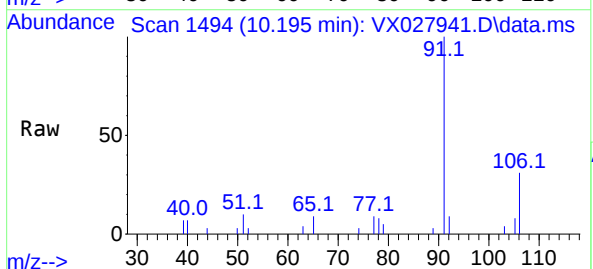




#68
m/p-Xylenes
Concen: 1.413 ug/l
RT: 10.305 min Scan# 1512
Delta R.T. 0.000 min
Lab File: VX027941.D
Acq: 02 Apr 2022 18:15




Instrument :
MSVOA_X
ClientSampleId :
MW-6D


Tgt Ion:106 Resp: 2472
Ion Ratio Lower Upper
106 100
91 207.4 160.4 240.6

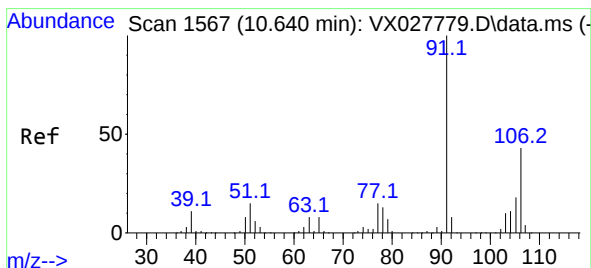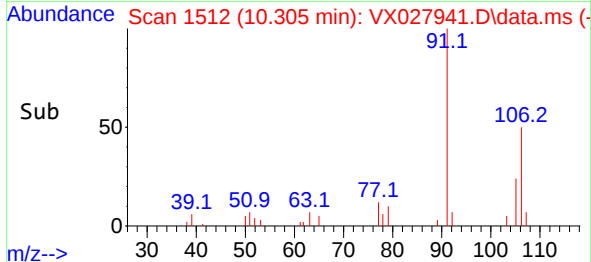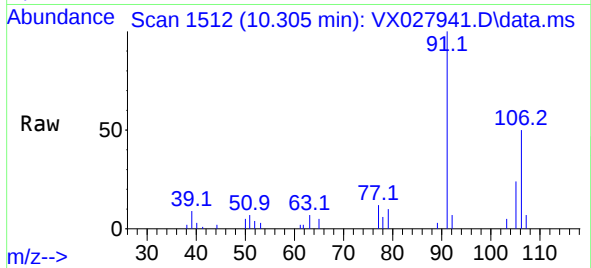

#69
o-Xylene
Concen: 0.384 ug/l
RT: 10.646 min Scan# 1568
Delta R.T. 0.006 min
Lab File: VX027941.D
Acq: 02 Apr 2022 18:15

Tgt Ion:106 Resp: 656
Ion Ratio Lower Upper
106 100
91 247.4 106.1 318.1


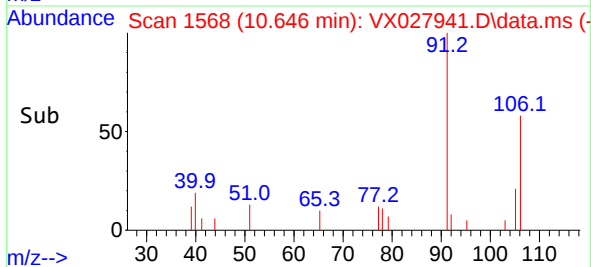

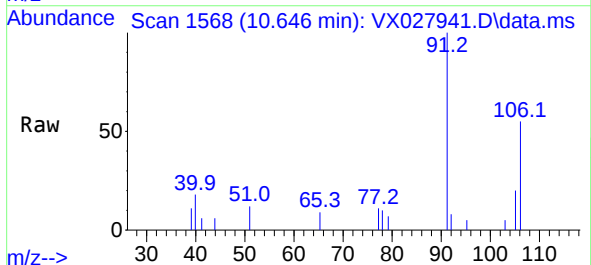




#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX027941.D
Acq: 02 Apr 2022 18:15




Instrument :
MSVOA_X
ClientSampleId :
MW-6D


Tgt Ion:152 Resp: 58587
Ion Ratio Lower Upper
152 100
115 64.4 37.5 112.7
150 156.6 0.0 338.2

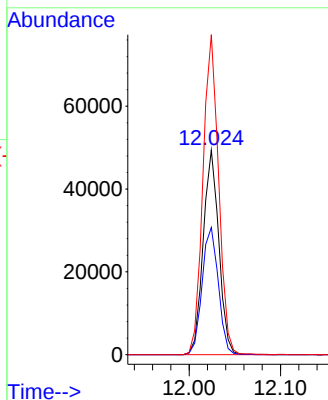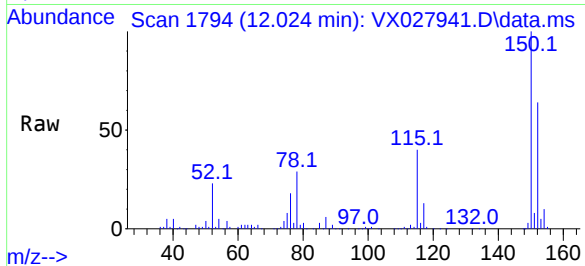

#76
1,2,3-Trichloropropane
Concen: 24.981 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.165 min
Lab File: VX027941.D
Acq: 02 Apr 2022 18:15

Tgt Ion: 75 Resp: 34333
Ion Ratio Lower Upper
75 100
77 0.9 19.4 58.2#


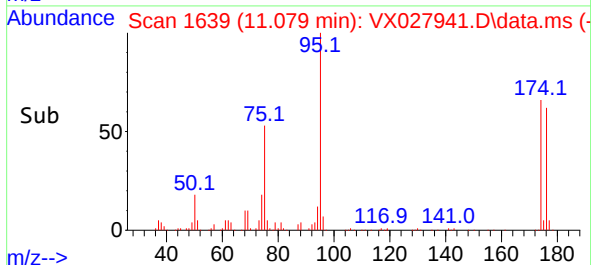
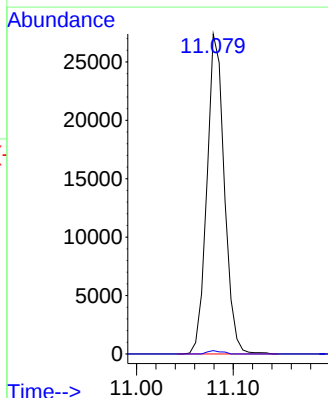
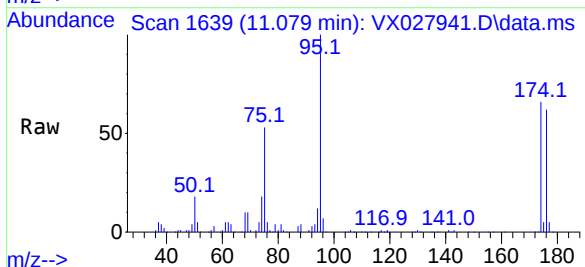




#81
trans-1,4-Dichloro-2-butene
Concen: 73.350 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.061 min
Lab File: VX027941.D
Acq: 02 Apr 2022 18:15




Instrument :
MSVOA_X
ClientSampleId :
MW-6D


Tgt Ion: 75 Resp: 34333
Ion Ratio Lower Upper
75 100
53 0.0 69.0 103.4#
89 0.0 37.0 55.6#

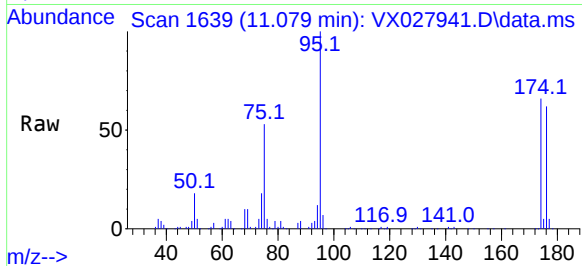

#84
1,2,4-Trimethylbenzene
Concen: 0.550 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. 0.000 min
Lab File: VX027941.D
Acq: 02 Apr 2022 18:15

Tgt Ion: 105 Resp: 2077
Ion Ratio Lower Upper
105 100
120 47.8 22.6 67.8


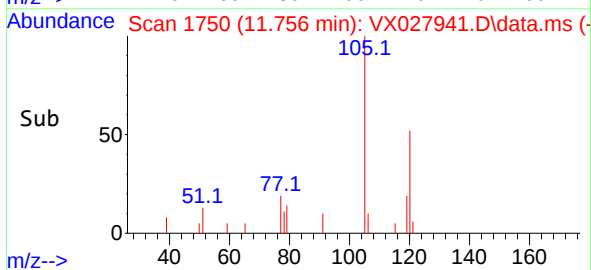

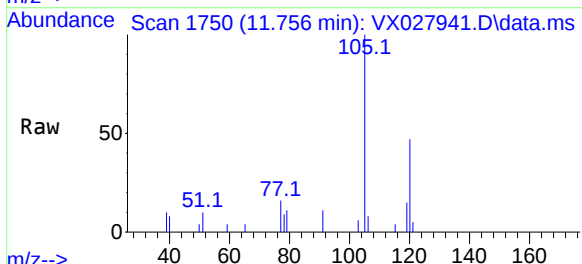




#85
sec-Butylbenzene
Concen: 0.201 ug/l
RT: 11.890 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX027941.D
Acq: 02 Apr 2022 18:15




Instrument :
MSVOA_X
ClientSampleId :
MW-6D


Tgt Ion:105 Resp: 909
Ion Ratio Lower Upper
105 100
134 16.0 10.2 30.4

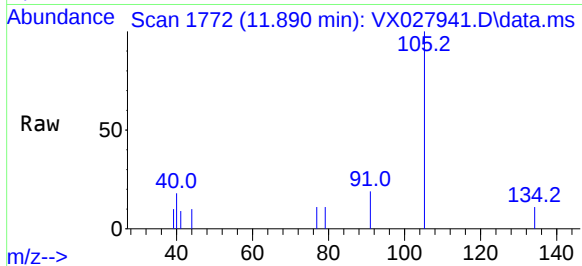

#90
Hexachloroethane
Concen: 0.902 ug/l
RT: 12.646 min Scan# 1896
Delta R.T. 0.104 min
Lab File: VX027941.D
Acq: 02 Apr 2022 18:15

Tgt Ion:117 Resp: 544
Ion Ratio Lower Upper
117 100
201 0.0 39.5 118.5#

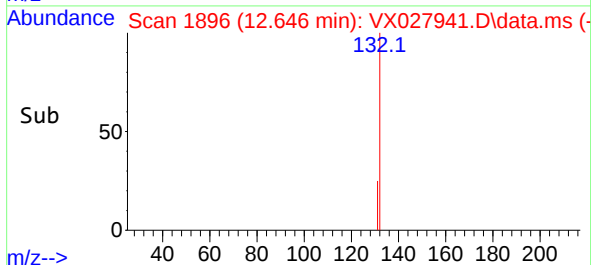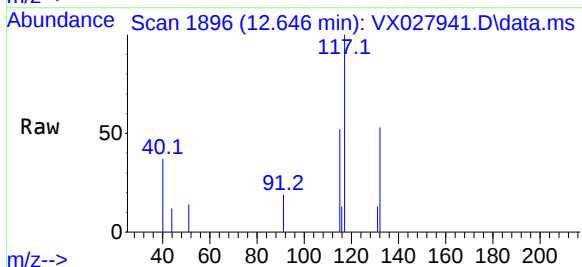

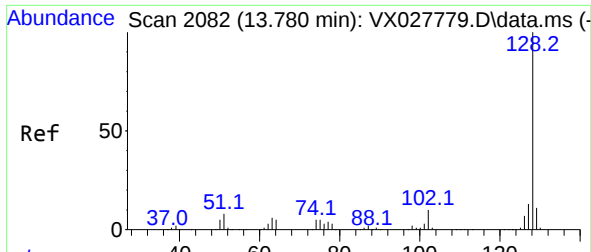

#95

Naphthalene

Concen: 0.204 ug/l

RT: 13.780 min Scan# 2082

Delta R.T. 0.000 min

Lab File: VX027941.D


Acq: 02 Apr 2022 18:15

Instrument :

MSVOA_X

ClientSampleId :

MW-6D

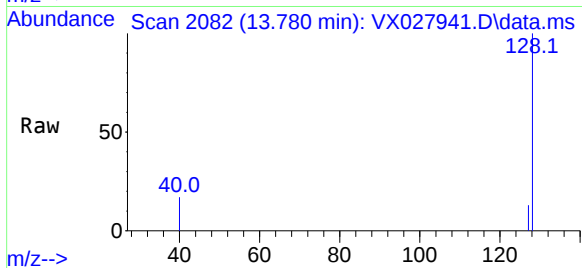

Tgt Ion:	128	Resp:	842
Ion	Ratio	Lower	Upper
128	100		
127	16.7	10.2	15.4#
129	3.2	8.7	13.1#

