

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX040222\
 Data File : VX027934.D
 Acq On : 02 Apr 2022 15:32
 Operator : JC/MD
 Sample : N2204-07RE
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 FIELD-BLANKRE

Quant Time: Apr 04 04:15:37 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032922W.M
 Quant Title : SW846 8260
 QLast Update : Wed Mar 30 04:39:27 2022
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.556	168	77596	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	6.763	114	137554	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	125937	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	55016	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	61752	61.678	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	= 123.360%	
35) Dibromofluoromethane	5.385	113	47851	53.894	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	= 107.780%	
50) Toluene-d8	8.653	98	164148	52.545	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	= 105.080%	
62) 4-Bromofluorobenzene	11.079	95	64030	48.231	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	= 96.460%	
Target Compounds						
16) Acetone	2.380	43	1118	2.523	ug/l	Qvalue 90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX040222\
Data File : VX027934.D
Acq On : 02 Apr 2022 15:32
Operator : JC/MD
Sample : N2204-07RE
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FIELD-BLANKRE


Quant Time: Apr 04 04:15:37 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032922W.M
Quant Title : SW846 8260
QLast Update : Wed Mar 30 04:39:27 2022
Response via : Initial Calibration

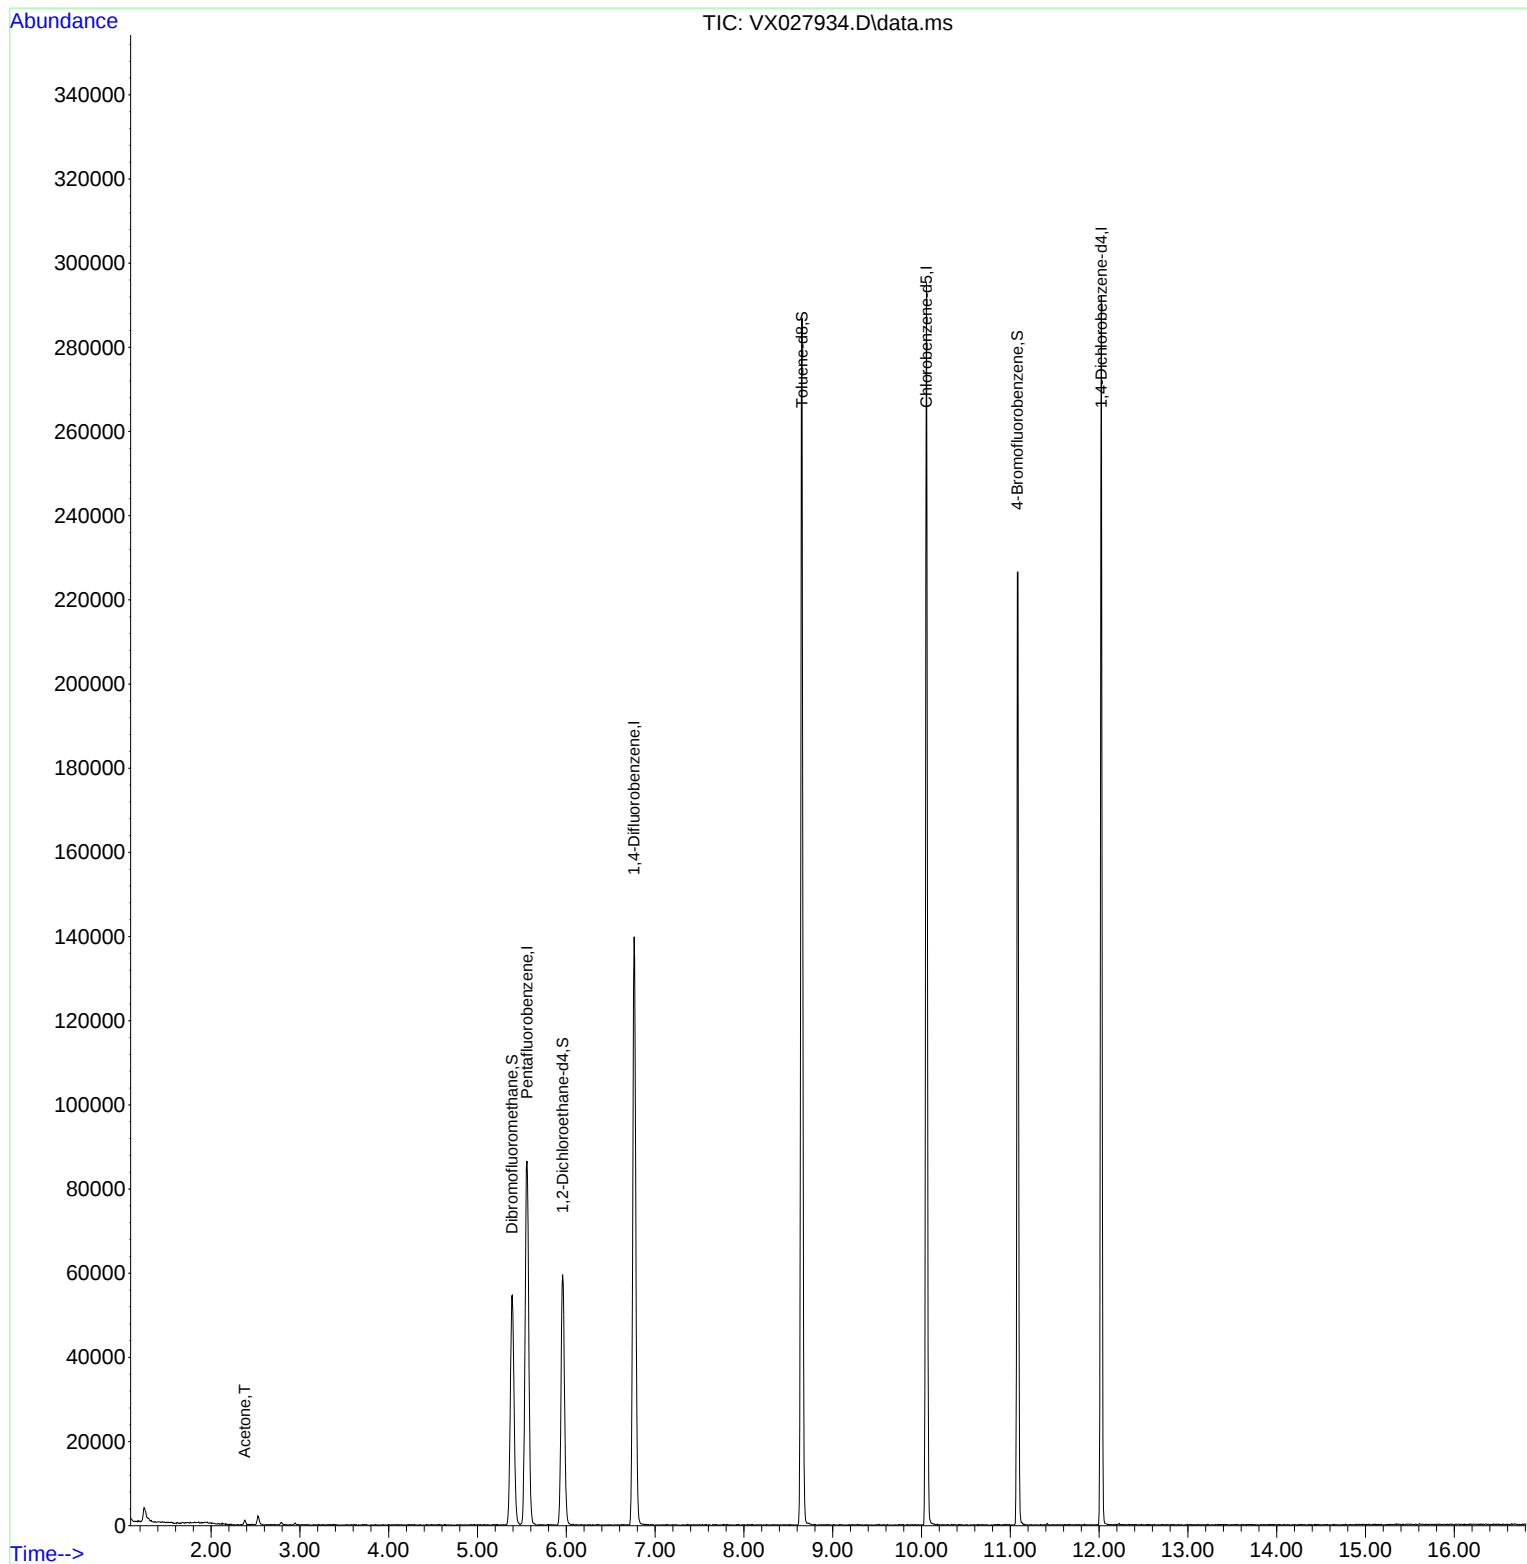



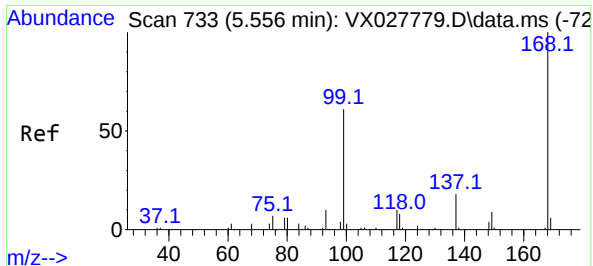


#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX027934.D
Acq: 02 Apr 2022 15:32

Instrument :
MSVOA_X
ClientSampleId :
FIELD-BLANKRE



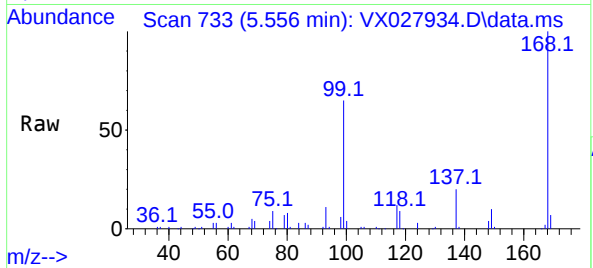



Tgt Ion:168 Resp: 77596
Ion Ratio Lower Upper
168 100
99 65.3 41.7 62.5#

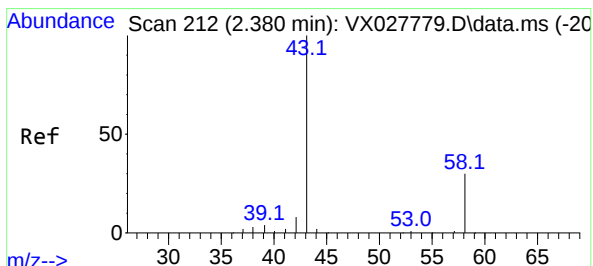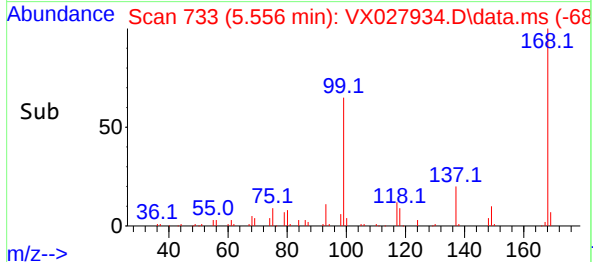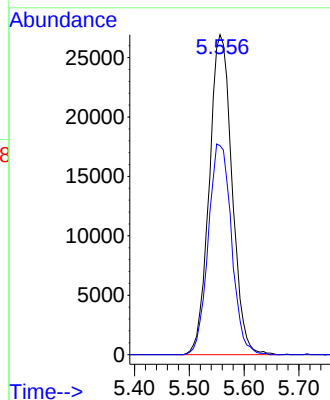

#16
Acetone
Concen: 2.523 ug/l
RT: 2.380 min Scan# 212
Delta R.T. -0.000 min
Lab File: VX027934.D
Acq: 02 Apr 2022 15:32

Tgt Ion: 43 Resp: 1118
Ion Ratio Lower Upper
43 100
58 30.2 28.8 43.2


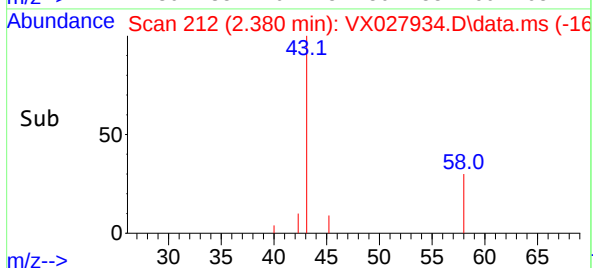
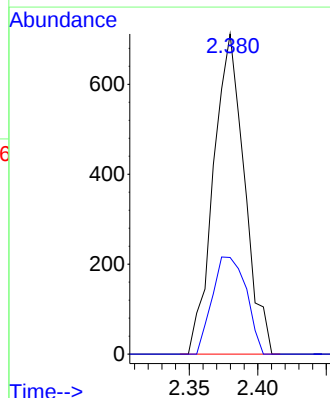
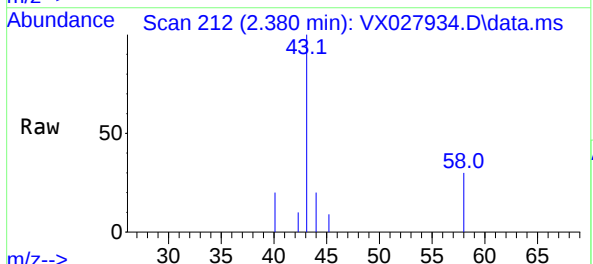


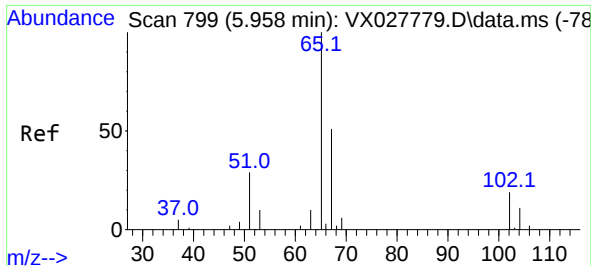

#33
1,2-Dichloroethane-d4
Concen: 61.678 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.000 min
Lab File: VX027934.D
Acq: 02 Apr 2022 15:32




Instrument :
MSVOA_X
ClientSampleId :
FIELD-BLANKRE


Tgt Ion: 65 Resp: 61752
Ion Ratio Lower Upper
65 100
67 49.6 0.0 107.4

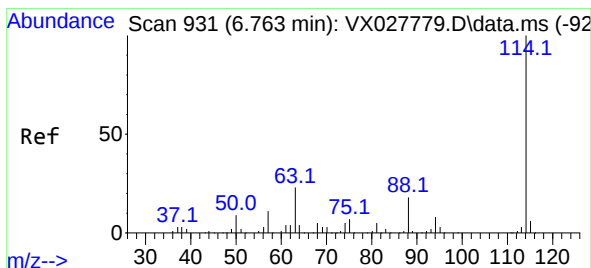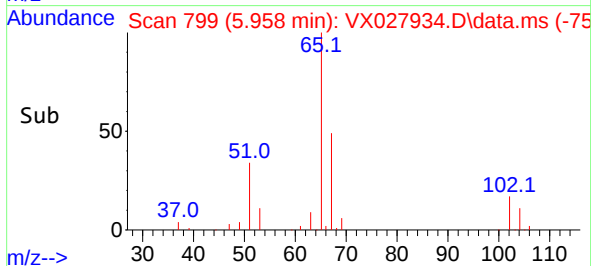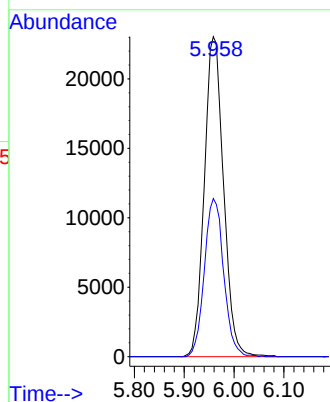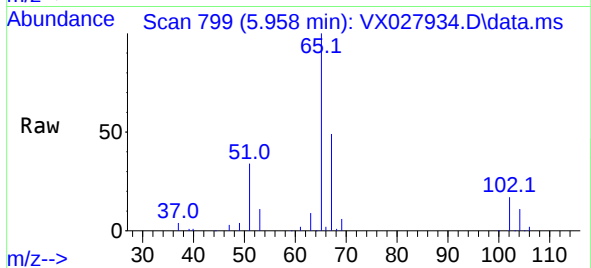

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 931
Delta R.T. 0.000 min
Lab File: VX027934.D
Acq: 02 Apr 2022 15:32

Tgt Ion: 114 Resp: 137554
Ion Ratio Lower Upper
114 100
63 22.5 0.0 36.8
88 16.7 0.0 32.4


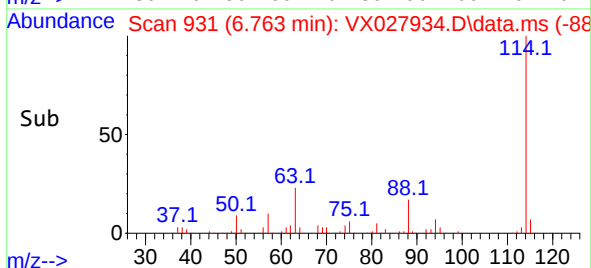
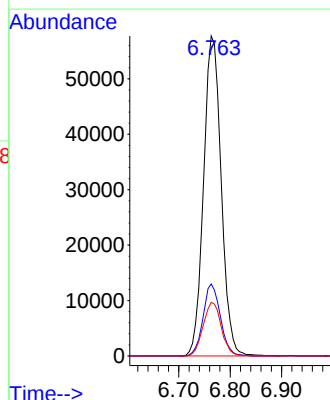
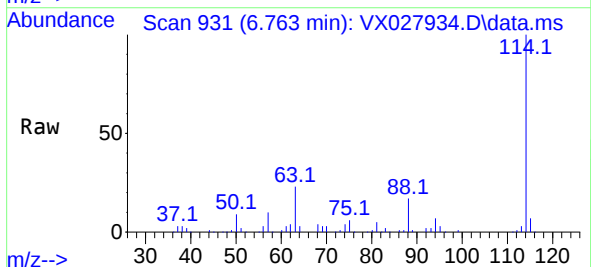


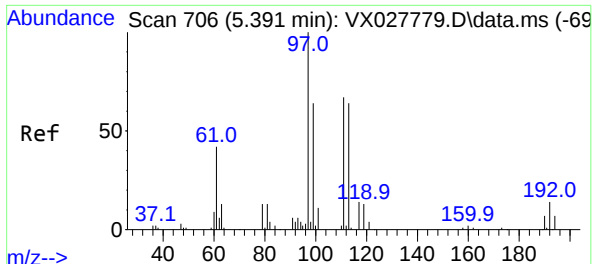

#35
Dibromofluoromethane
Concen: 53.894 ug/l
RT: 5.385 min Scan# 706
Delta R.T. -0.006 min
Lab File: VX027934.D
Acq: 02 Apr 2022 15:32




Instrument :
MSVOA_X
ClientSampleId :
FIELD-BLANKRE


Tgt Ion:113 Resp: 47851
Ion Ratio Lower Upper
113 100
111 101.3 82.8 124.2
192 17.8 16.9 25.3

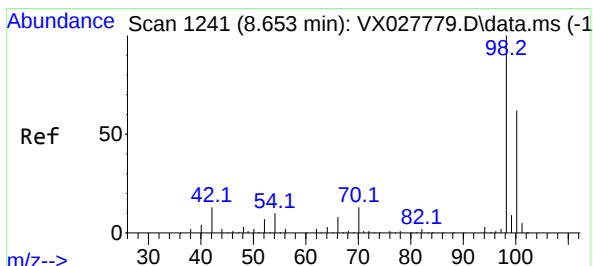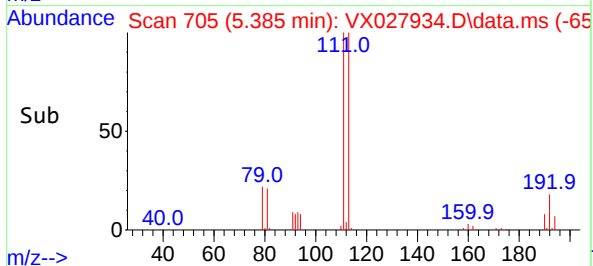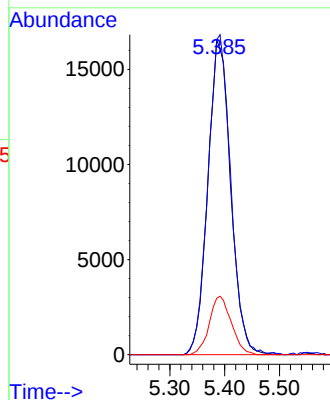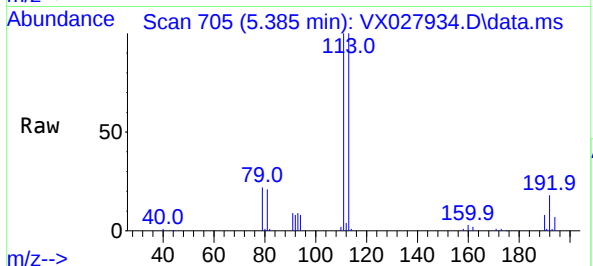

#50
Toluene-d8
Concen: 52.545 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. -0.000 min
Lab File: VX027934.D
Acq: 02 Apr 2022 15:32

Tgt Ion: 98 Resp: 164148
Ion Ratio Lower Upper
98 100
100 65.2 52.6 78.8


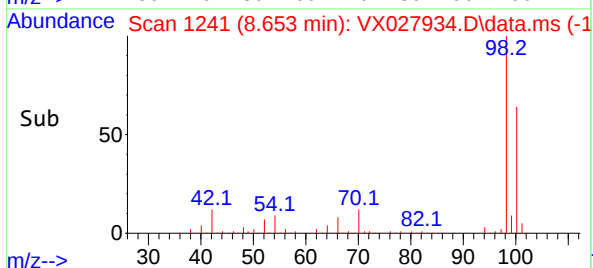
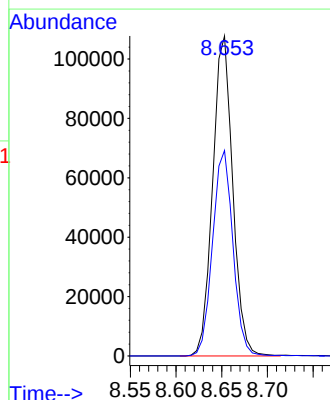
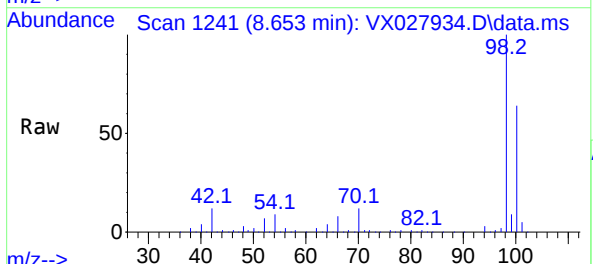


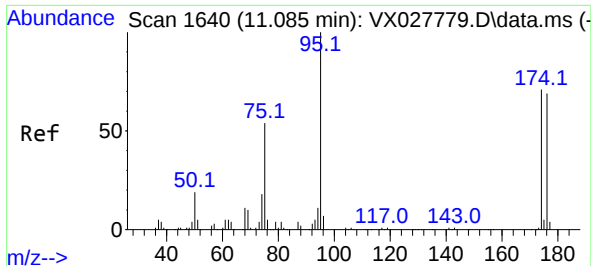

#62
4-Bromofluorobenzene
Concen: 48.231 ug/l
RT: 11.079 min Scan# 1
Delta R.T. -0.006 min
Lab File: VX027934.D
Acq: 02 Apr 2022 15:32




Instrument :
MSVOA_X
ClientSampleId :
FIELD-BLANKRE


Tgt Ion: 95 Resp: 64030
Ion Ratio Lower Upper
95 100
174 68.6 0.0 163.0
176 64.9 0.0 155.0

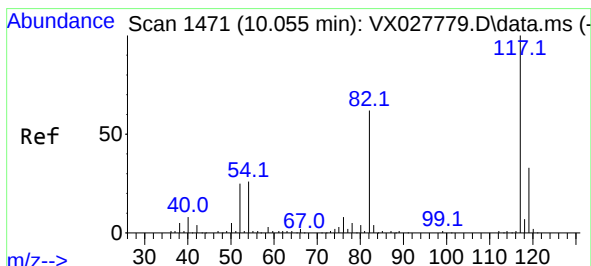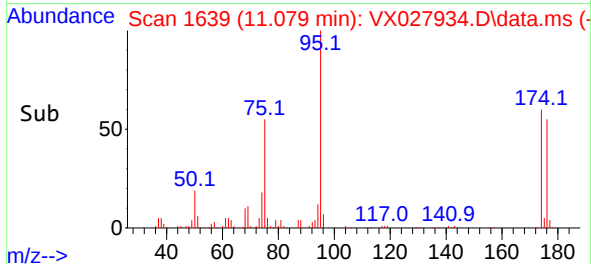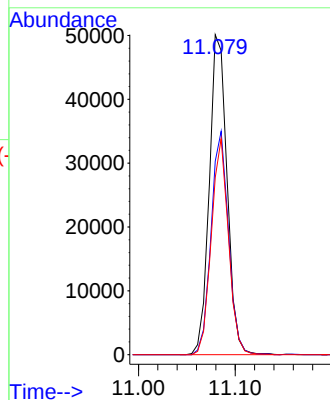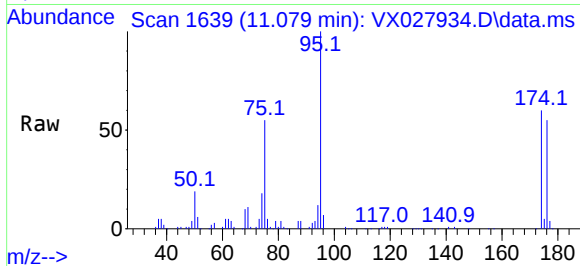

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX027934.D
Acq: 02 Apr 2022 15:32


Tgt Ion: 117 Resp: 125937
Ion Ratio Lower Upper
117 100
82 60.9 41.8 62.8
119 32.4 24.8 37.2

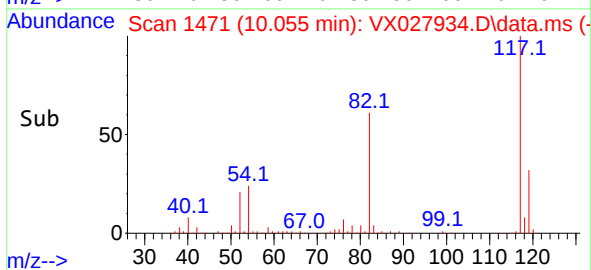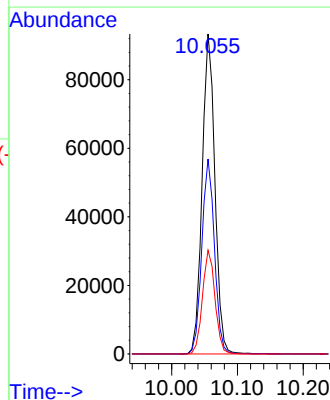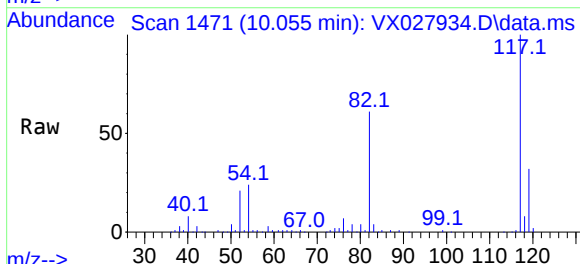

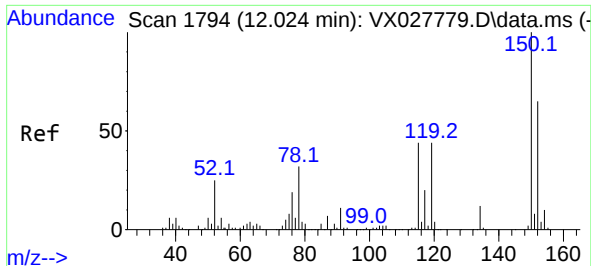

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 12.024 min Scan# 11
 Delta R.T. 0.000 min
 Lab File: VX027934.D
 Acq: 02 Apr 2022 15:32

Instrument :
 MSVOA_X
 ClientSampleId :
 FIELD-BLANKRE

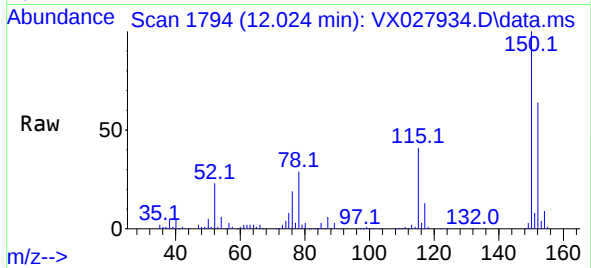

Tgt Ion:152 Resp: 55016
 Ion Ratio Lower Upper
 152 100
 115 63.8 37.5 112.7
 150 154.8 0.0 338.2

