
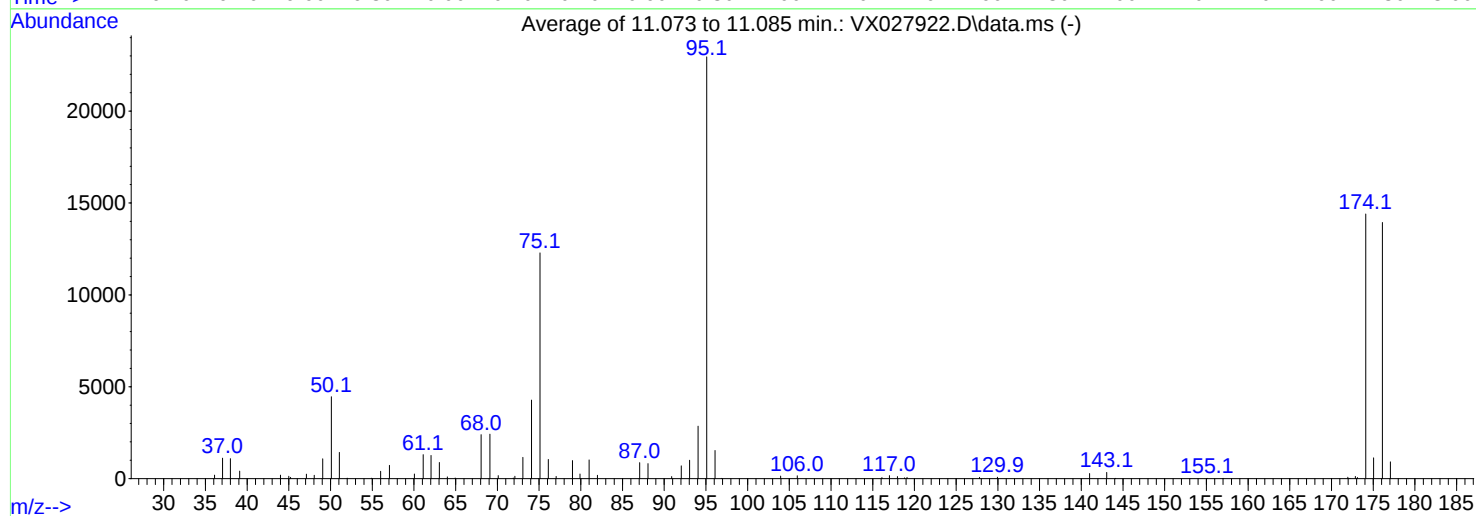


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX040222\
 Data File : VX027922.D
 Acq On : 02 Apr 2022 09:59
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032922W.M
 Title : SW846 8260
 Last Update : Tue Apr 05 14:48:33 2022

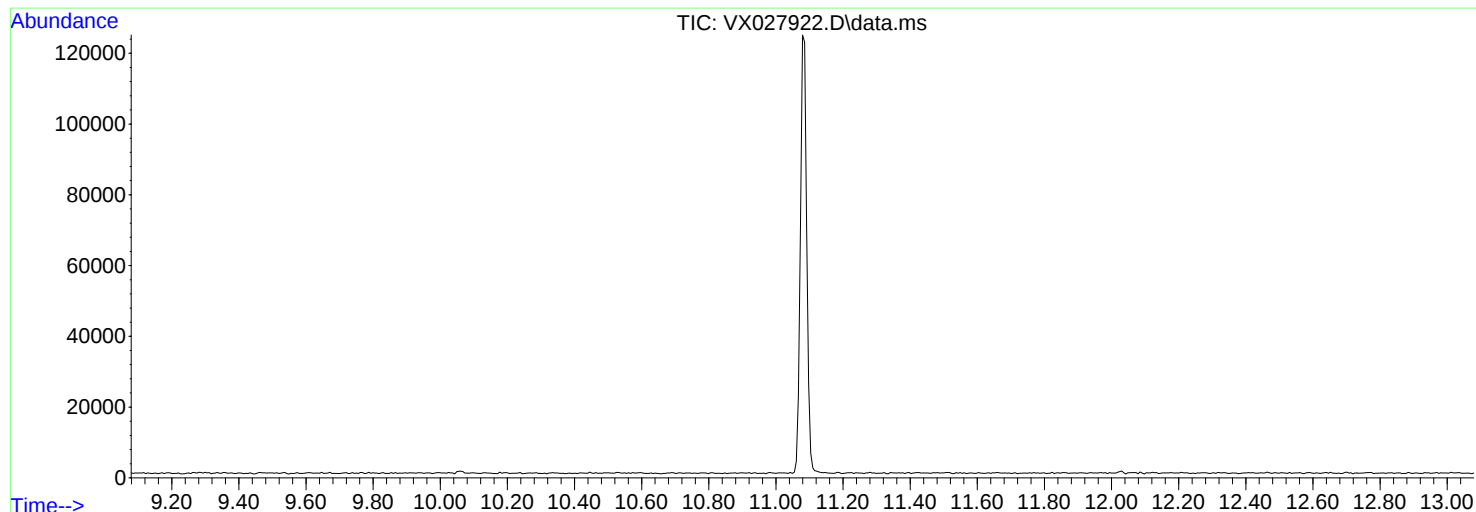

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.4	4455	PASS
75	95	30	60	53.5	12285	PASS
95	95	100	100	100.0	22953	PASS
96	95	5	9	6.7	1534	PASS
173	174	0.00	2	0.9	124	PASS
174	95	50	100	62.8	14404	PASS
175	174	5	9	7.9	1135	PASS
176	174	95	101	96.8	13937	PASS
177	176	5	9	6.6	915	PASS