

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX040224\
 Data File : VX040853.D
 Acq On : 02 Apr 2024 10:20
 Operator : JC/MD
 Sample : VX0402WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0402WBL01

Quant Time: Apr 03 00:58:15 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X040124W.M
 Quant Title : SW846 8260
 QLast Update : Tue Apr 02 05:40:55 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	43371	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	77992	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	77087	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	40986	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	37901	48.704	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	97.400%
35) Dibromofluoromethane	5.385	113	27095	49.048	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	98.100%
50) Toluene-d8	8.647	98	98515	49.353	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	98.700%
62) 4-Bromofluorobenzene	11.079	95	40827	51.216	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	102.440%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX040224\
Data File : VX040853.D
Acq On : 02 Apr 2024 10:20
Operator : JC/MD
Sample : VX0402WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0402WBL01

Quant Time: Apr 03 00:58:15 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X040124W.M
Quant Title : SW846 8260
QLast Update : Tue Apr 02 05:40:55 2024
Response via : Initial Calibration




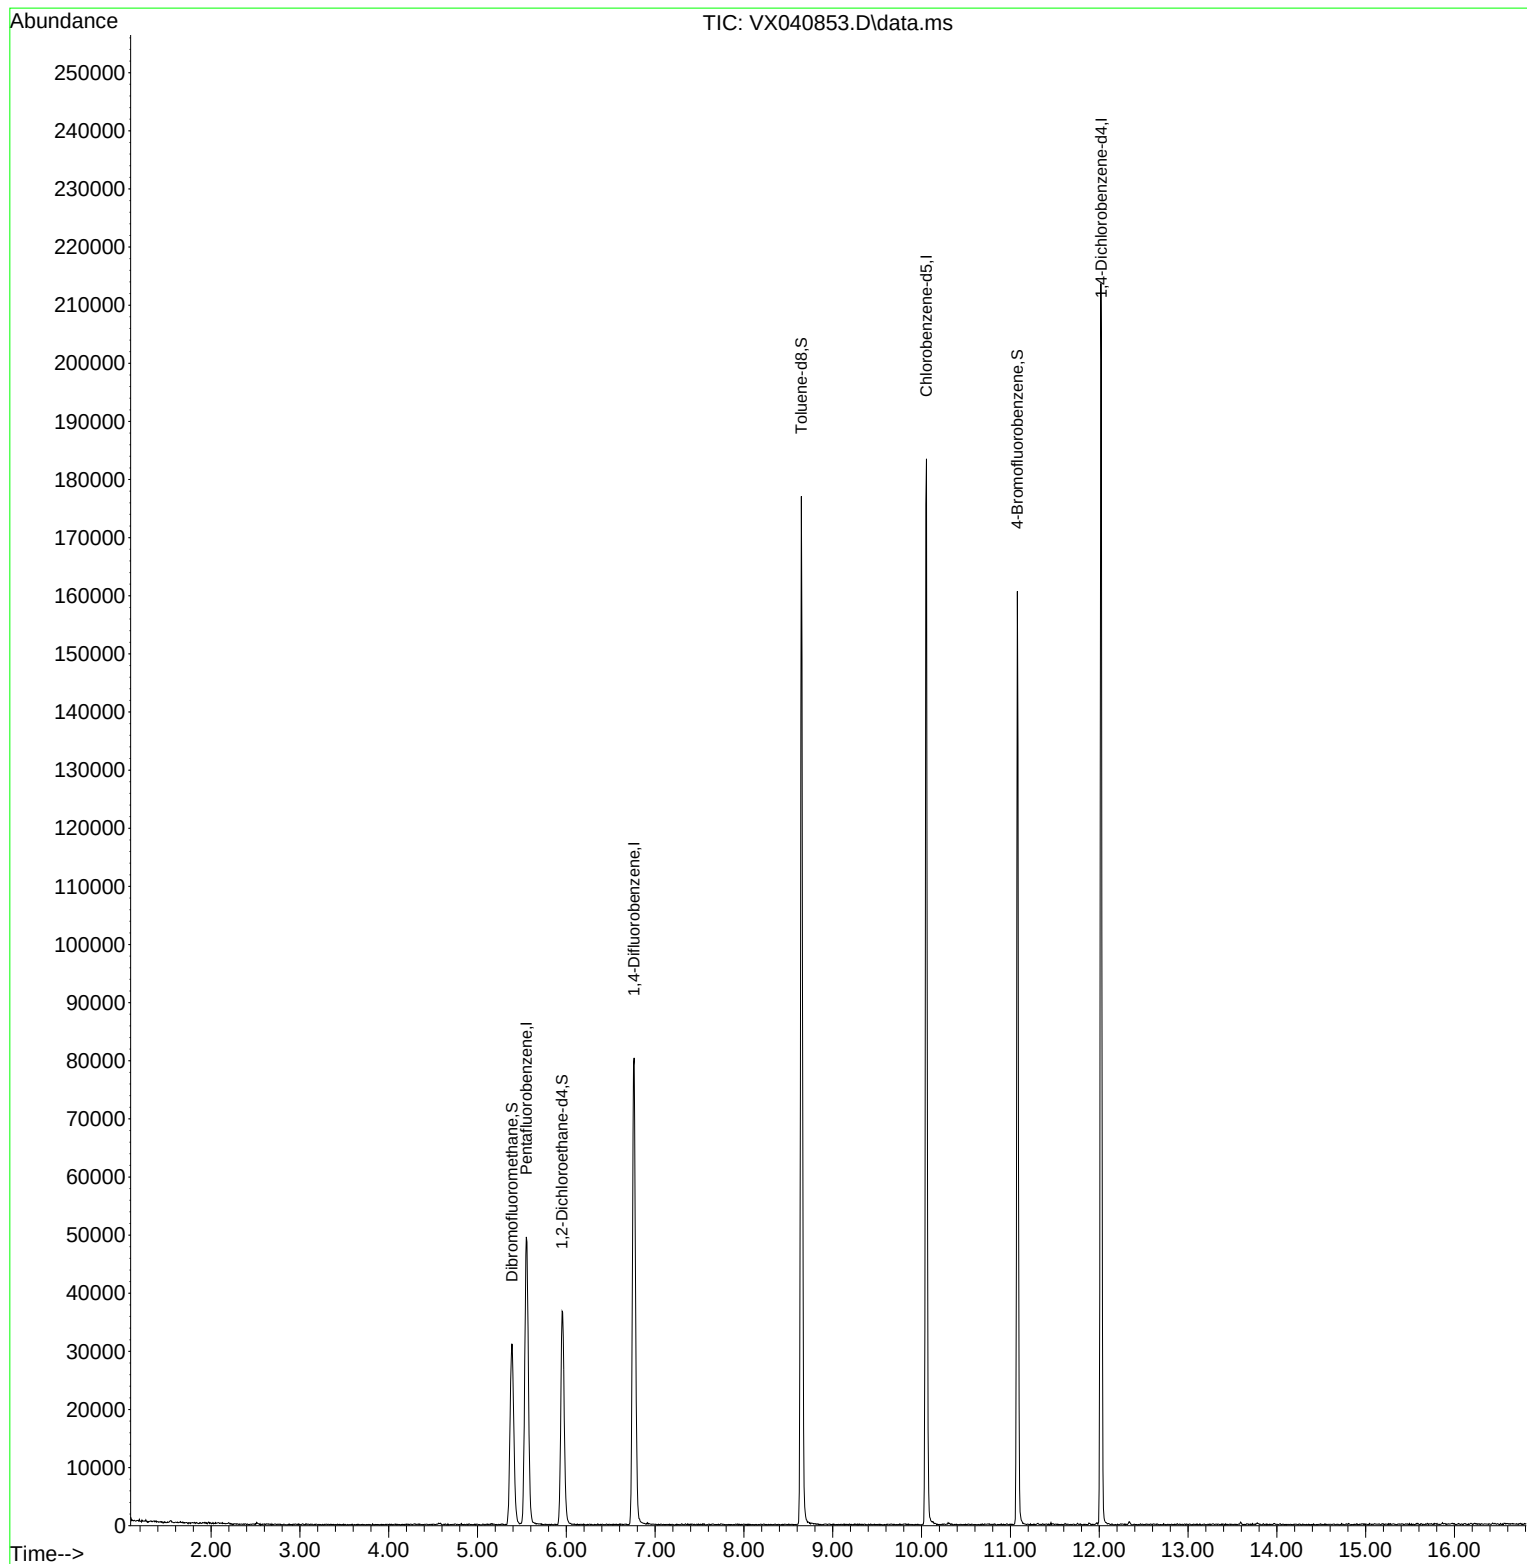


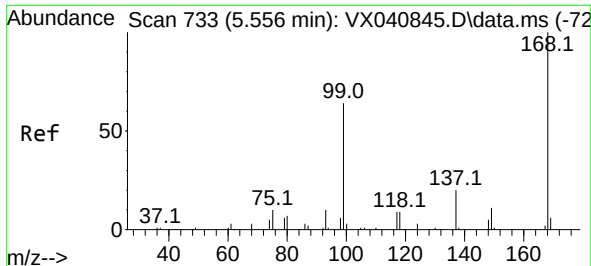

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 712
Delta R.T. -0.006 min
Lab File: VX040853.D
Acq: 02 Apr 2024 10:20




Instrument :
MSVOA_X
ClientSampleId :
VX0402WBL01


Tgt Ion:168 Resp: 43371
Ion Ratio Lower Upper
168 100
99 66.5 56.6 85.0

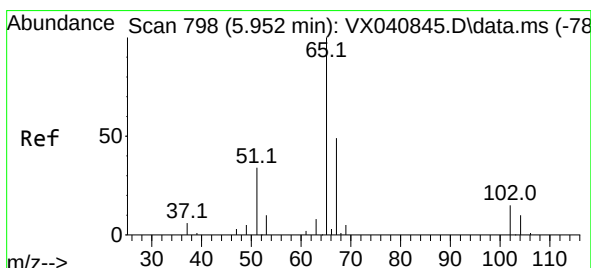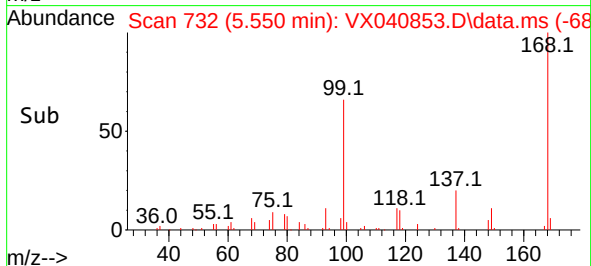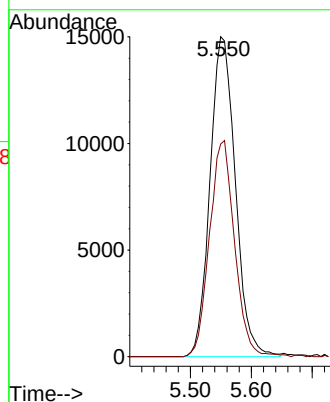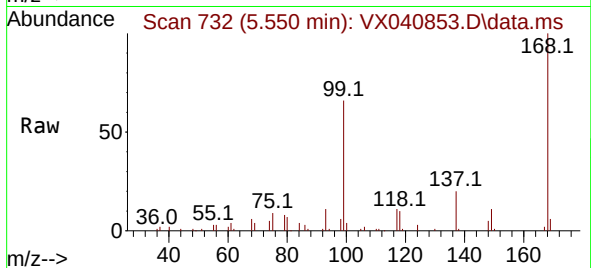

#33
1,2-Dichloroethane-d4
Concen: 48.704 ug/l
RT: 5.952 min Scan# 798
Delta R.T. 0.000 min
Lab File: VX040853.D
Acq: 02 Apr 2024 10:20

Tgt Ion: 65 Resp: 37901
Ion Ratio Lower Upper
65 100
67 48.4 0.0 100.2


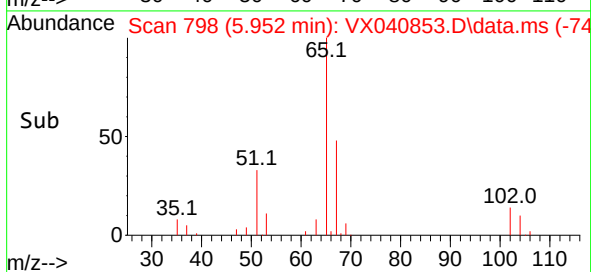
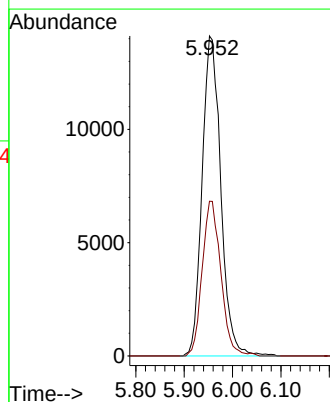
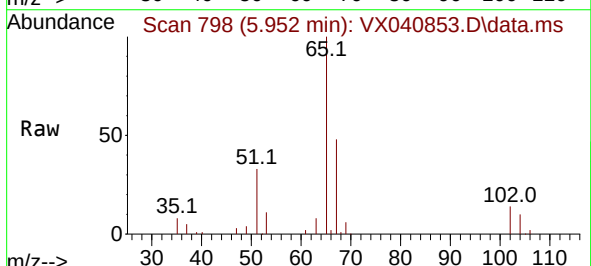


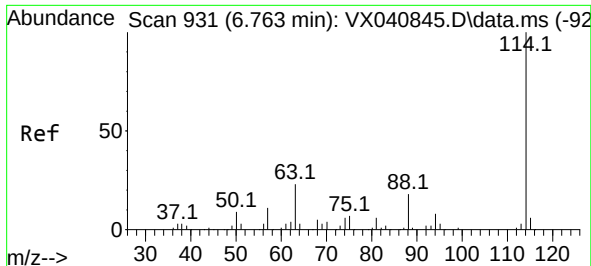

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 911
Delta R.T. 0.000 min
Lab File: VX040853.D
Acq: 02 Apr 2024 10:20




Instrument :
MSVOA_X
ClientSampleId :
VX0402WBL01


Tgt Ion:114 Resp: 77992
Ion Ratio Lower Upper
114 100
63 22.7 0.0 45.0
88 15.6 0.0 36.6

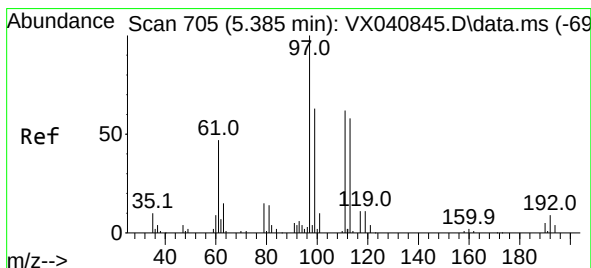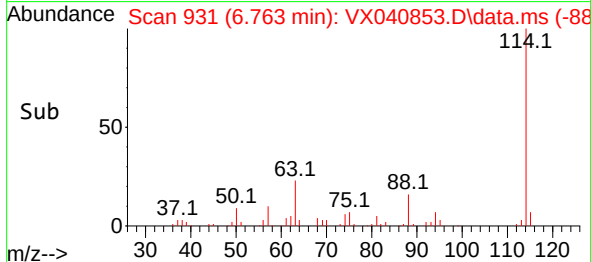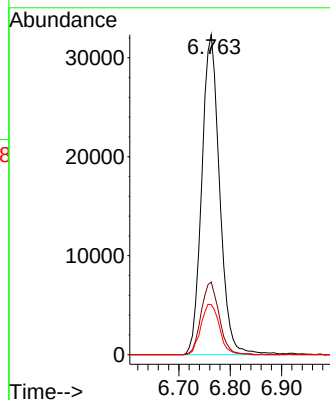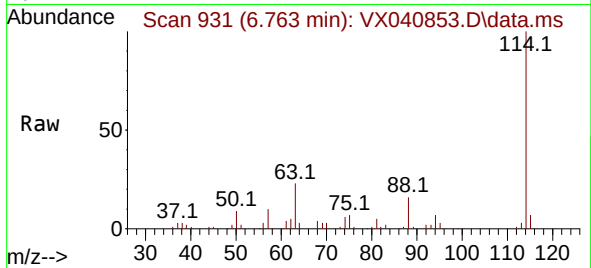

#35
Dibromofluoromethane
Concen: 49.048 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.000 min
Lab File: VX040853.D
Acq: 02 Apr 2024 10:20

Tgt Ion:113 Resp: 27095
Ion Ratio Lower Upper
113 100
111 103.3 82.9 124.3
192 16.6 13.3 19.9


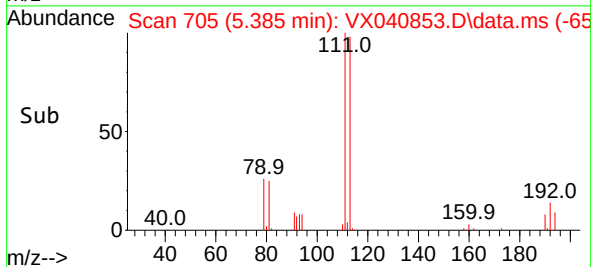
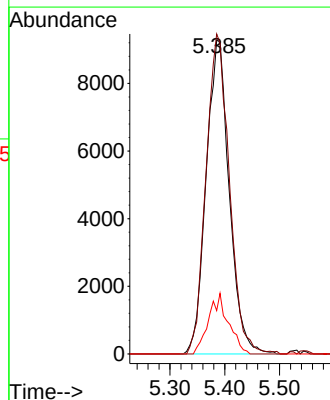
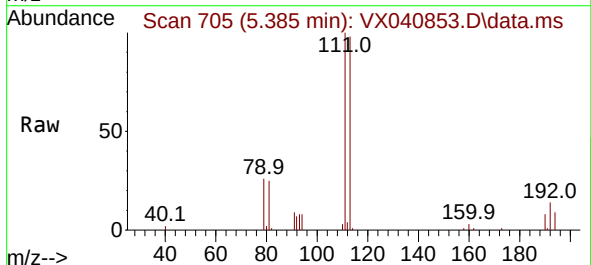


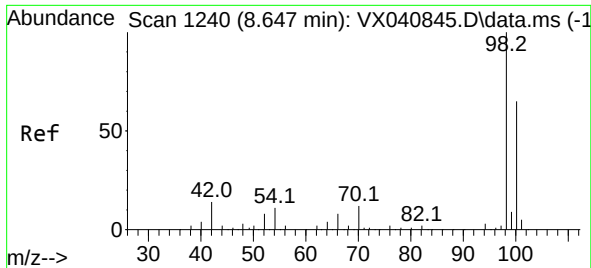

#50
Toluene-d8
Concen: 49.353 ug/l
RT: 8.647 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX040853.D
Acq: 02 Apr 2024 10:20




Instrument :
MSVOA_X
ClientSampleId :
VX0402WBL01


Tgt Ion: 98 Resp: 98515
Ion Ratio Lower Upper
98 100
100 63.6 53.1 79.7

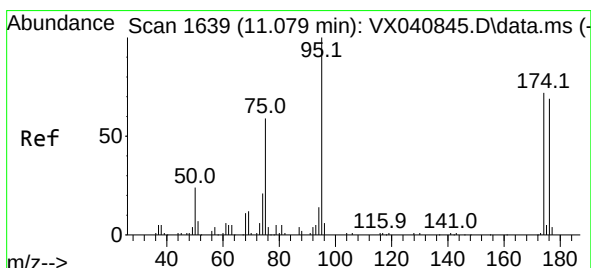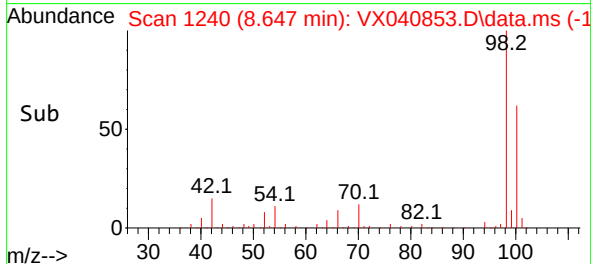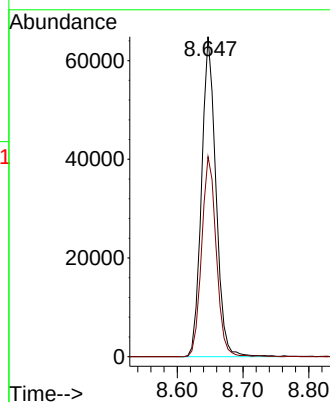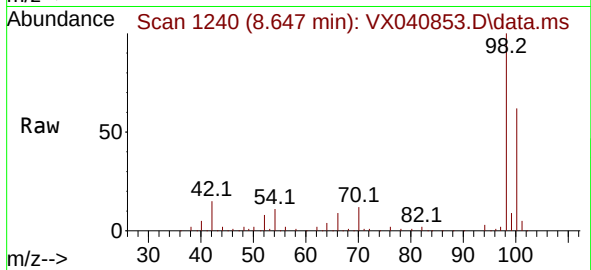

#62
4-Bromofluorobenzene
Concen: 51.216 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX040853.D
Acq: 02 Apr 2024 10:20

Tgt Ion: 95 Resp: 40827
Ion Ratio Lower Upper
95 100
174 70.9 0.0 135.6
176 70.2 0.0 131.0


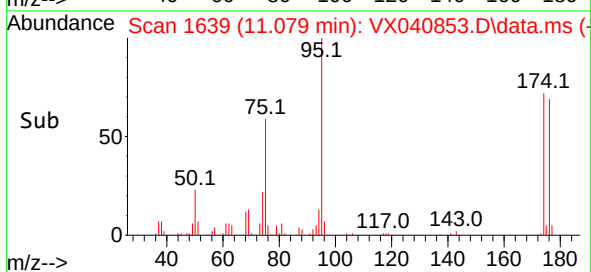
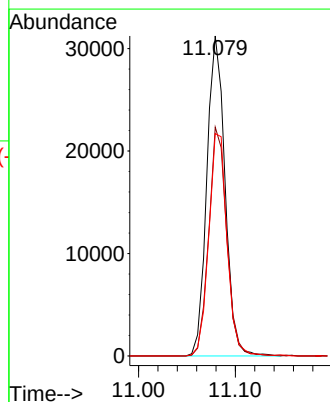
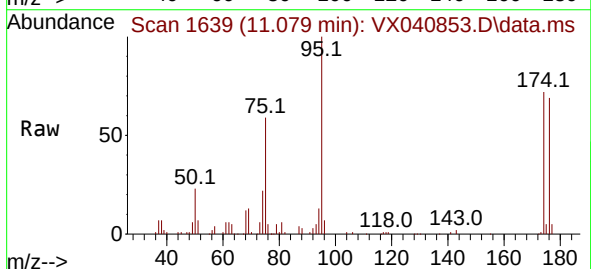


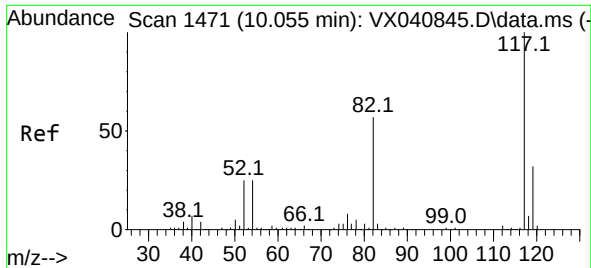

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX040853.D
Acq: 02 Apr 2024 10:20

Instrument :
MSVOA_X
ClientSampleId :
VX0402WBL01

Tgt Ion:	117	Resp:	77087
Ion	Ratio	Lower	Upper
117	100		
82	59.2	46.2	69.4
119	32.6	25.5	38.3

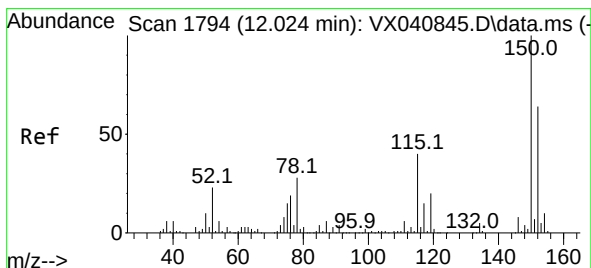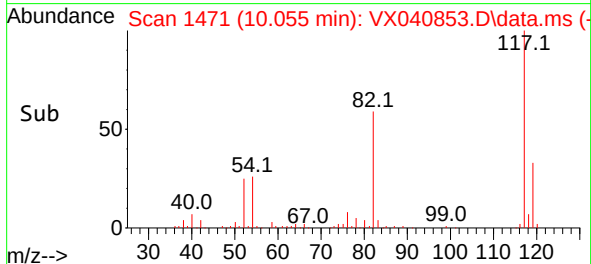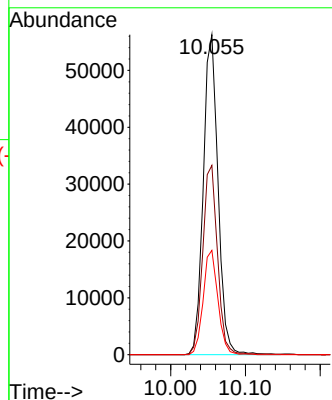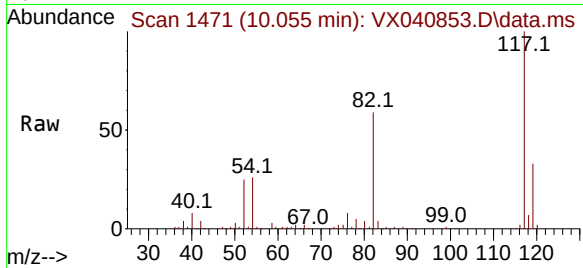

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX040853.D
Acq: 02 Apr 2024 10:20

Tgt Ion:	152	Resp:	40986
Ion	Ratio	Lower	Upper
152	100		
115	61.8	43.3	129.9
150	153.7	0.0	345.0

