

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX040225\
 Data File : VX045535.D
 Acq On : 02 Apr 2025 10:30
 Operator : JC/MD
 Sample : VX0402MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0402MBL01

Quant Time: Apr 03 01:46:04 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X040225W.M
 Quant Title : SW846 8260
 QLast Update : Wed Apr 02 03:11:43 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.543	168	66955	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	129348	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	122427	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	52544	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.946	65	63952	52.230	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	= 104.460%	
35) Dibromofluoromethane	5.379	113	47325	51.568	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 103.140%	
50) Toluene-d8	8.646	98	162002	50.575	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	= 101.140%	
62) 4-Bromofluorobenzene	11.079	95	60256	51.643	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	= 103.280%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX040225\
Data File : VX045535.D
Acq On : 02 Apr 2025 10:30
Operator : JC/MD
Sample : VX0402MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0402MBL01

Quant Time: Apr 03 01:46:04 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X040225W.M
Quant Title : SW846 8260
QLast Update : Wed Apr 02 03:11:43 2025
Response via : Initial Calibration




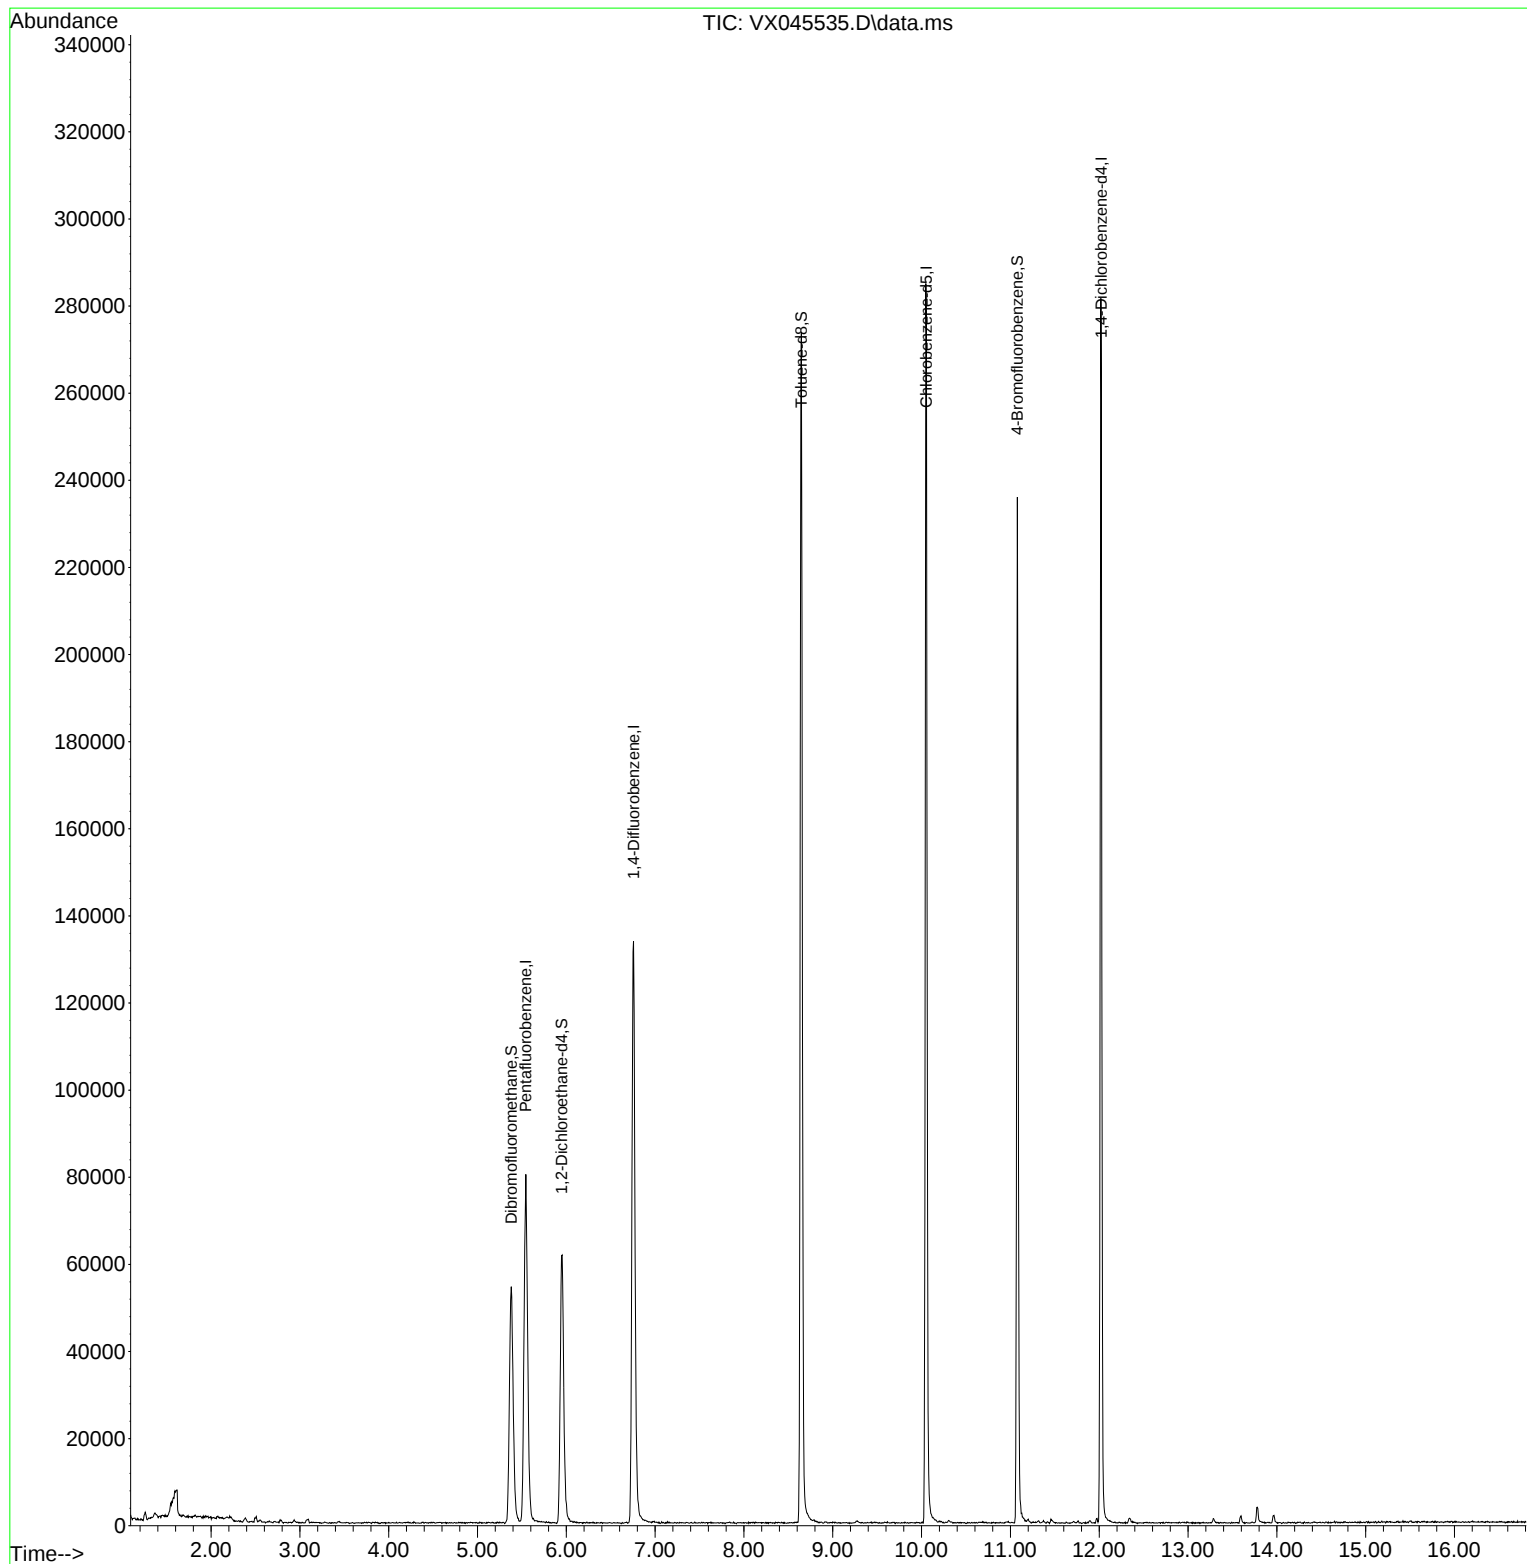


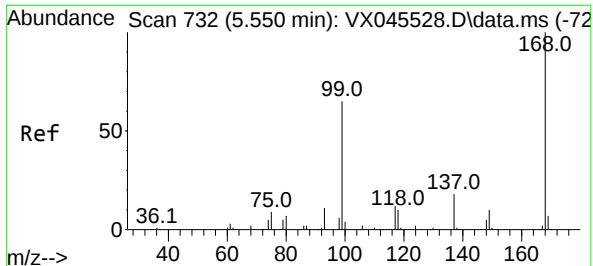

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.543 min Scan# 71
Delta R.T. -0.007 min
Lab File: VX045535.D
Acq: 02 Apr 2025 10:30




Instrument :
MSVOA_X
ClientSampleId :
VX0402MBL01


Tgt Ion:168 Resp: 66955
Ion Ratio Lower Upper
168 100
99 69.9 52.3 78.5

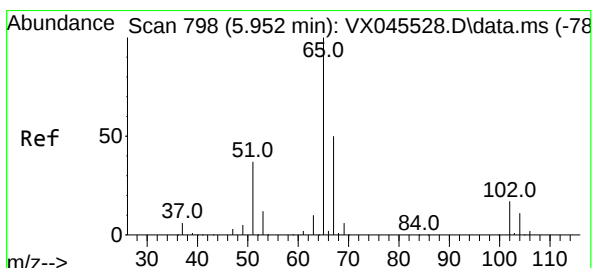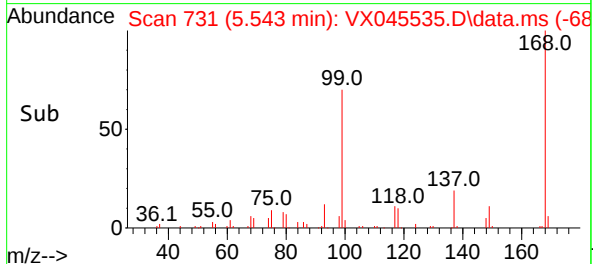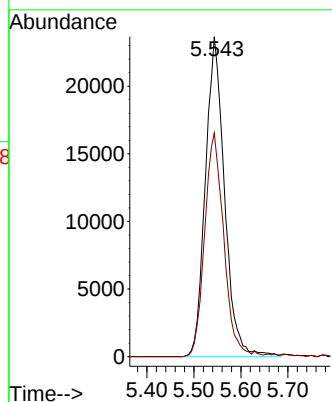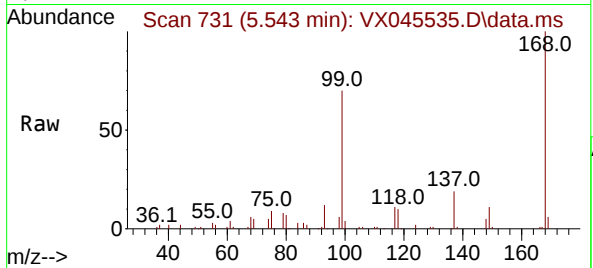

#33
1,2-Dichloroethane-d4
Concen: 52.230 ug/l
RT: 5.946 min Scan# 797
Delta R.T. -0.006 min
Lab File: VX045535.D
Acq: 02 Apr 2025 10:30

Tgt Ion: 65 Resp: 63952
Ion Ratio Lower Upper
65 100
67 49.0 0.0 99.0

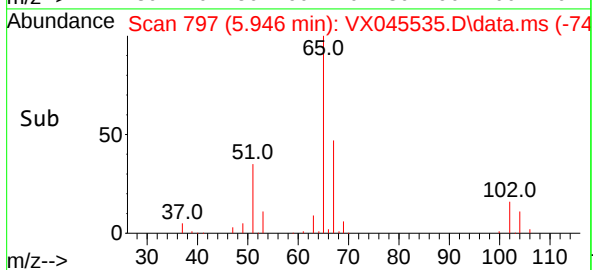
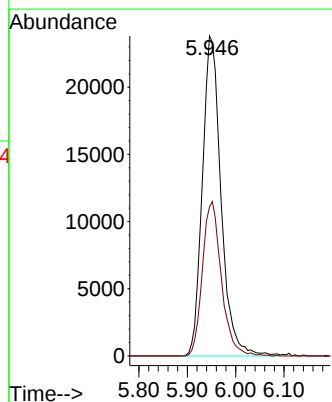
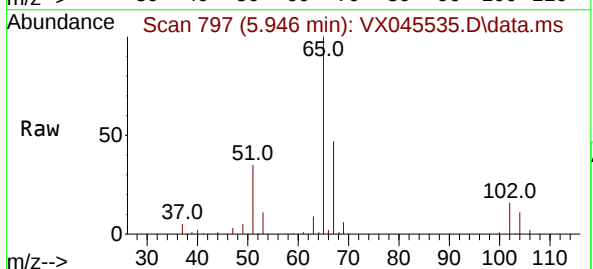


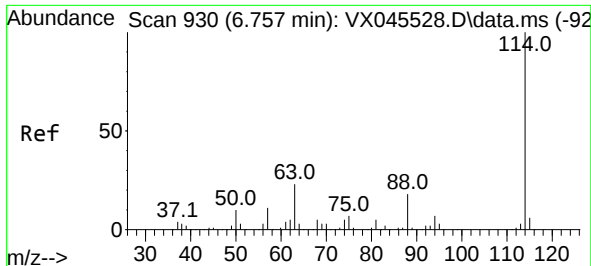

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.757 min Scan# 91
Delta R.T. -0.000 min
Lab File: VX045535.D
Acq: 02 Apr 2025 10:30




Instrument :
MSVOA_X
ClientSampleId :
VX0402MBL01


Tgt Ion:114 Resp: 129348
Ion Ratio Lower Upper
114 100
63 23.8 0.0 46.8
88 16.8 0.0 35.4

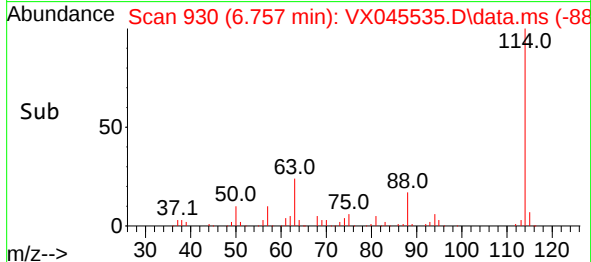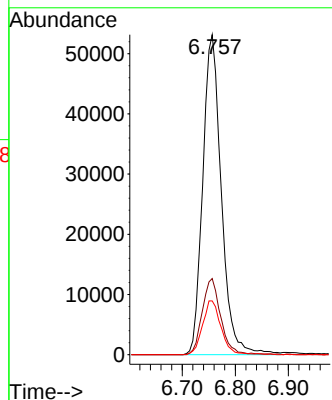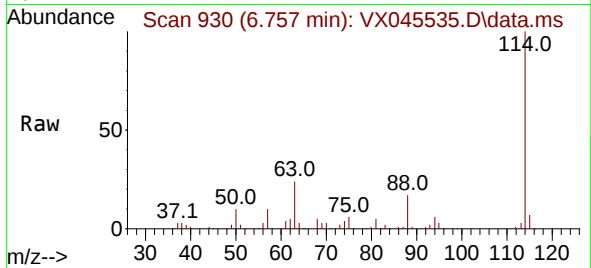

#35
Dibromofluoromethane
Concen: 51.568 ug/l
RT: 5.379 min Scan# 704
Delta R.T. -0.000 min
Lab File: VX045535.D
Acq: 02 Apr 2025 10:30

Tgt Ion:113 Resp: 47325
Ion Ratio Lower Upper
113 100
111 103.6 81.8 122.6
192 16.5 13.8 20.6


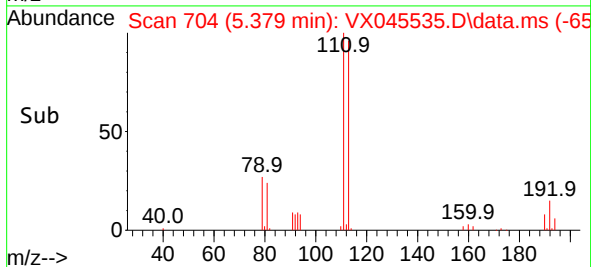
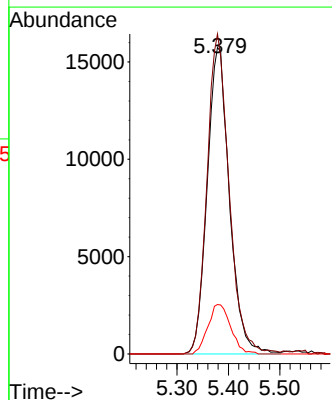
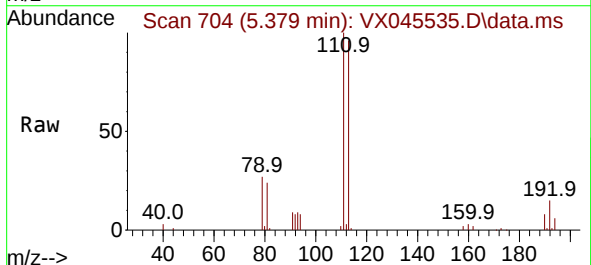


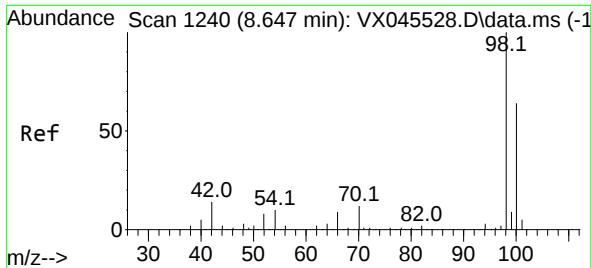

#50
Toluene-d8
Concen: 50.575 ug/l
RT: 8.646 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX045535.D
Acq: 02 Apr 2025 10:30




Instrument :
MSVOA_X
ClientSampleId :
VX0402MBL01


Tgt Ion: 98 Resp: 162002
Ion Ratio Lower Upper
98 100
100 64.1 52.2 78.4

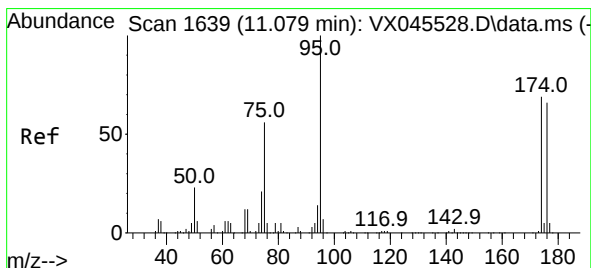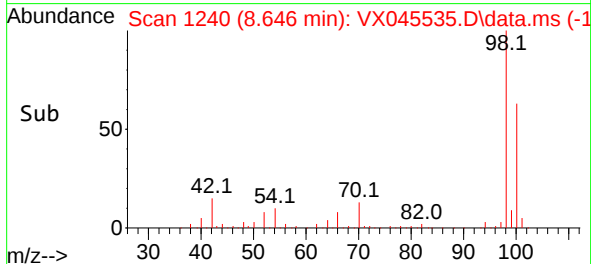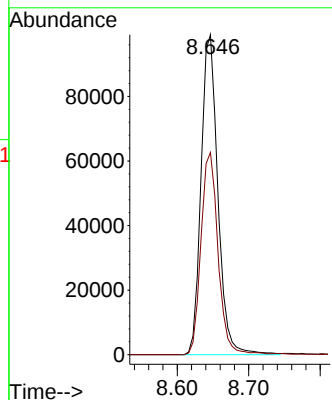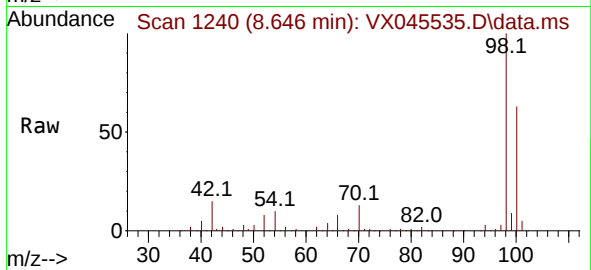

#62
4-Bromofluorobenzene
Concen: 51.643 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.000 min
Lab File: VX045535.D
Acq: 02 Apr 2025 10:30

Tgt Ion: 95 Resp: 60256
Ion Ratio Lower Upper
95 100
174 68.8 0.0 135.8
176 66.7 0.0 131.4

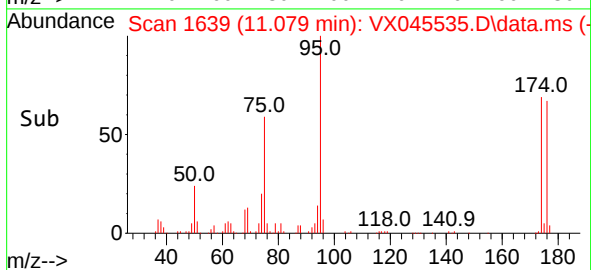
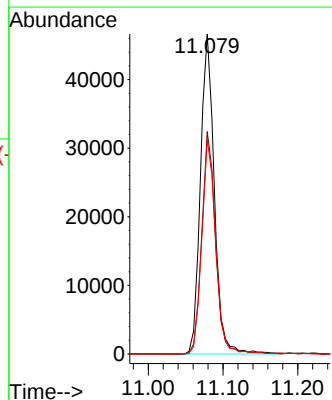
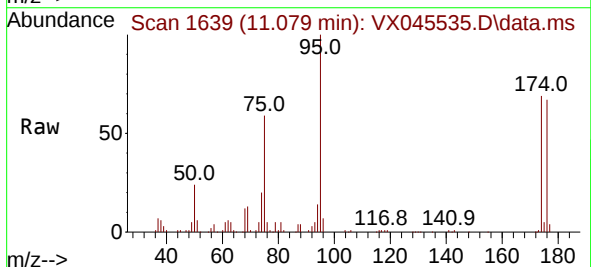


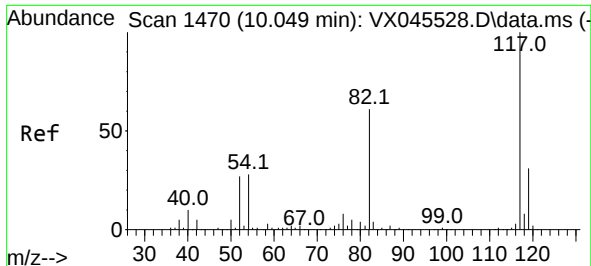

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1470
Delta R.T. 0.006 min
Lab File: VX045535.D
Acq: 02 Apr 2025 10:30

Instrument :
MSVOA_X
ClientSampleId :
VX0402MBL01

Tgt Ion:117 Resp: 122427
Ion Ratio Lower Upper
117 100
82 56.4 49.2 73.8
119 31.1 25.1 37.7

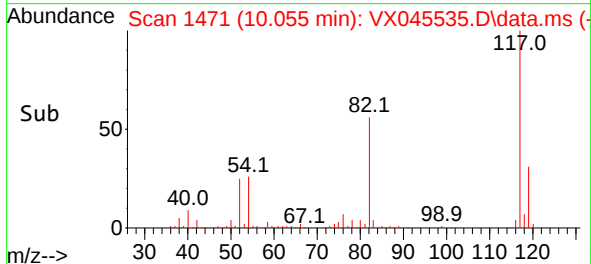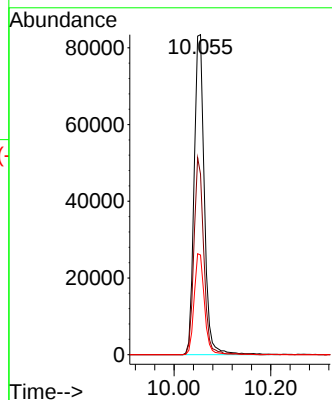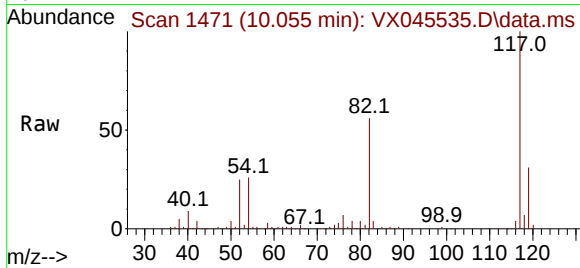

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.006 min
Lab File: VX045535.D
Acq: 02 Apr 2025 10:30

Tgt Ion:152 Resp: 52544
Ion Ratio Lower Upper
152 100
115 64.5 46.9 140.7
150 157.5 0.0 349.4

