

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX040225\
 Data File : VX045531.D
 Acq On : 01 Apr 2025 19:25
 Operator : JC/MD
 Sample : IBLK
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 IBLK

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X040225W.M
 Title : SW846 8260

Signal : TIC: VX045531.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.568	69	79	80	rBV4	4667	10751	2.78%	0.507%
2	1.593	82	83	87	rVB3	6017	4032	1.04%	0.190%
3	2.324	197	203	208	rVB6	1963	4359	1.13%	0.206%
4	2.507	227	233	241	rVB	3999	7095	1.83%	0.335%
5	3.086	319	328	336	rBV6	2774	6704	1.73%	0.316%
6	5.379	694	704	722	rBV	45582	138290	35.71%	6.520%
7	5.543	722	731	747	rVB	67050	193971	50.08%	9.145%
8	5.952	789	798	812	rBV	53493	144224	37.24%	6.800%
9	6.756	922	930	945	rBV	116495	279750	72.23%	13.190%
10	8.646	1234	1240	1250	rBV	237244	387305	100.00%	18.261%
11	10.049	1465	1470	1482	rBV	240489	347730	89.78%	16.395%
12	10.305	1507	1512	1520	rBV3	3486	5664	1.46%	0.267%
13	11.079	1634	1639	1653	rBV	192882	250921	64.79%	11.830%
14	11.457	1697	1701	1708	rVB2	4246	6412	1.66%	0.302%
15	11.969	1782	1785	1788	rBV2	3715	4780	1.23%	0.225%
16	12.018	1788	1793	1807	rVB	222302	284226	73.39%	13.401%
17	12.335	1840	1845	1854	rBV2	5798	8994	2.32%	0.424%
18	13.280	1996	2000	2006	rBV2	3176	4417	1.14%	0.208%
19	13.591	2043	2051	2057	rBV4	5616	7772	2.01%	0.366%
20	13.780	2077	2082	2090	rBV	10711	15565	4.02%	0.734%
21	13.962	2107	2112	2117	rBV2	6057	8007	2.07%	0.378%




Sum of corrected areas: 2120969

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX040225\
Data File : VX045531.D
Acq On : 01 Apr 2025 19:25
Operator : JC/MD
Sample : IBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X040225W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

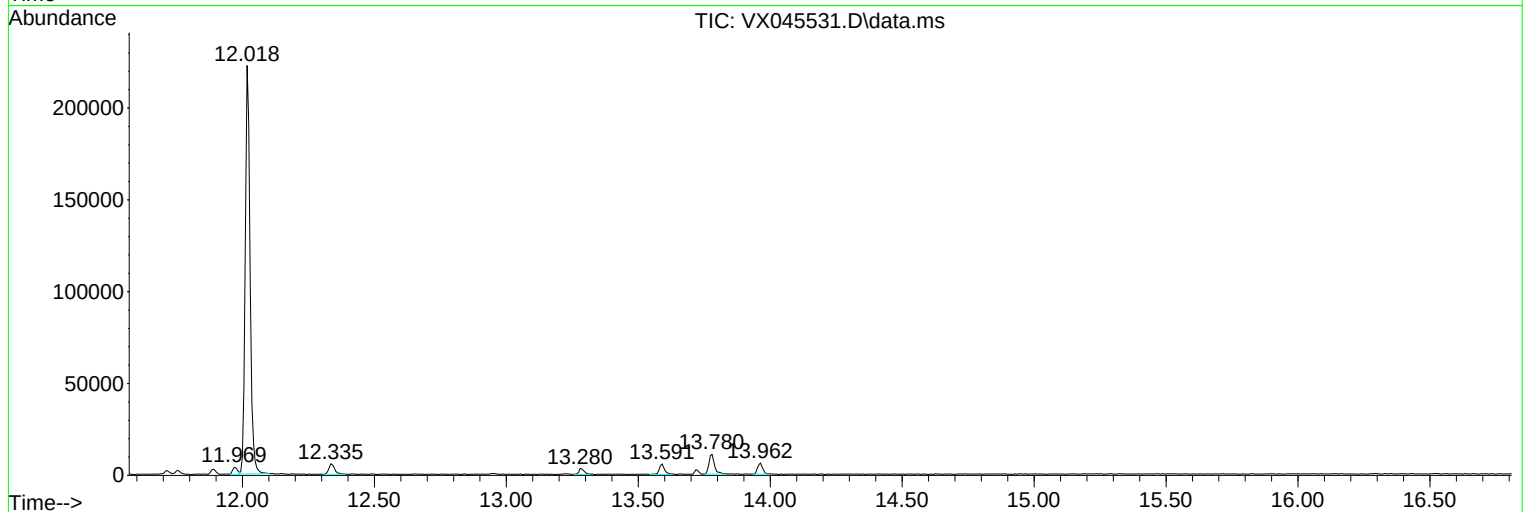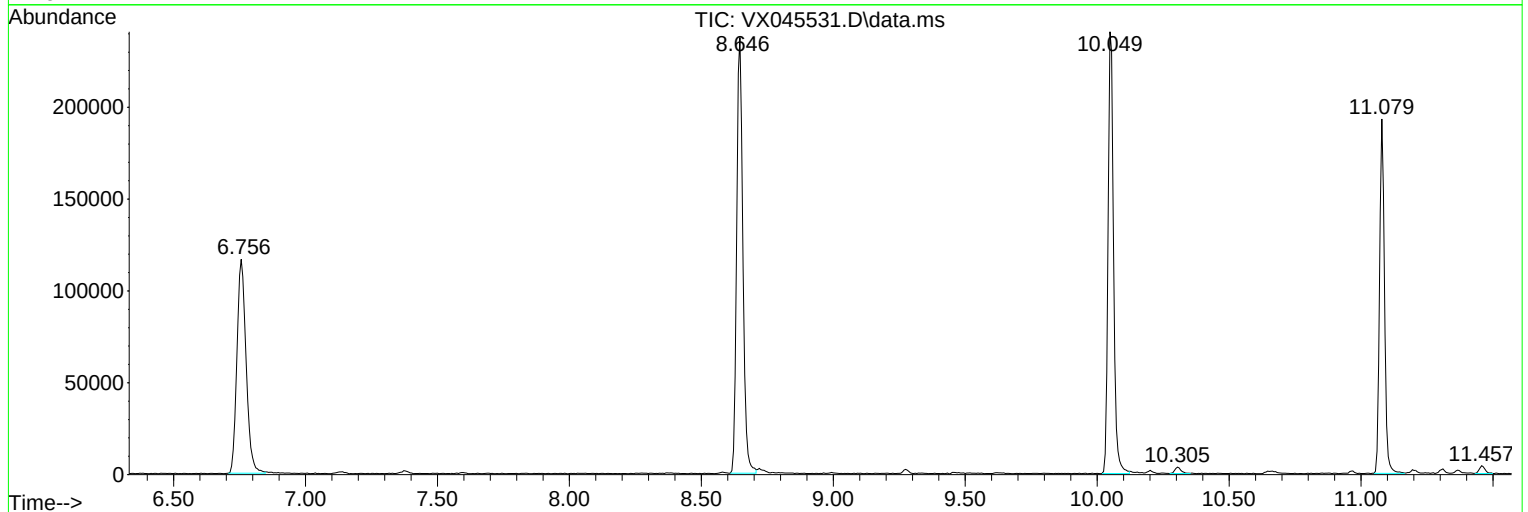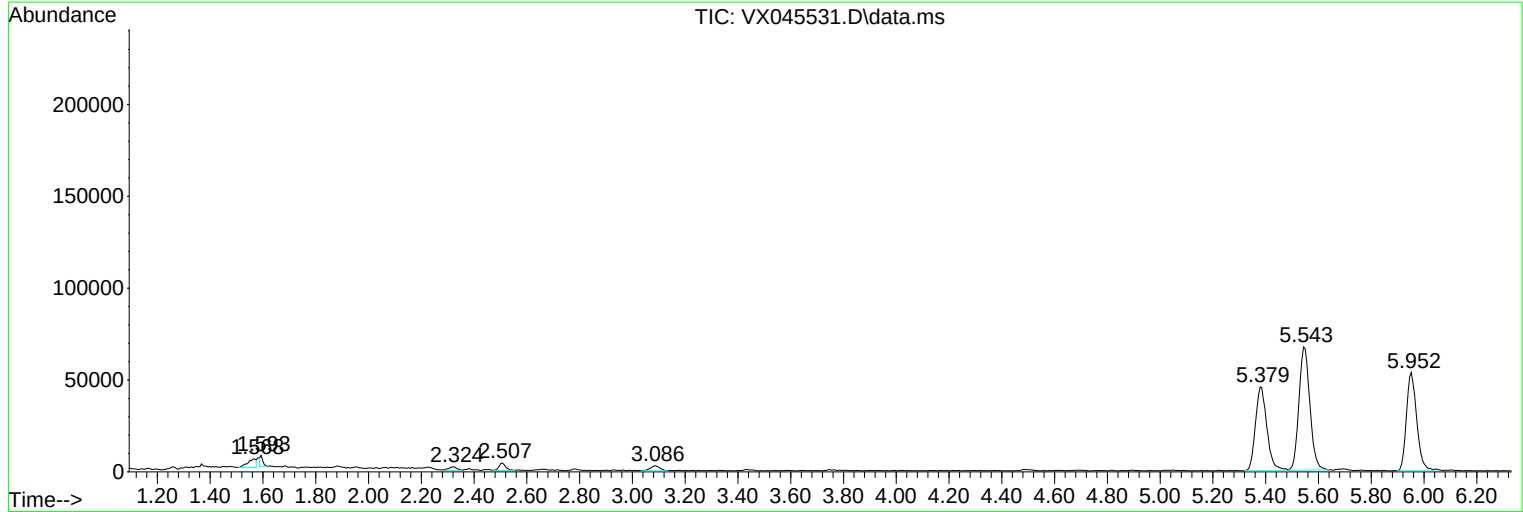

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX040225\
Data File : VX045531.D
Acq On : 01 Apr 2025 19:25
Operator : JC/MD
Sample : IBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X040225W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX040225\
Data File : VX045531.D
Acq On : 01 Apr 2025 19:25
Operator : JC/MD
Sample : IBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X040225W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc