

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX040225\
 Data File : VX045540.D
 Acq On : 02 Apr 2025 12:30
 Operator : JC/MD
 Sample : Q1697-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 IW-01-55-040125

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X040225W.M
 Title : SW846 8260

Signal : TIC: VX045540.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	6	9	19	rVB	131770	130042	7.71%	2.782%
2	2.130	166	171	181	rVB	25724	42376	2.51%	0.906%
3	2.319	193	202	210	rBV2	126972	251609	14.92%	5.382%
4	3.605	404	413	423	rVB2	9771	22149	1.31%	0.474%
5	4.483	544	557	574	rBV	140420	387531	22.98%	8.290%
6	5.013	636	644	664	rBV3	10626	38748	2.30%	0.829%
7	5.385	694	705	720	rBV2	47841	142849	8.47%	3.056%
8	5.544	720	731	747	rVV	67570	198983	11.80%	4.257%
9	5.952	787	798	809	rBV2	57610	151874	9.01%	3.249%
10	6.757	921	930	945	rBV2	120158	292850	17.36%	6.264%
11	7.123	981	990	1006	rBV	757773	1686535	100.00%	36.077%
12	8.647	1234	1240	1251	rBV	258089	405359	24.04%	8.671%
13	9.275	1337	1343	1350	rBV2	12421	20014	1.19%	0.428%
14	10.055	1465	1471	1491	rBV	251786	358167	21.24%	7.662%
15	11.079	1634	1639	1656	rBV	200464	254479	15.09%	5.444%
16	12.018	1788	1793	1803	rBV	225460	291215	17.27%	6.229%




Sum of corrected areas: 4674780

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX040225\
Data File : VX045540.D
Acq On : 02 Apr 2025 12:30
Operator : JC/MD
Sample : Q1697-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IW-01-55-040125

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X040225W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

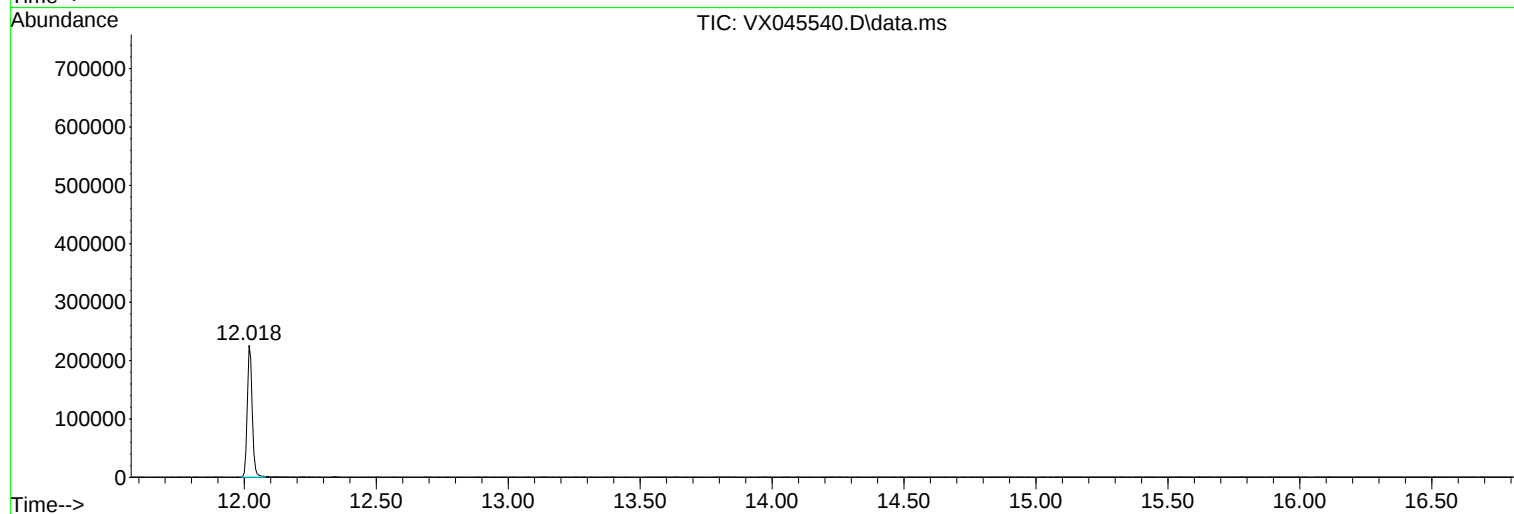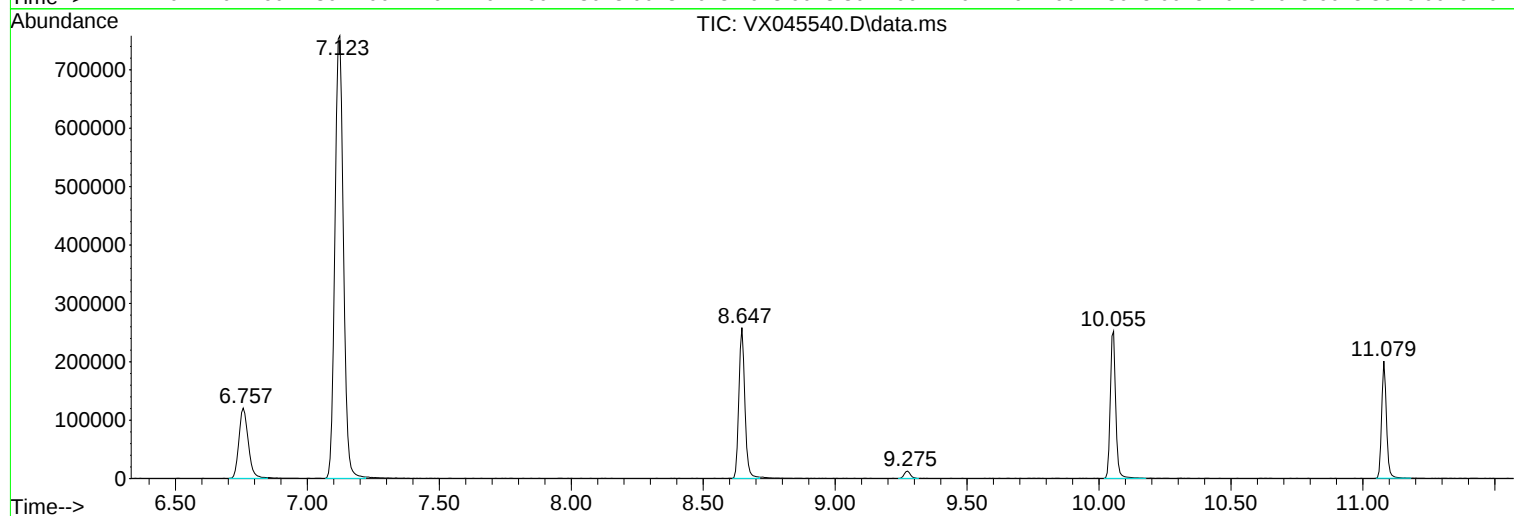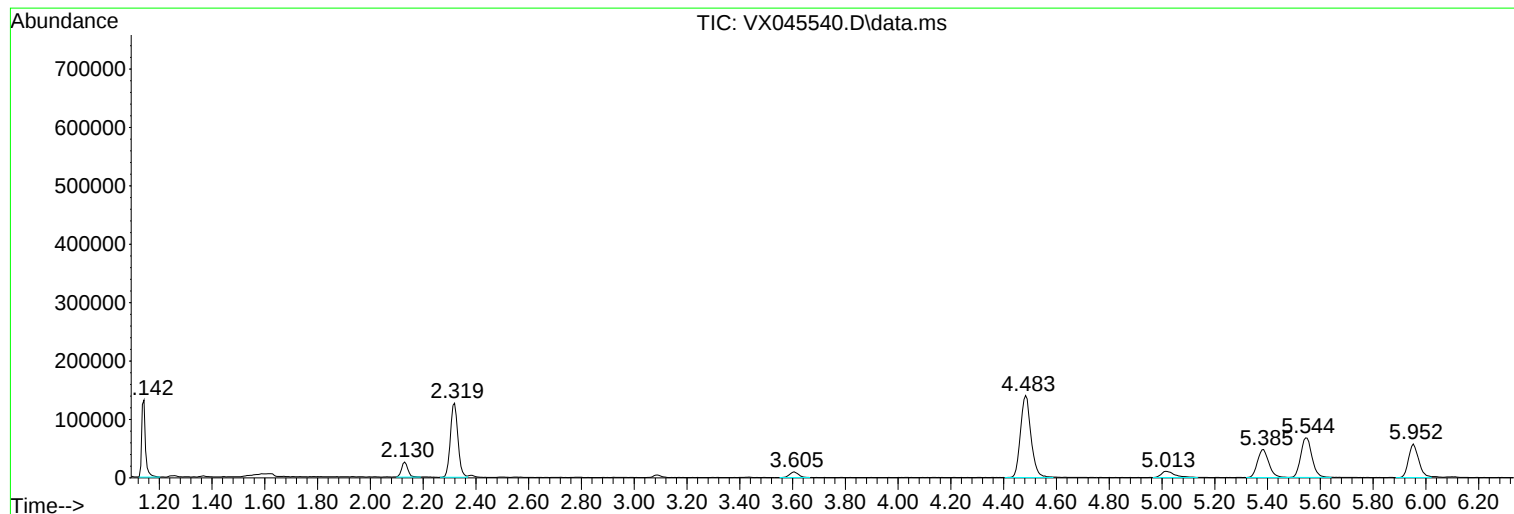

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\WX040225\
Data File : VX045540.D
Acq On : 02 Apr 2025 12:30
Operator : JC/MD
Sample : Q1697-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IW-01-55-040125










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X040225W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Ethene, chlorotrifluoro- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.142	32.68 ug/l	130042	Pentafluorobenzene	5.544

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Ethene, chlorotrifluoro-	116	C2ClF3	000079-38-9	97
2			5-Chloro-1-methylimidazole	116	C4H5ClN2	000872-49-1	9
3			3-Ethylthiolane	116	C6H12S	062184-67-2	9
4			1-Propene, 1-(ethylthio)-2-methyl-	116	C6H12S	027482-14-0	5
5			Indene	116	C9H8	000095-13-6	4

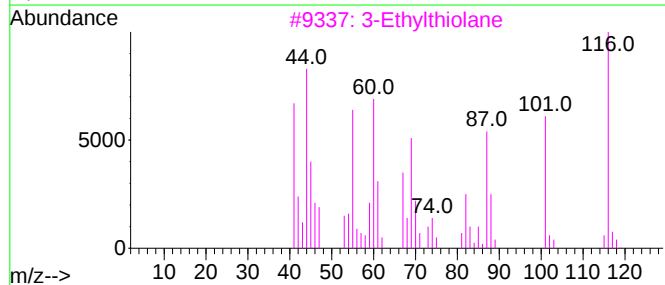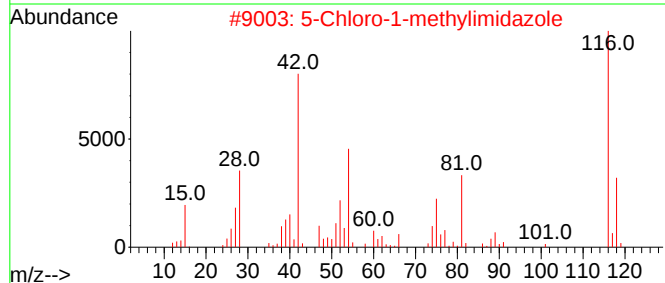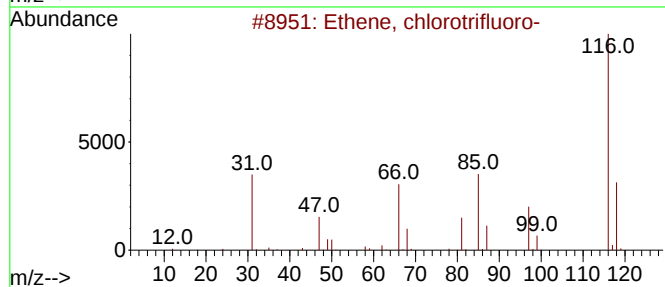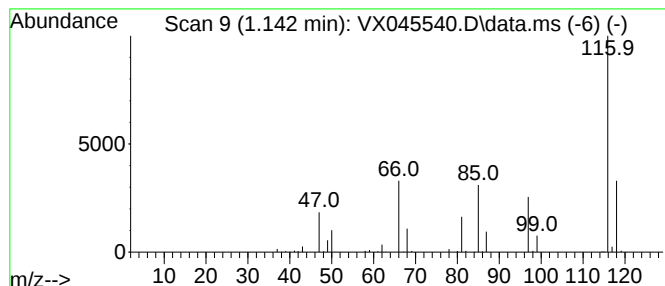

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX040225\
Data File : VX045540.D
Acq On : 02 Apr 2025 12:30
Operator : JC/MD
Sample : Q1697-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IW-01-55-040125










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X040225W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Ethane, 1,2-dichloro-1,1,2-... Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.130	10.65 ug/l	42376	Pentafluorobenzene	5.544

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Ethane, 1,2-dichloro-1,1,2-trifl...	152	C2HCl2F3	000354-23-4	95
2			Cyclopropane, 1,2-dimethyl-3-met...	82	C6H10	062338-02-7	12
3			Fluorodichloromethane	102	CHCl2F	000075-43-4	12
4			1-Butyne, 3,3-dimethyl-	82	C6H10	000917-92-0	10
5			2-Pentyn-4-one	82	C5H6O	007299-55-0	9

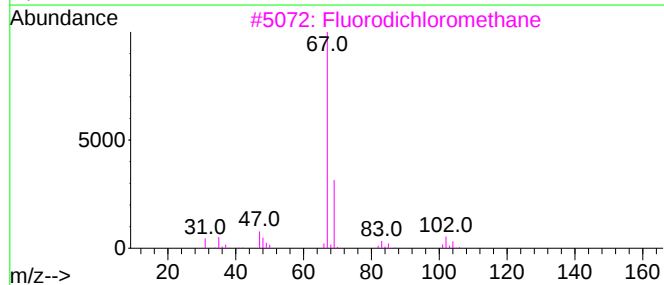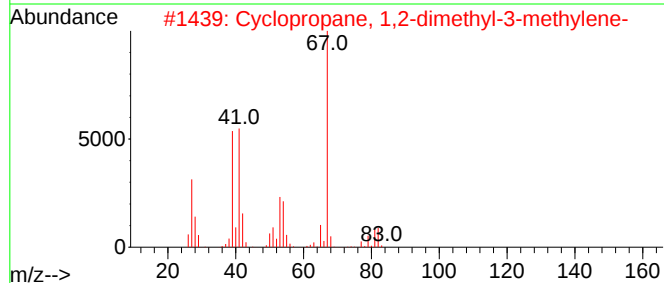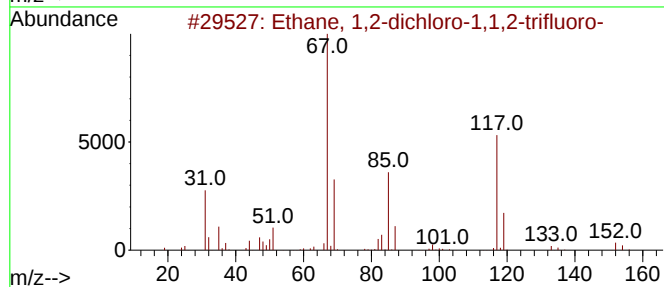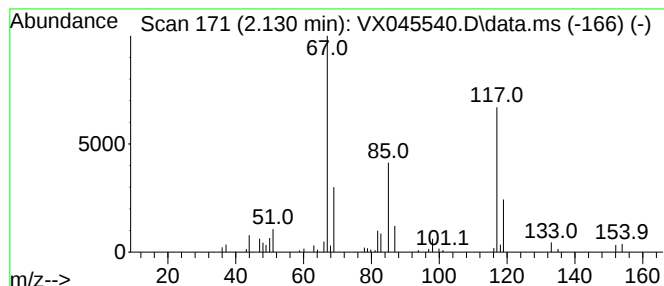

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX040225\
Data File : VX045540.D
Acq On : 02 Apr 2025 12:30
Operator : JC/MD
Sample : Q1697-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IW-01-55-040125

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X040225W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Ethene, chlorot...	1.142	32.7	ug/l	130042	1	5.544	198983	50.0
Ethane, 1,2-dic...	2.130	10.7	ug/l	42376	1	5.544	198983	50.0