


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_X\DATA\VX040319\
Data File : VX008604.D
Acq On : 03 Apr 2019 08:58
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X040319W.M
Title : SW846 8260
Last Update : Thu Apr 04 04:47:41 2019

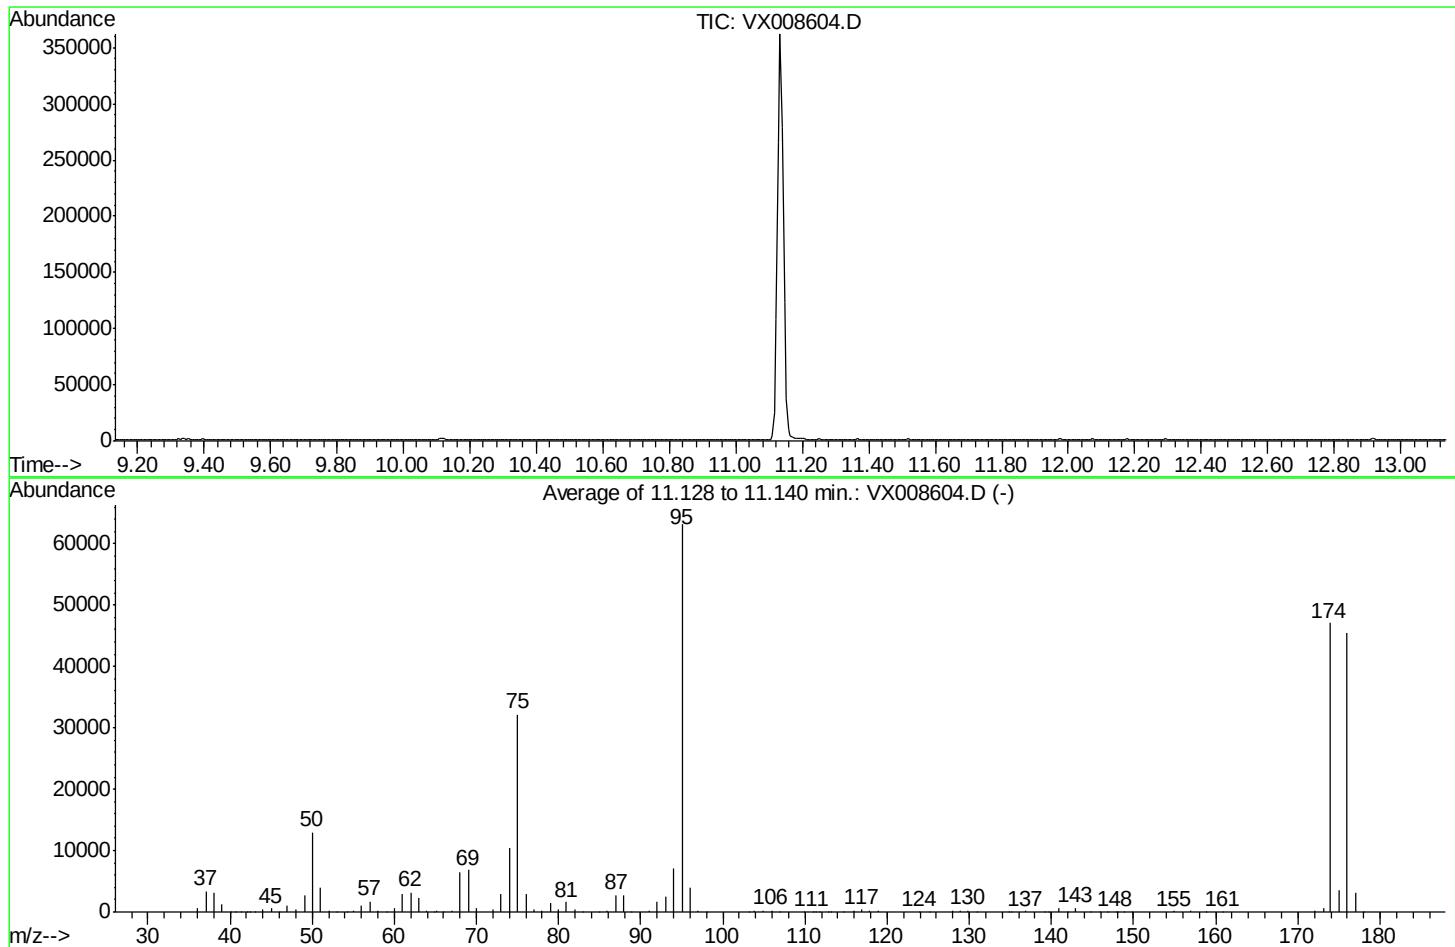

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1629

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.5	12950	PASS
75	95	30	60	50.9	32138	PASS
95	95	100	100	100.0	63168	PASS
96	95	5	9	6.4	4046	PASS
173	174	0.00	2	1.1	530	PASS
174	95	50	100	74.5	47045	PASS
175	174	5	9	7.6	3562	PASS
176	174	95	101	96.5	45421	PASS
177	176	5	9	6.9	3155	PASS