

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX040323\
 Data File : VX034929.D
 Acq On : 03 Apr 2023 14:01
 Operator : JC/MD
 Sample : 02163-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 FB

Quant Time: Apr 03 21:36:42 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032923W.M
 Quant Title : SW846 8260
 QLast Update : Sat Apr 01 01:50:18 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	272318	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	464773	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	413840	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	178782	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	205148	49.259	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	98.520%
35) Dibromofluoromethane	5.385	113	147736	48.058	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	96.120%
50) Toluene-d8	8.647	98	557139	49.101	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	98.200%
62) 4-Bromofluorobenzene	11.079	95	204594	46.595	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	93.200%


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX040323\
Data File : VX034929.D
Acq On : 03 Apr 2023 14:01
Operator : JC/MD
Sample : 02163-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FB

Quant Time: Apr 03 21:36:42 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032923W.M
Quant Title : SW846 8260
QLast Update : Sat Apr 01 01:50:18 2023
Response via : Initial Calibration




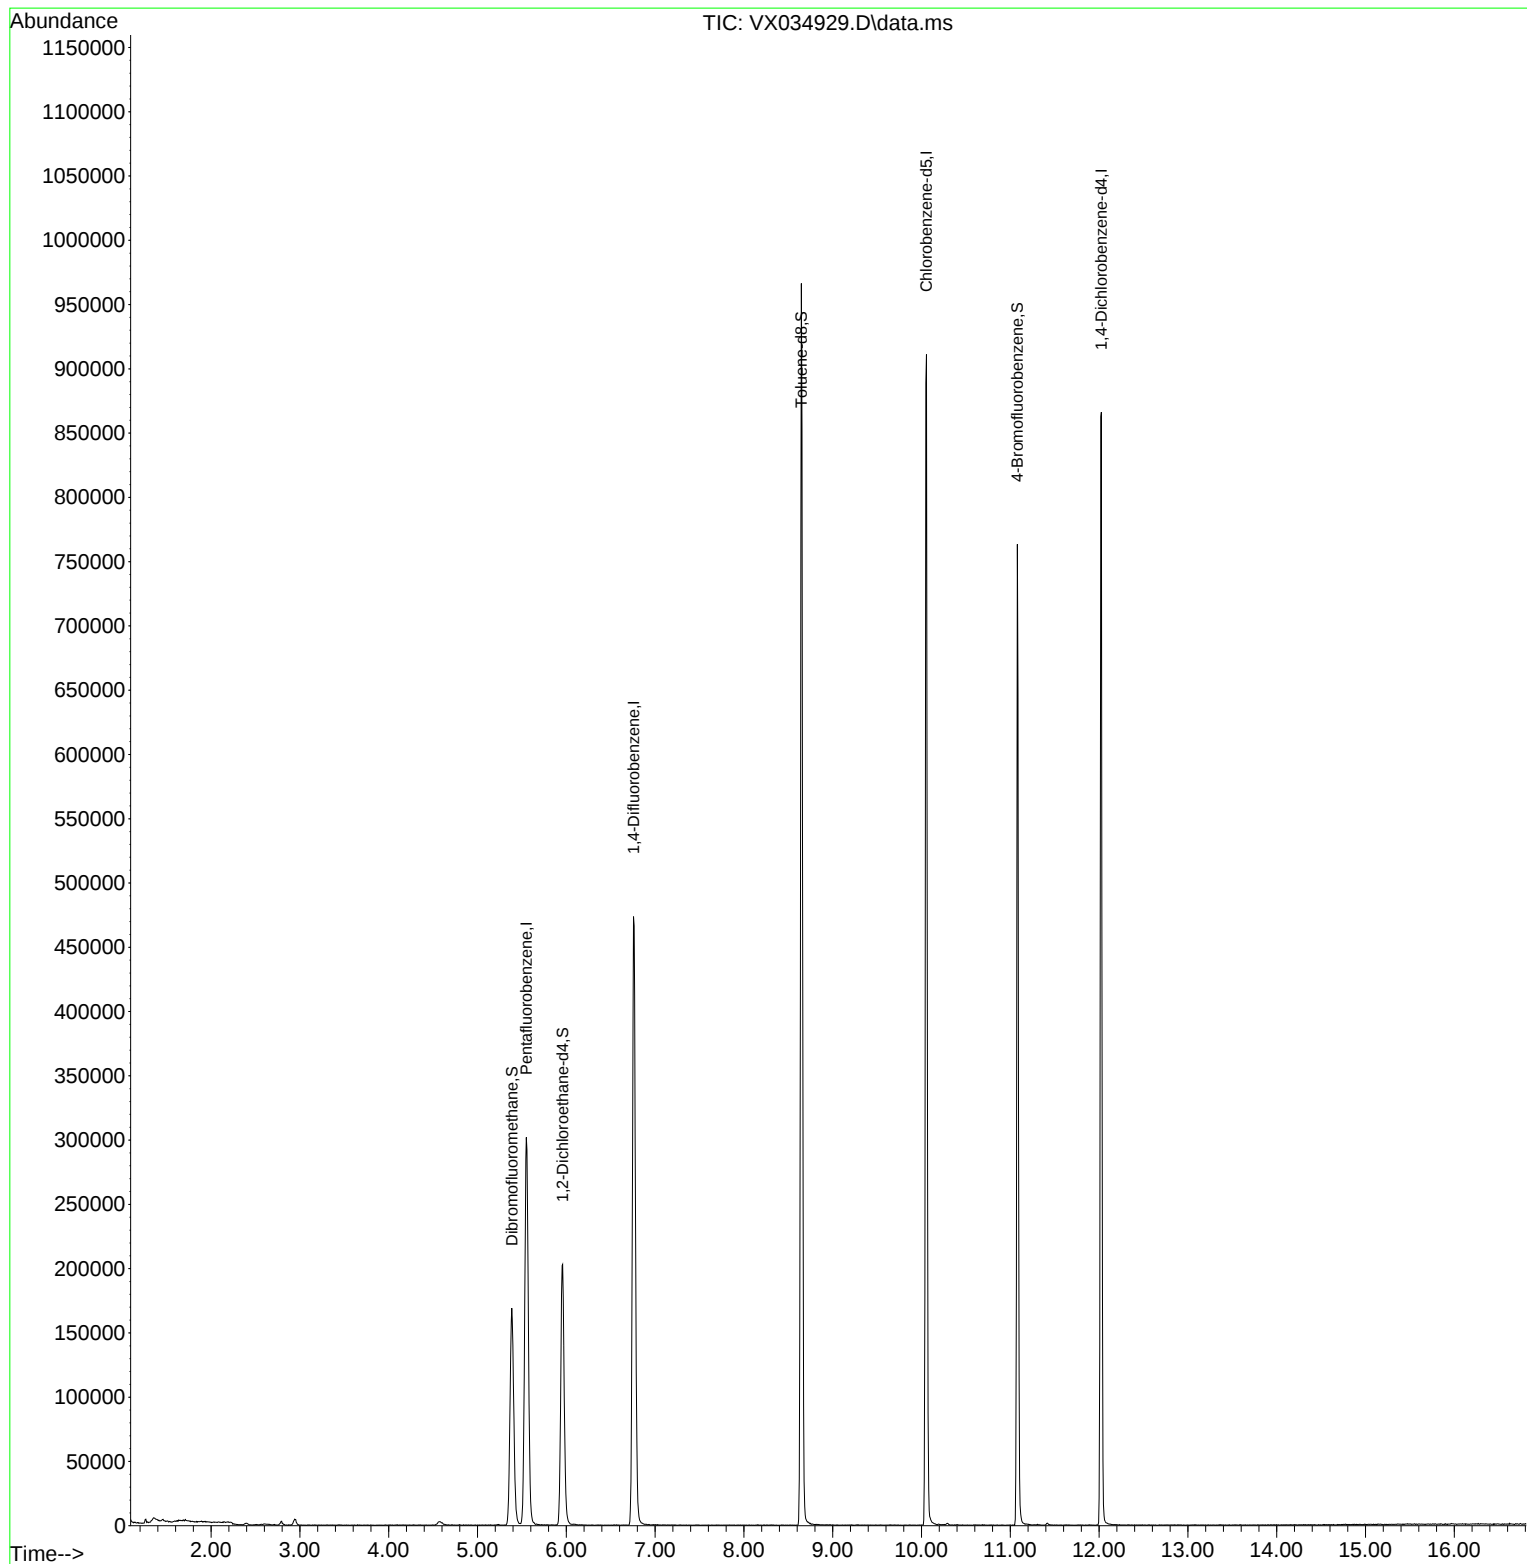




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX034929.D
Acq: 03 Apr 2023 14:01




Instrument :
MSVOA_X
ClientSampleId :
FB


Tgt Ion:168 Resp: 272318
Ion Ratio Lower Upper
168 100
99 65.5 45.7 68.5

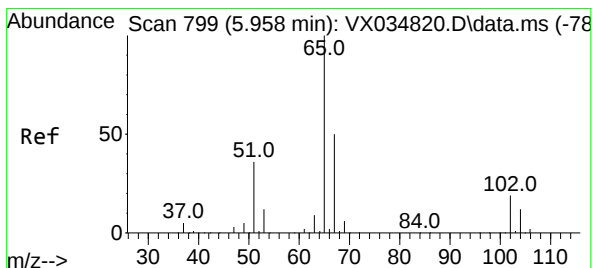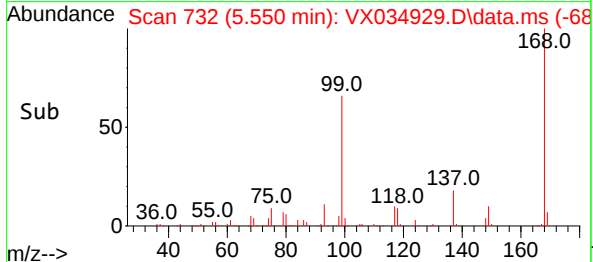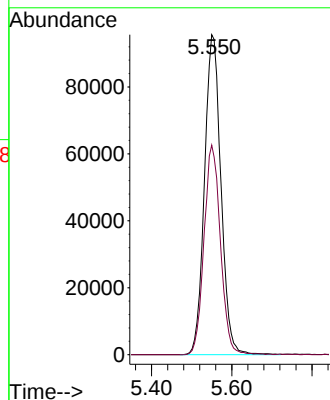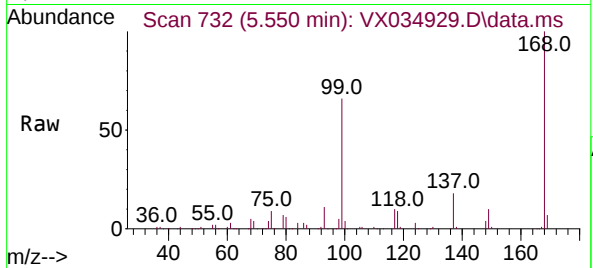

#33
1,2-Dichloroethane-d4
Concen: 49.259 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.000 min
Lab File: VX034929.D
Acq: 03 Apr 2023 14:01

Tgt Ion: 65 Resp: 205148
Ion Ratio Lower Upper
65 100
67 50.0 0.0 104.0

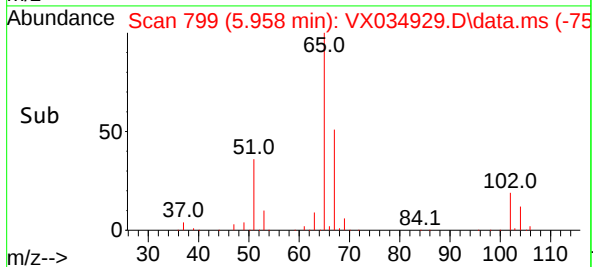
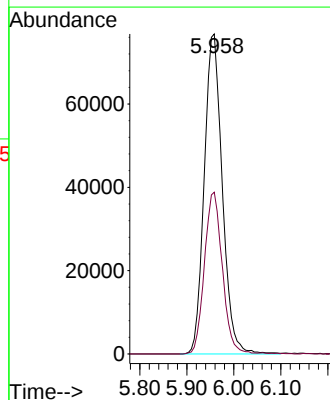
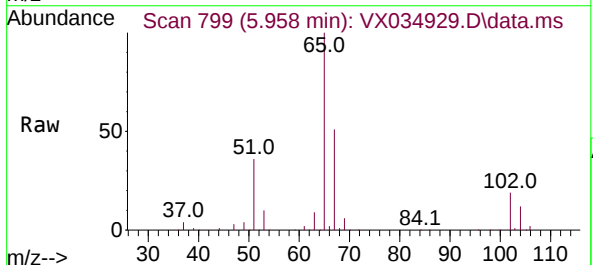


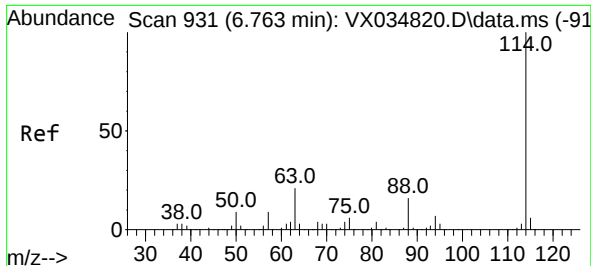

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.757 min Scan# 91
Delta R.T. -0.006 min
Lab File: VX034929.D
Acq: 03 Apr 2023 14:01




Instrument :
MSVOA_X
ClientSampleId :
FB

Tgt Ion:114 Resp: 464773
Ion Ratio Lower Upper
114 100
63 22.7 0.0 42.2
88 16.9 0.0 33.2

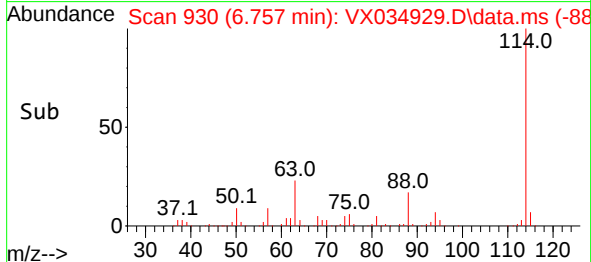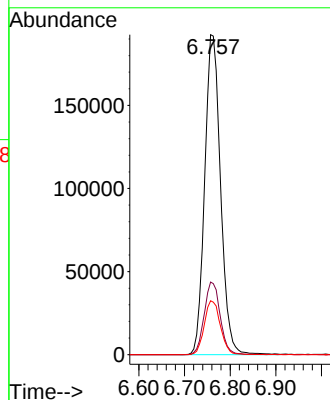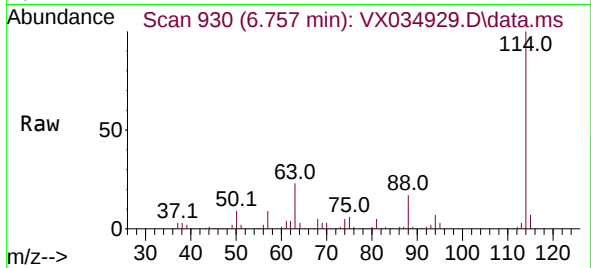

#35
Dibromofluoromethane
Concen: 48.058 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.000 min
Lab File: VX034929.D
Acq: 03 Apr 2023 14:01

Tgt Ion:113 Resp: 147736
Ion Ratio Lower Upper
113 100
111 102.5 83.7 125.5
192 17.8 15.4 23.2


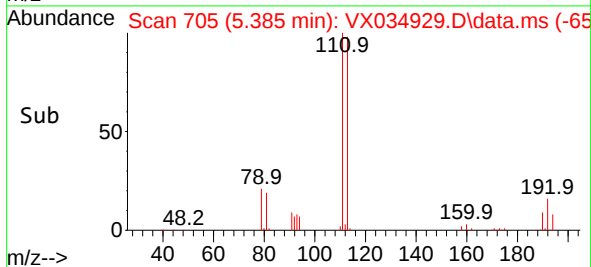
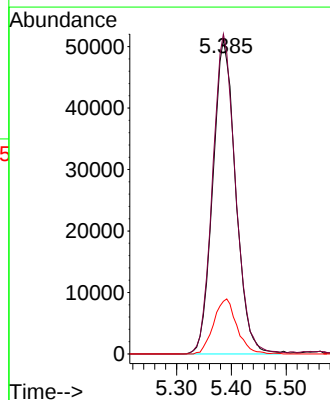
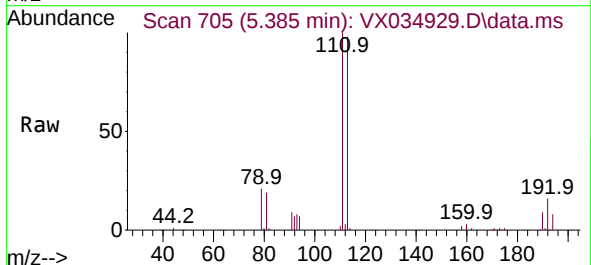




#50
Toluene-d8
Concen: 49.101 ug/l
RT: 8.647 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX034929.D
Acq: 03 Apr 2023 14:01




Instrument :
MSVOA_X
ClientSampleId :
FB


Tgt Ion: 98 Resp: 557139
Ion Ratio Lower Upper
98 100
100 66.3 52.5 78.7

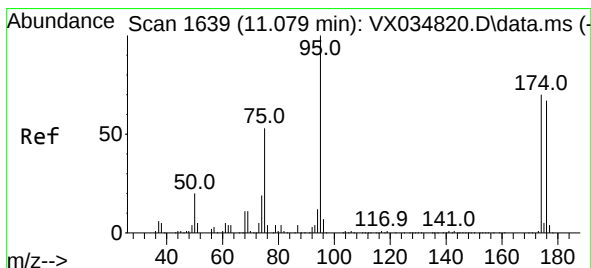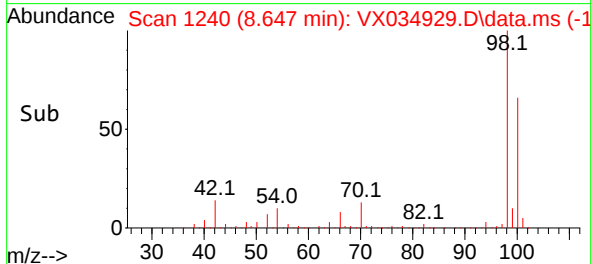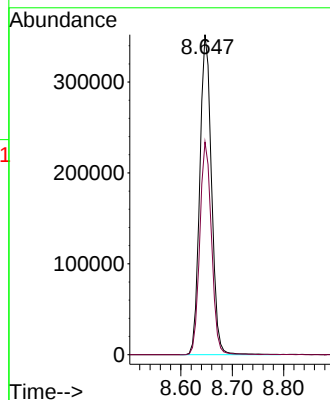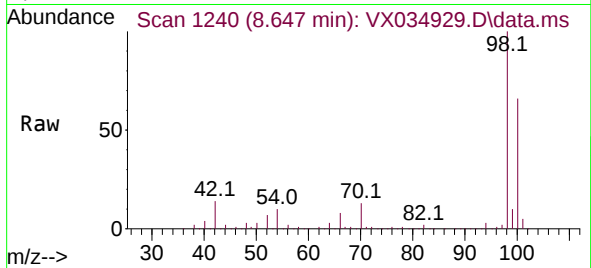

#62
4-Bromofluorobenzene
Concen: 46.595 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX034929.D
Acq: 03 Apr 2023 14:01

Tgt Ion: 95 Resp: 204594
Ion Ratio Lower Upper
95 100
174 70.1 0.0 147.4
176 68.9 0.0 140.6


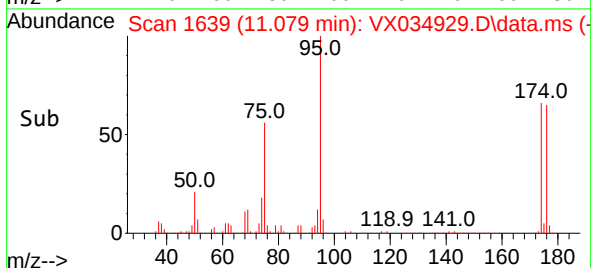
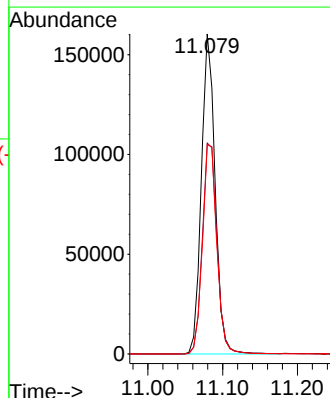
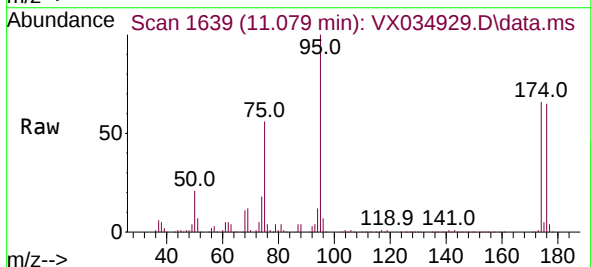


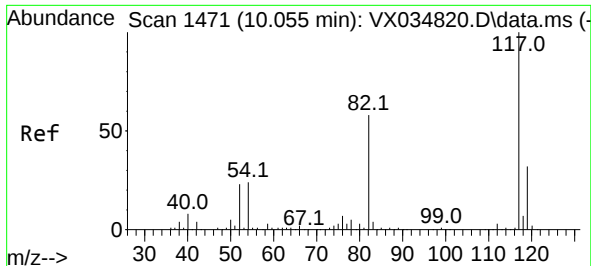

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX034929.D
Acq: 03 Apr 2023 14:01

Instrument :
MSVOA_X
ClientSampleId :
FB

Tgt Ion:117 Resp: 413840
Ion Ratio Lower Upper
117 100
82 58.7 45.0 67.4
119 32.2 26.0 39.0

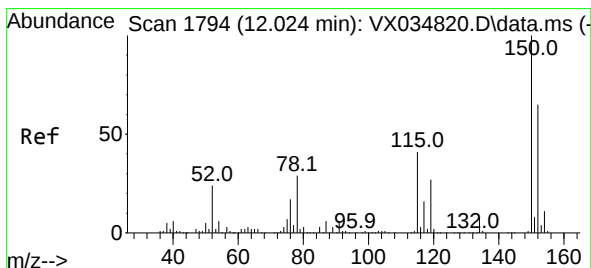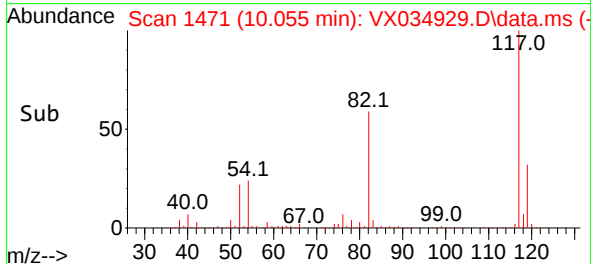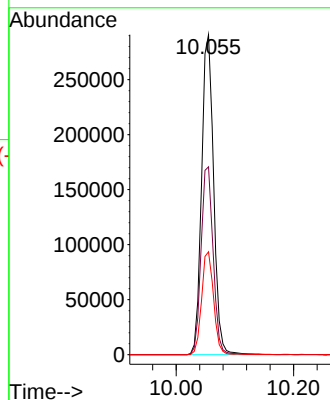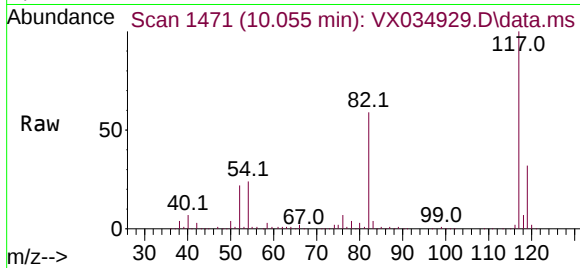

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX034929.D
Acq: 03 Apr 2023 14:01

Tgt Ion:152 Resp: 178782
Ion Ratio Lower Upper
152 100
115 62.8 45.0 135.0
150 155.6 0.0 352.4

